

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071620\
 Data File : BF120888.D
 Acq On : 16 Jul 2020 16:28
 Operator : JU/CG
 Sample : PB130244BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB130244BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	562	568	571	rBV	3476887	3531958	71.92%	11.773%
2	6.439	734	740	743	rBV	3217012	3545019	72.18%	11.816%
3	6.810	800	803	807	rBV	1162657	948754	19.32%	3.162%
4	7.375	894	899	902	rBV	2519745	2391031	48.69%	7.970%
5	8.092	1017	1021	1025	rBV	1378554	1264216	25.74%	4.214%
6	9.175	1200	1205	1208	rBV	4303763	4194213	85.40%	13.980%
7	9.845	1315	1319	1323	rBV	1600489	1466582	29.86%	4.889%
8	10.633	1448	1453	1457	rBV	2694904	2842695	57.88%	9.475%
9	11.333	1567	1572	1575	rBV	1857903	1600946	32.60%	5.336%
10	12.921	1837	1842	1845	rBV2	4363455	4911042	100.00%	16.370%
11	13.968	2015	2020	2023	rBV	1799381	1627515	33.14%	5.425%
12	15.415	2260	2266	2270	rBV	1241579	1491159	30.36%	4.970%
13	15.457	2270	2273	2282	rVB	45165	60222	1.23%	0.201%
14	15.886	2341	2346	2351	rVB	42012	61782	1.26%	0.206%
15	16.380	2423	2430	2438	rBV4	31644	63517	1.29%	0.212%


Sum of corrected areas: 30000651

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071620\
Data File : BF120888.D
Acq On : 16 Jul 2020 16:28
Operator : JU/CG
Sample : PB130244BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130244BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

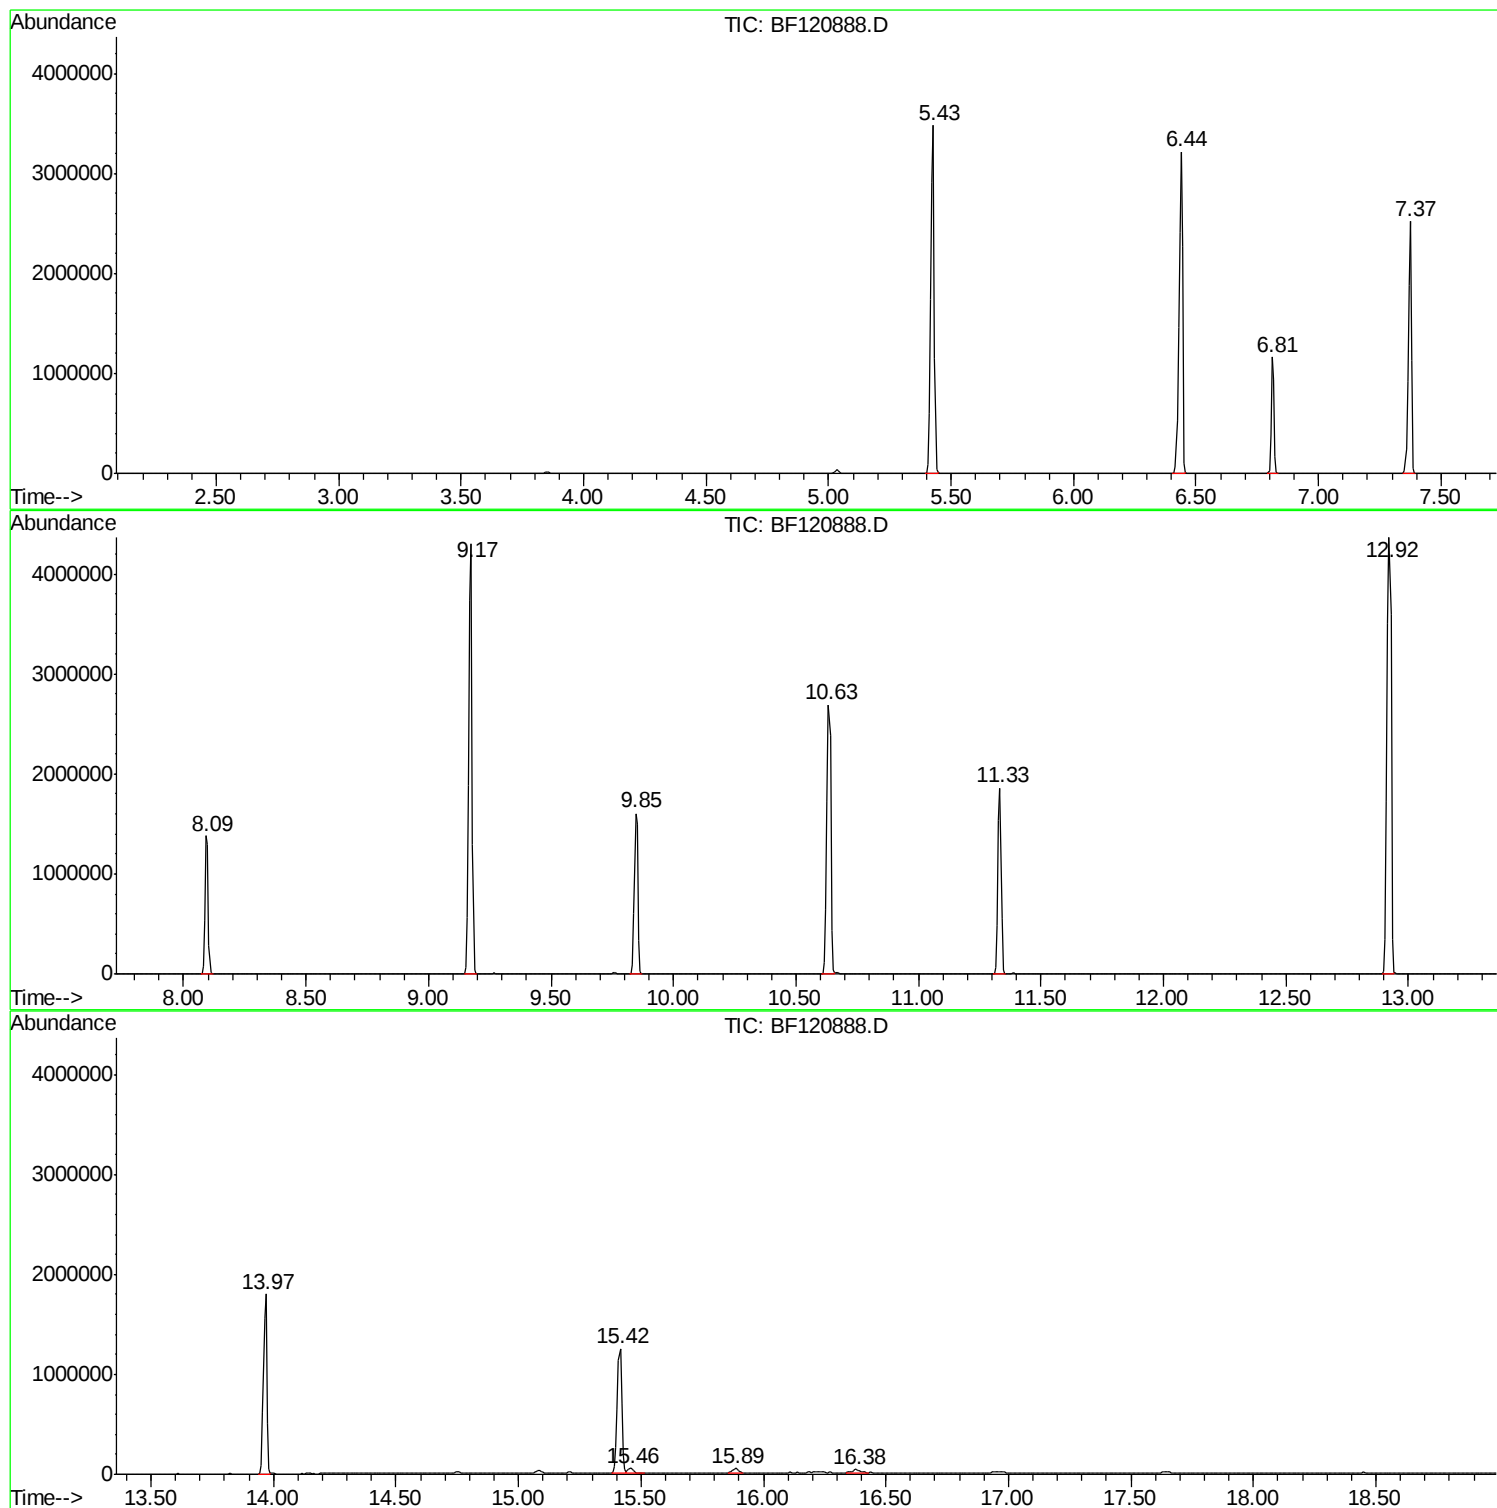

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071620\
Data File : BF120888.D
Acq On : 16 Jul 2020 16:28
Operator : JU/CG
Sample : PB130244BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130244BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071620\
Data File : BF120888.D
Acq On : 16 Jul 2020 16:28
Operator : JU/CG
Sample : PB130244BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130244BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc