


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071620\
 Data File : BF120876.D
 Acq On : 16 Jul 2020 9:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 16 14:20:32 2020

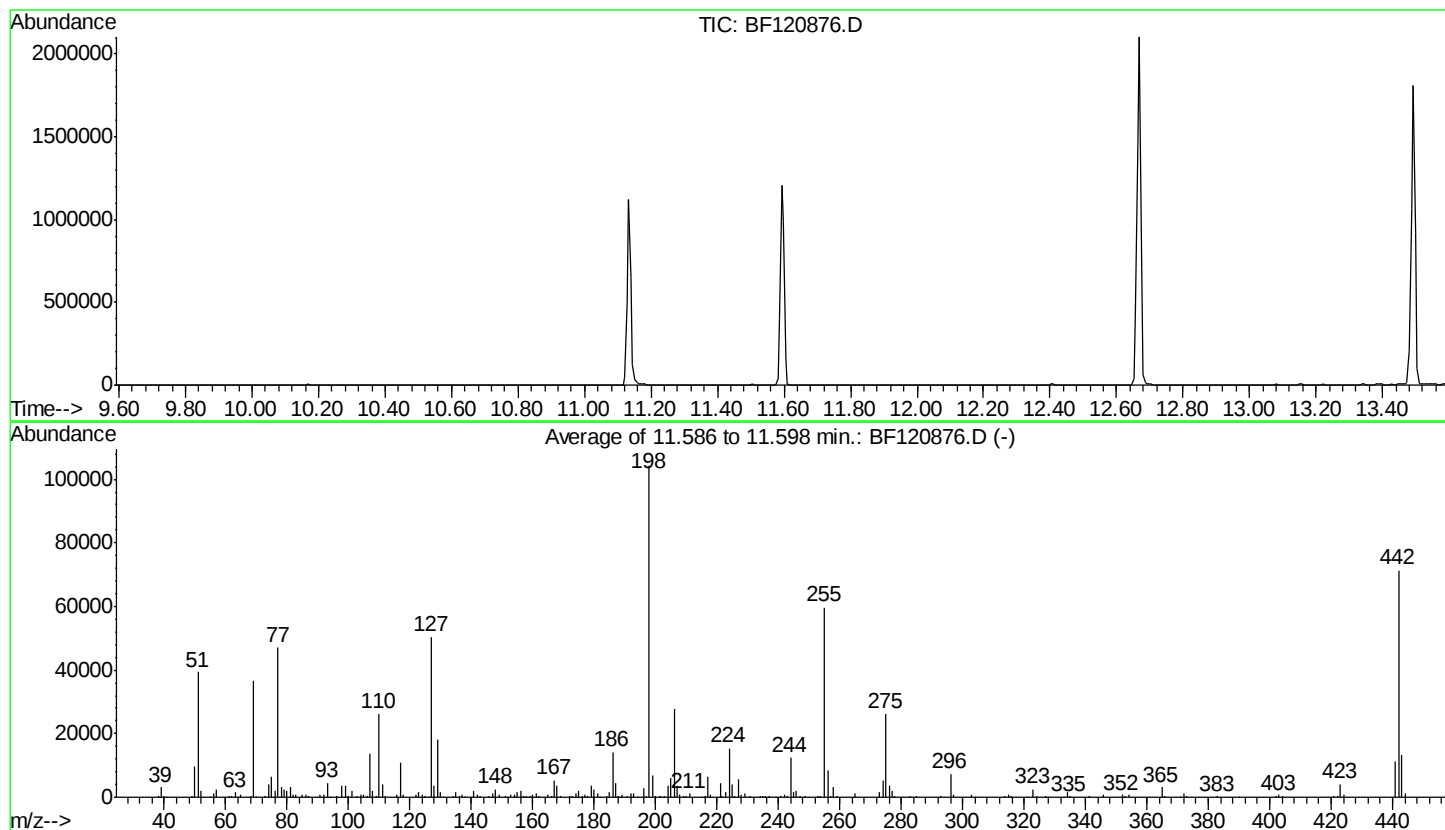

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	39301	PASS
68	69	0.00	2	1.6	573	PASS
69	198	0.00	100	35.2	36706	PASS
70	69	0.00	2	0.3	118	PASS
127	198	10	80	48.4	50490	PASS
197	198	0.00	2	0.6	590	PASS
198	198	100	100	100.0	104261	PASS
199	198	5	9	6.7	7019	PASS
275	198	10	60	25.3	26344	PASS
365	198	1	100	3.0	3159	PASS
441	198	0.01	100	10.8	11254	PASS
442	198	50	100	68.3	71243	PASS
443	442	15	24	18.9	13431	PASS