

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF071621\  
 Data File : BF124589.D  
 Acq On : 16 Jul 2021 10:11  
 Operator : JU/CG  
 Sample : PB137634BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB137634BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF070721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124589.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.545       | 583           | 588         | 591          | rBB      | 141488         | 129391        | 43.66%          | 8.431%        |
| 2         | 6.540       | 752           | 757         | 760          | rBB      | 131140         | 130442        | 44.01%          | 8.500%        |
| 3         | 6.922       | 819           | 822         | 825          | rBB      | 49914          | 36686         | 12.38%          | 2.390%        |
| 4         | 7.081       | 845           | 849         | 852          | rBB      | 207327         | 180468        | 60.89%          | 11.759%       |
| 5         | 7.487       | 913           | 918         | 920          | rBB      | 138415         | 137398        | 46.36%          | 8.953%        |
| 6         | 8.204       | 1036          | 1040        | 1043         | rBB      | 59830          | 50847         | 17.16%          | 3.313%        |
| 7         | 9.286       | 1218          | 1224        | 1227         | rBB      | 282224         | 275583        | 92.99%          | 17.957%       |
| 8         | 9.963       | 1335          | 1339        | 1342         | rBB      | 74405          | 60890         | 20.55%          | 3.968%        |
| 9         | 10.751      | 1469          | 1473        | 1476         | rBB      | 128243         | 103999        | 35.09%          | 6.777%        |
| 10        | 11.451      | 1588          | 1592        | 1595         | rBV      | 82643          | 63342         | 21.37%          | 4.127%        |
| 11        | 13.045      | 1858          | 1863        | 1866         | rBV      | 326427         | 296365        | 100.00%         | 19.311%       |
| 12        | 14.092      | 2038          | 2041        | 2044         | rBV      | 51508          | 41452         | 13.99%          | 2.701%        |
| 13        | 15.586      | 2291          | 2295        | 2300         | rBB2     | 23340          | 27805         | 9.38%           | 1.812%        |




Sum of corrected areas: 1534668

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF071621\  
Data File : BF124589.D  
Acq On : 16 Jul 2021 10:11  
Operator : JU/CG  
Sample : PB137634BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB137634BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF070721.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

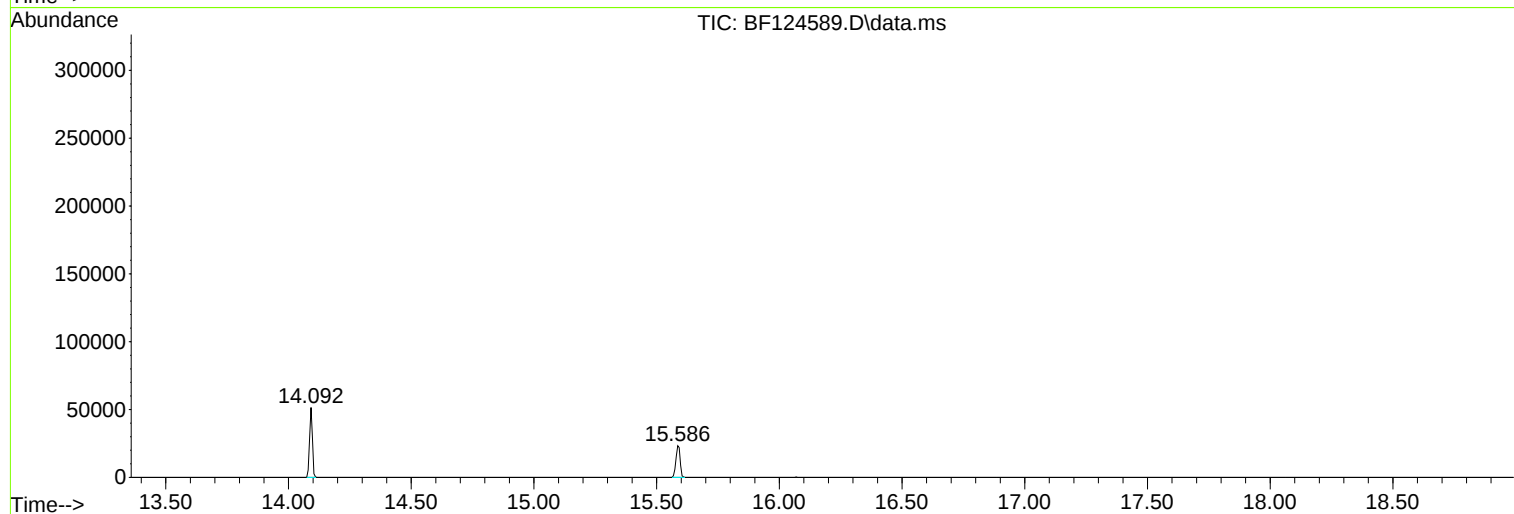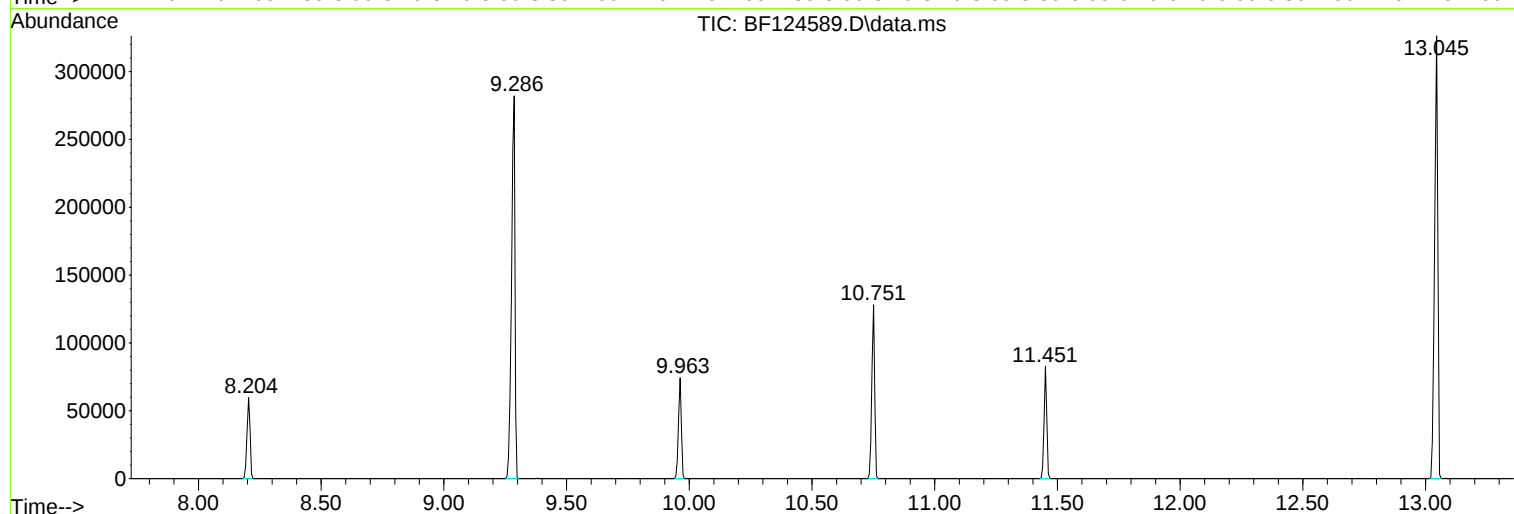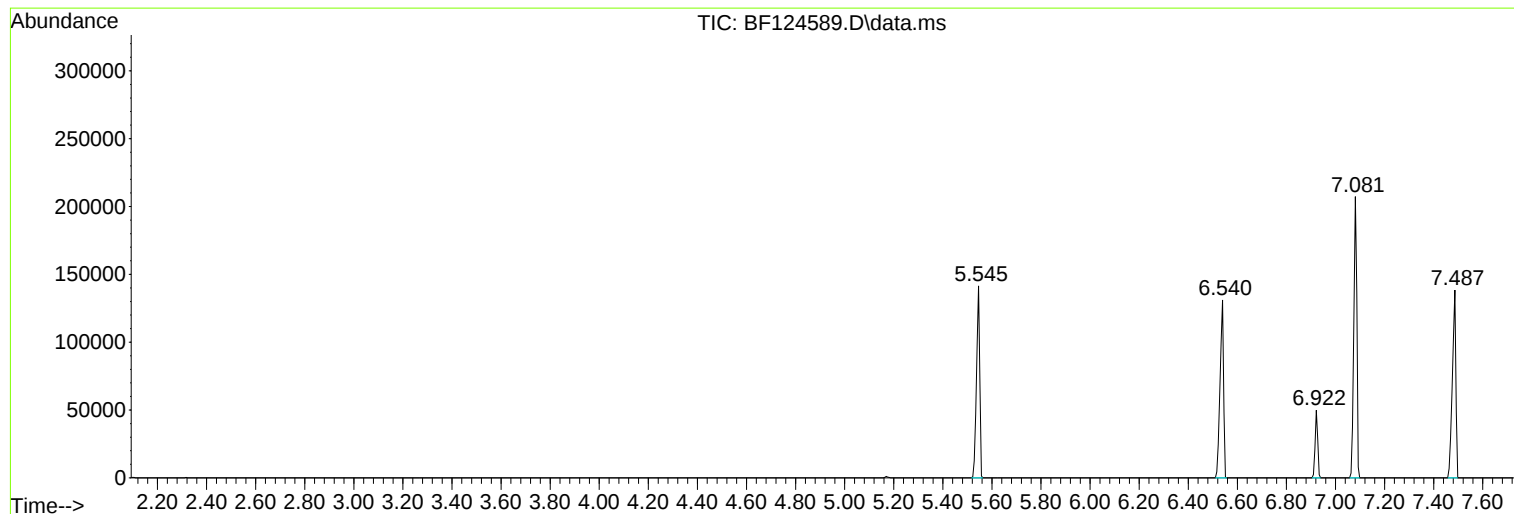

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF071621\  
Data File : BF124589.D  
Acq On : 16 Jul 2021 10:11  
Operator : JU/CG  
Sample : PB137634BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB137634BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF070721.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF071621\  
Data File : BF124589.D  
Acq On : 16 Jul 2021 10:11  
Operator : JU/CG  
Sample : PB137634BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB137634BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF070721.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|