

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071621\
 Data File : BF124593.D
 Acq On : 16 Jul 2021 13:09
 Operator : JU/CG
 Sample : PB137695BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137695BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124593.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.181	523	526	530	rBB	2830	3096	1.13%	0.212%
2	5.551	584	589	592	rBB	188668	185899	67.55%	12.742%
3	6.545	752	758	760	rBB	168273	189899	69.01%	13.016%
4	6.922	819	822	825	rBB	48306	36022	13.09%	2.469%
5	7.486	912	918	920	rBB	113194	124708	45.32%	8.548%
6	8.204	1036	1040	1043	rBB	56337	48521	17.63%	3.326%
7	9.286	1218	1224	1227	rBB	241383	255330	92.78%	17.501%
8	9.963	1335	1339	1342	rBB	73290	58967	21.43%	4.042%
9	10.751	1469	1473	1476	rBV	156473	153998	55.96%	10.555%
10	11.451	1588	1592	1595	rBV	78479	60043	21.82%	4.115%
11	13.045	1858	1863	1866	rBV	302189	275195	100.00%	18.862%
12	14.092	2038	2041	2044	rBB	53565	41011	14.90%	2.811%
13	15.586	2291	2295	2300	rBB	21979	26273	9.55%	1.801%




Sum of corrected areas: 1458962

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071621\
Data File : BF124593.D
Acq On : 16 Jul 2021 13:09
Operator : JU/CG
Sample : PB137695BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137695BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

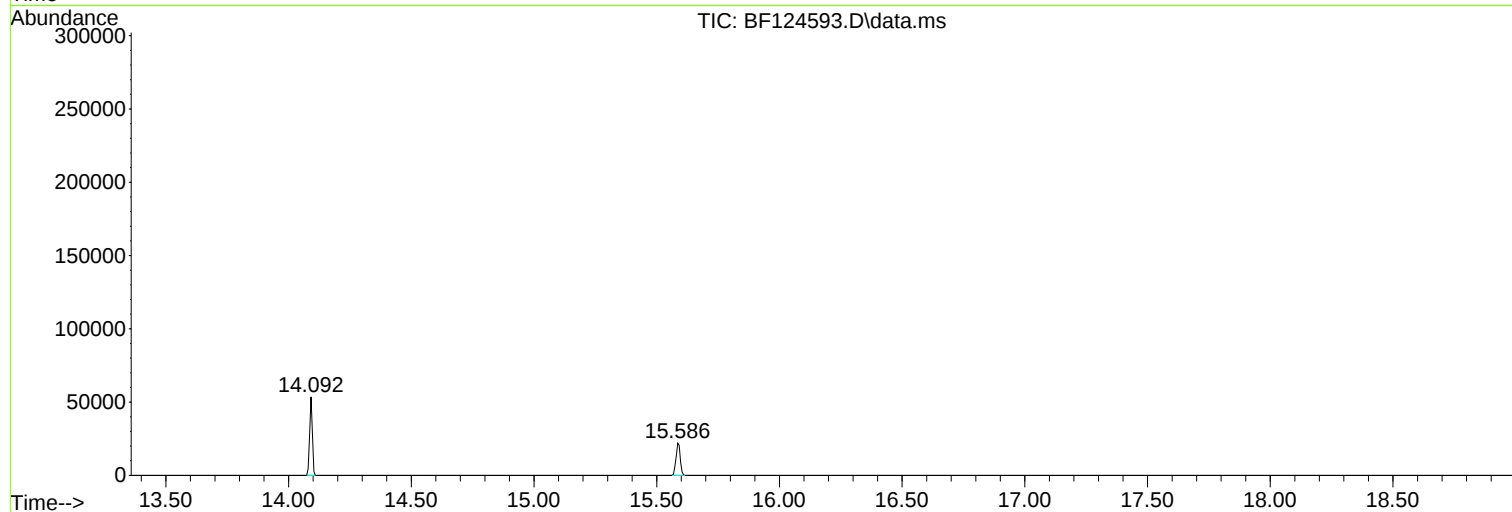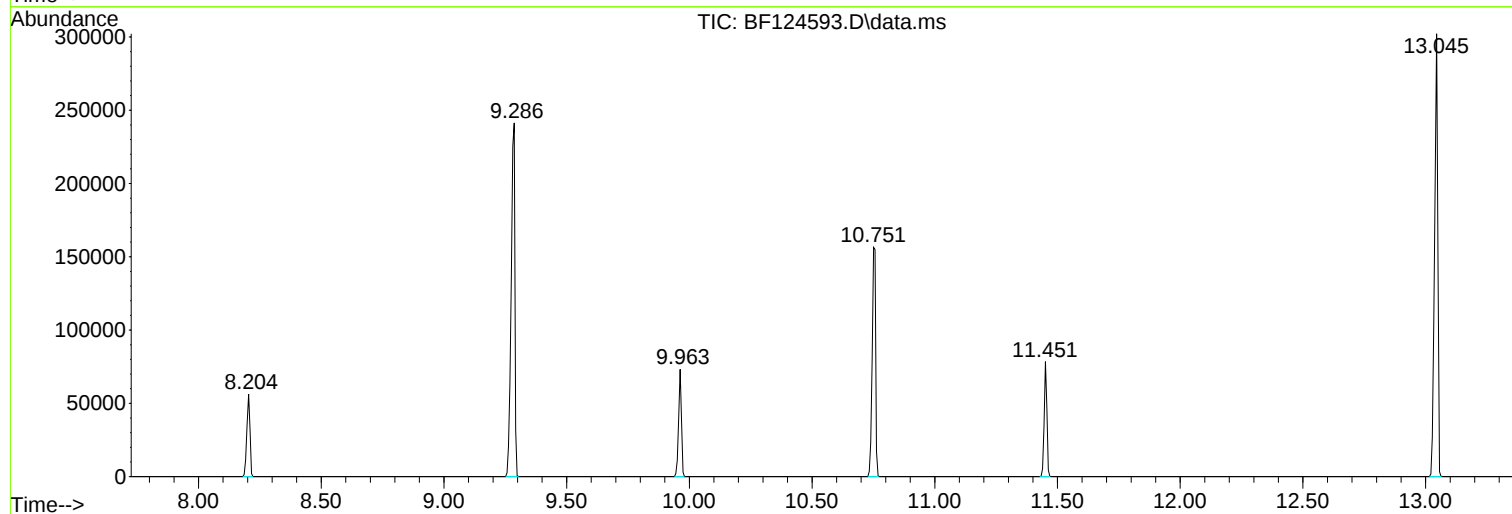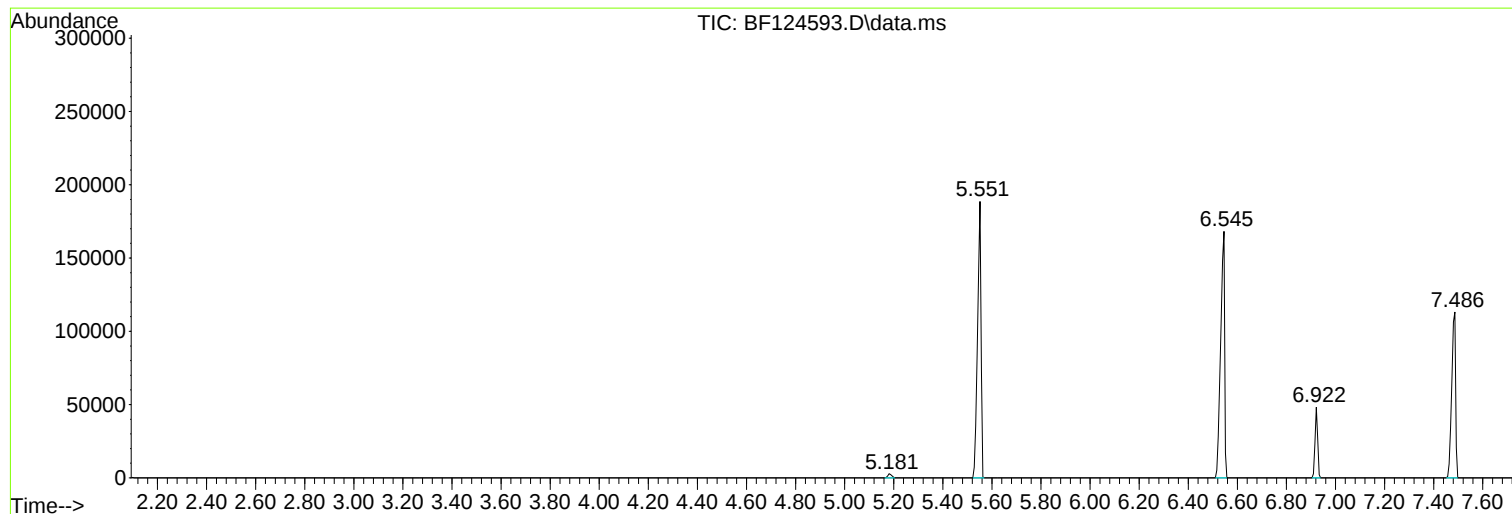

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071621\
Data File : BF124593.D
Acq On : 16 Jul 2021 13:09
Operator : JU/CG
Sample : PB137695BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137695BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071621\
Data File : BF124593.D
Acq On : 16 Jul 2021 13:09
Operator : JU/CG
Sample : PB137695BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137695BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------