

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071621\
 Data File : BF124596.D
 Acq On : 16 Jul 2021 14:55
 Operator : JU/CG
 Sample : PB137738BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137738BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124596.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.545	583	588	591	rBB	142840	130395	43.02%	8.424%
2	6.539	752	757	760	rBB	131716	132127	43.59%	8.536%
3	6.922	819	822	825	rBB	48761	37461	12.36%	2.420%
4	7.081	845	849	852	rBB	208119	178657	58.94%	11.541%
5	7.486	912	918	920	rBB	135905	137259	45.28%	8.867%
6	8.204	1036	1040	1043	rBB	57227	51039	16.84%	3.297%
7	9.286	1218	1224	1227	rBB	290164	281044	92.72%	18.156%
8	9.963	1335	1339	1342	rBB	77501	60507	19.96%	3.909%
9	10.751	1469	1473	1476	rBB	127818	104474	34.47%	6.749%
10	11.451	1589	1592	1596	rBB	82326	63820	21.06%	4.123%
11	13.045	1858	1863	1866	rBV	308790	303107	100.00%	19.581%
12	14.092	2038	2041	2044	rBV	53184	40978	13.52%	2.647%
13	15.586	2291	2295	2300	rBB	23353	27086	8.94%	1.750%




Sum of corrected areas: 1547954

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071621\
Data File : BF124596.D
Acq On : 16 Jul 2021 14:55
Operator : JU/CG
Sample : PB137738BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137738BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

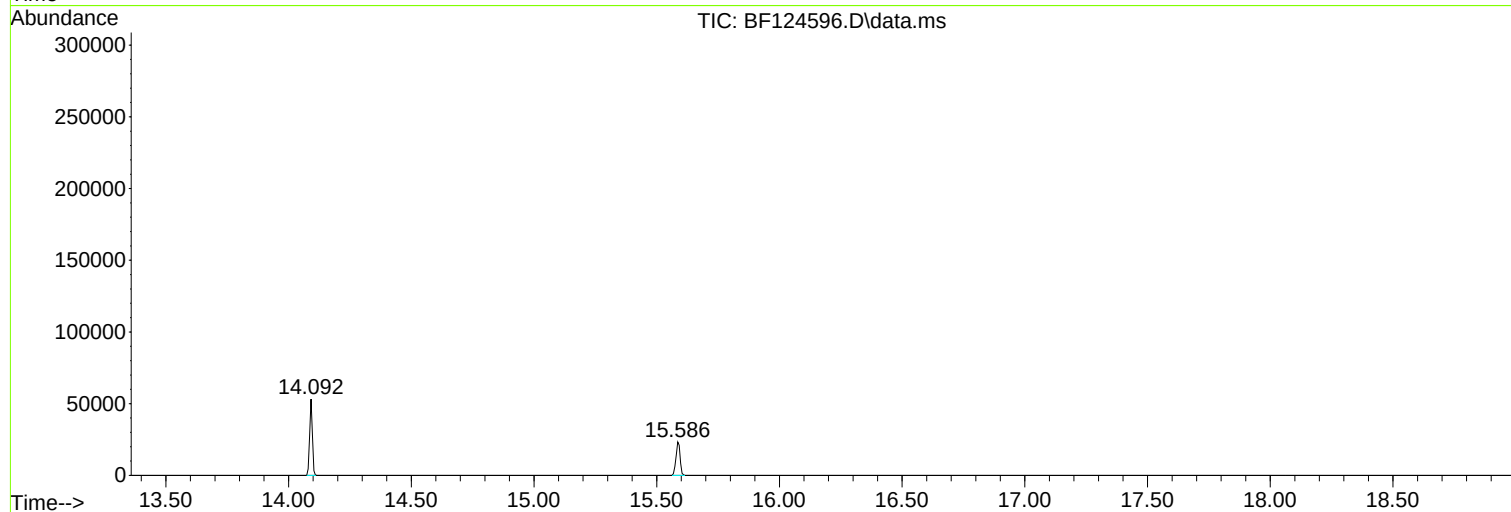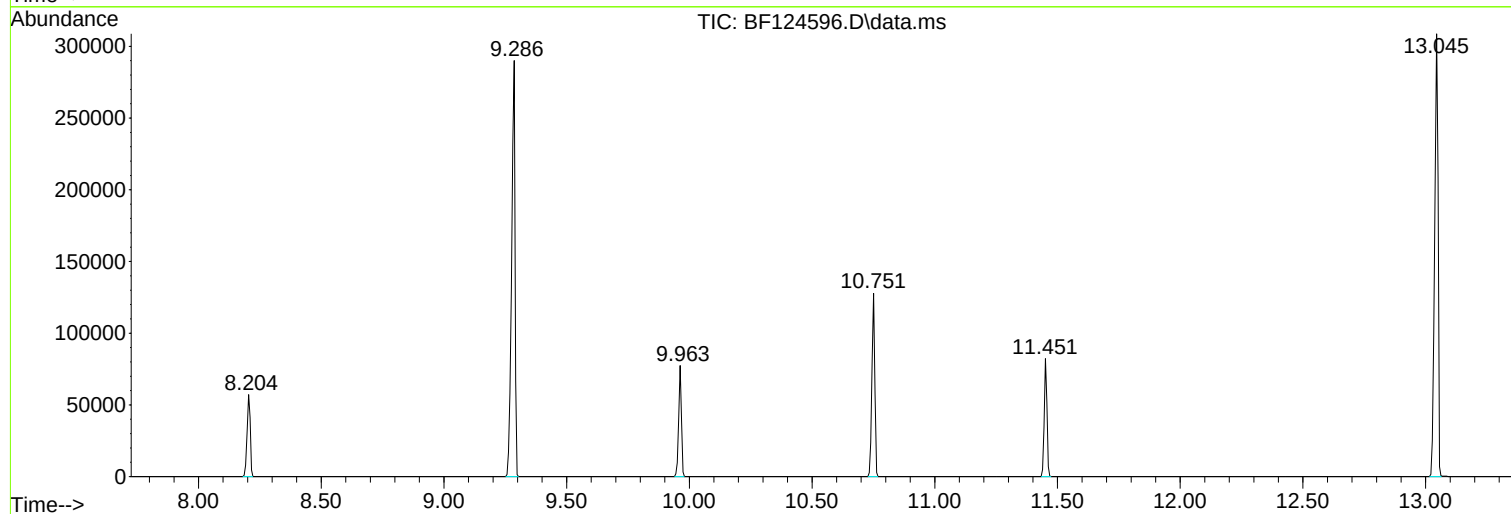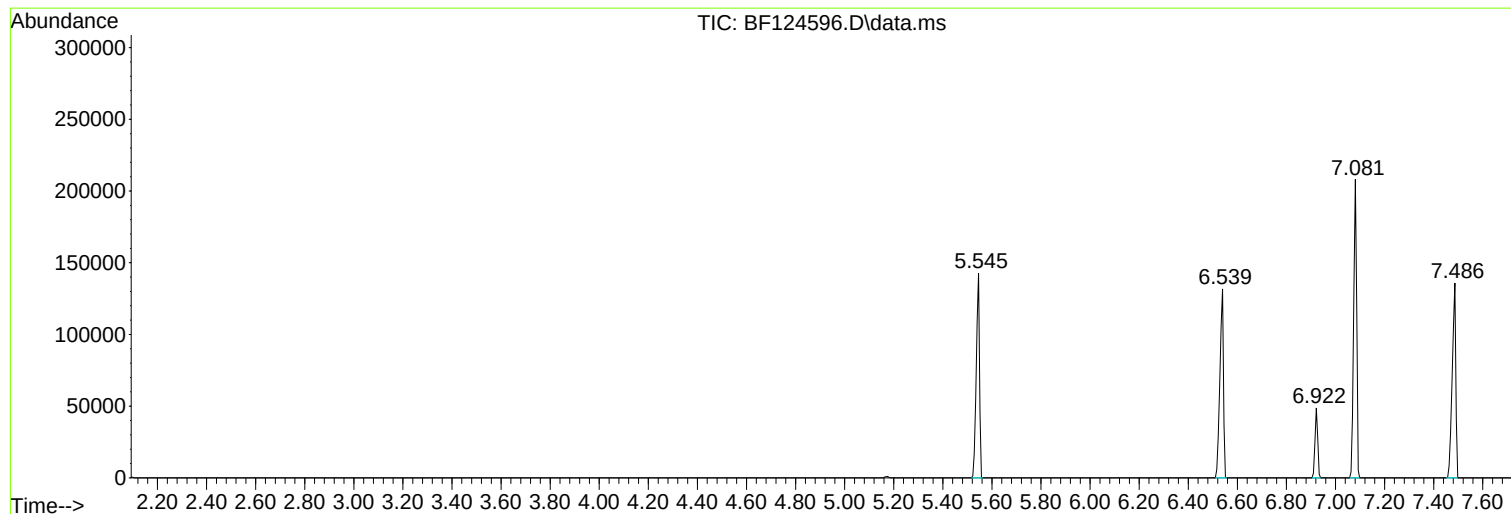

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071621\
Data File : BF124596.D
Acq On : 16 Jul 2021 14:55
Operator : JU/CG
Sample : PB137738BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137738BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071621\
Data File : BF124596.D
Acq On : 16 Jul 2021 14:55
Operator : JU/CG
Sample : PB137738BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137738BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------