
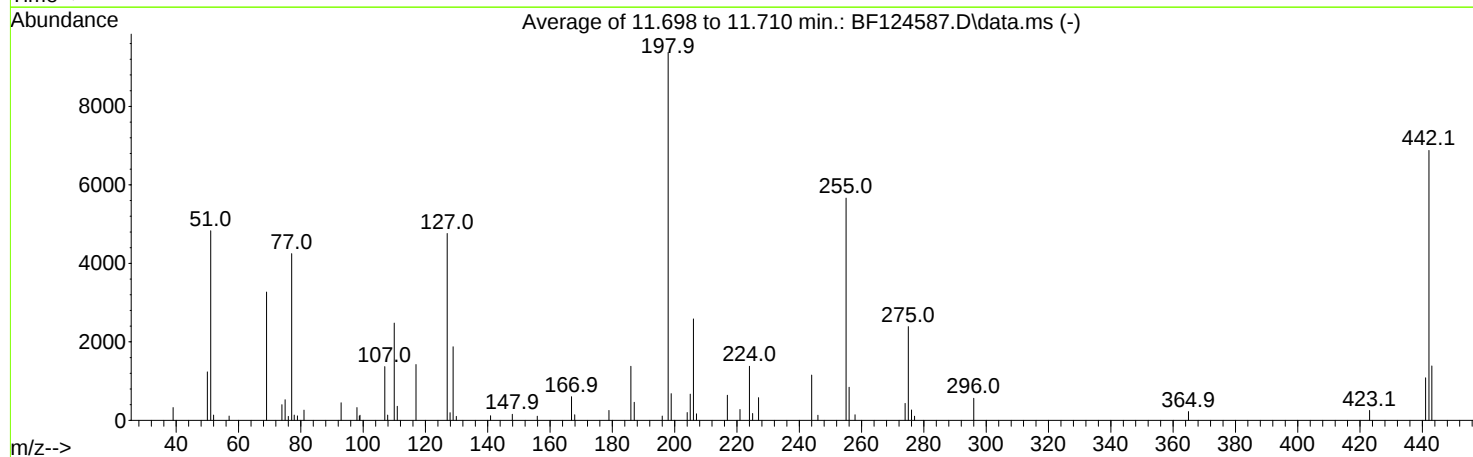


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071621\
 Data File : BF124587.D
 Acq On : 16 Jul 2021 9:05
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 08 07:49:42 2021

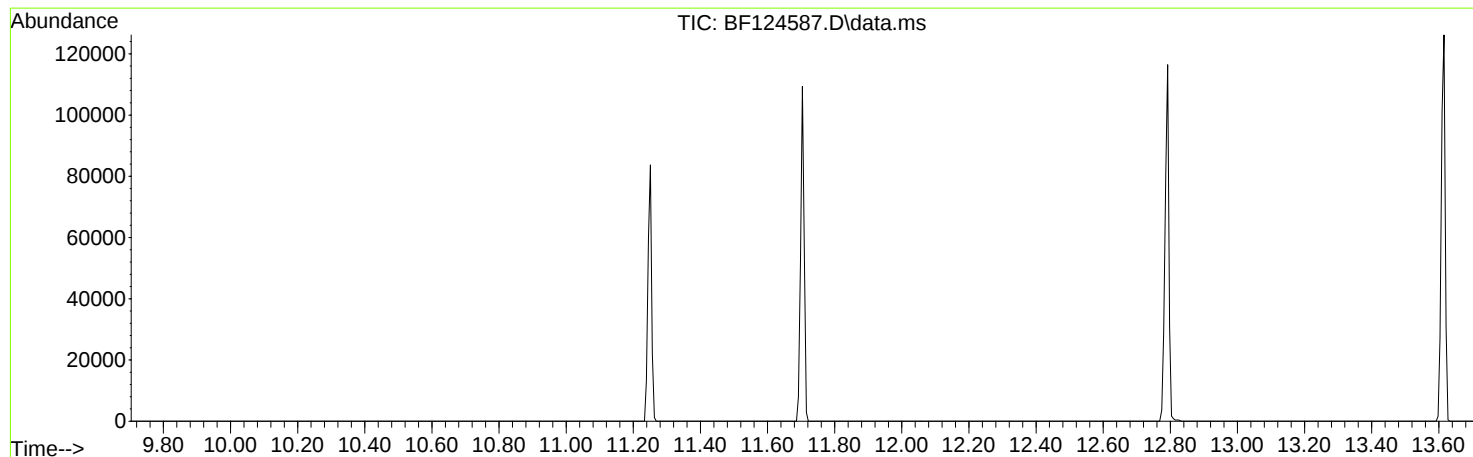

AutoFind: Scans 1634, 1635, 1636; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.6	4832	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.9	3271	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.8	4760	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	9372	PASS
199	198	5	9	7.3	681	PASS
275	198	10	60	25.5	2389	PASS
365	198	1	100	2.4	225	PASS
441	198	0.01	100	11.6	1083	PASS
442	442	50	100	100.0	6878	PASS
443	442	15	24	20.2	1388	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/16/2021	BNA_F	<u>BF124587.D</u>
Compound Name	Response	Retention Time
DDT	20861	13.61
DDD	0	13.3
DDE	0	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
0	20861	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071621\
Data File : BF124587.D
Acq On : 16 Jul 2021 9:05
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 16 12:04:43 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 08 07:49:42 2021
Response via : Initial Calibration

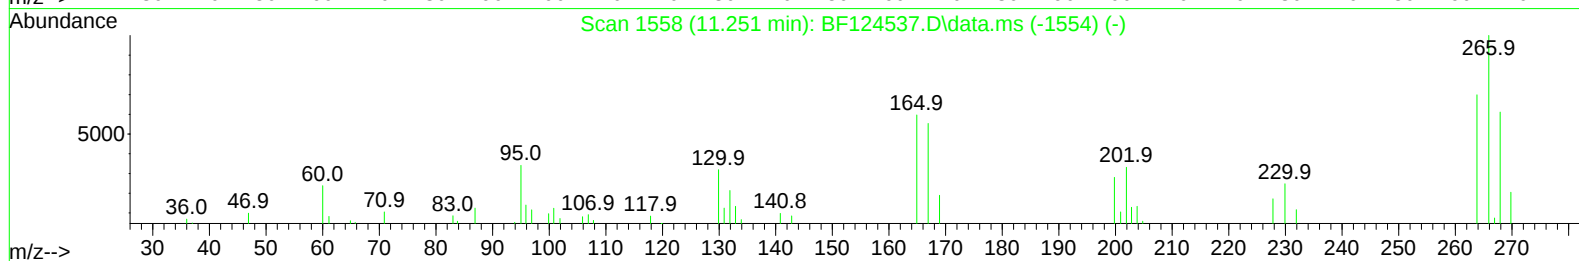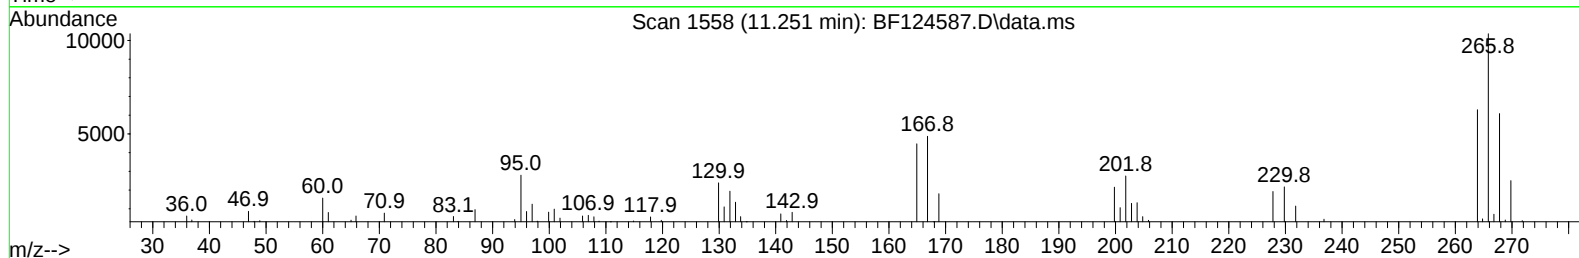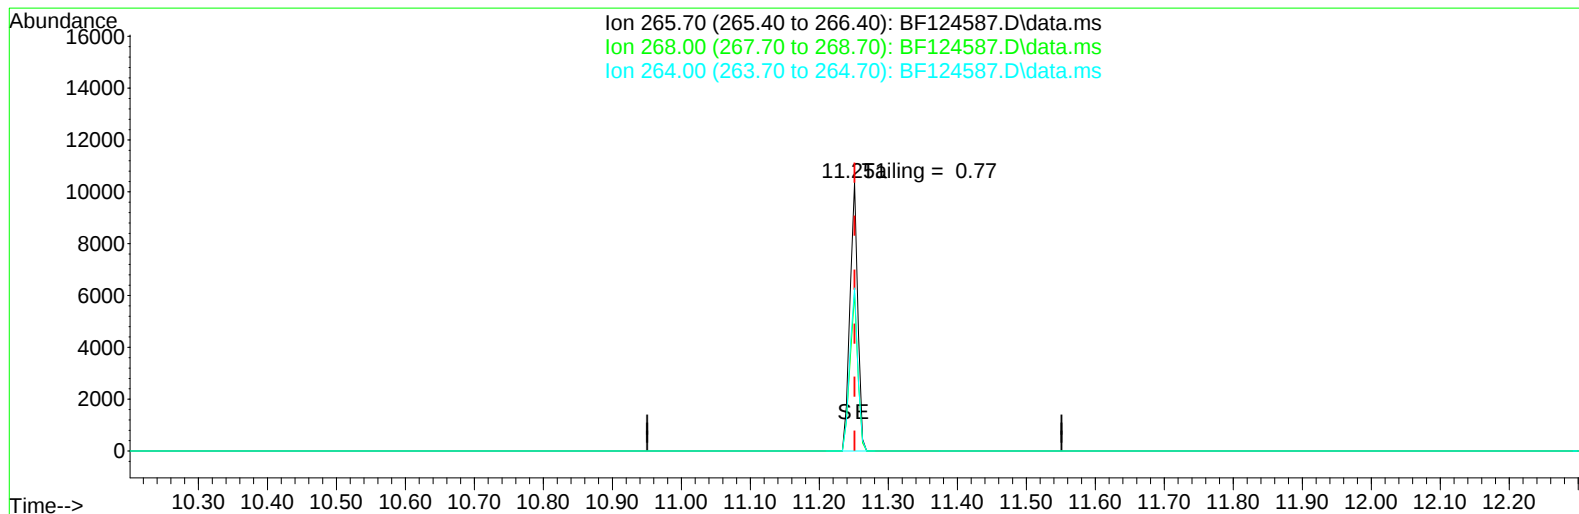

TIC: BF124587.D\data.ms

(70) Pentachlorophenol (C)

11.251min (+ 0.000) 0.00 ng




response 8273

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	58.79
264.00	69.90	60.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071621\
Data File : BF124587.D
Acq On : 16 Jul 2021 9:05
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 16 12:04:43 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 08 07:49:42 2021
Response via : Initial Calibration

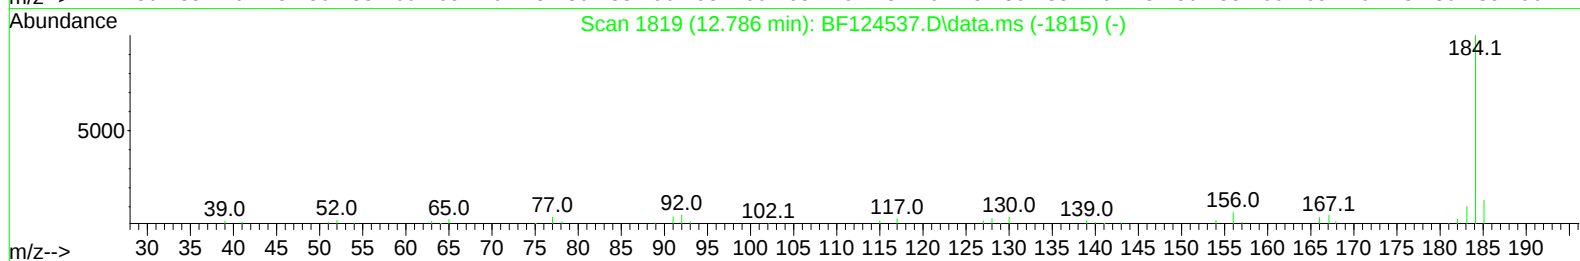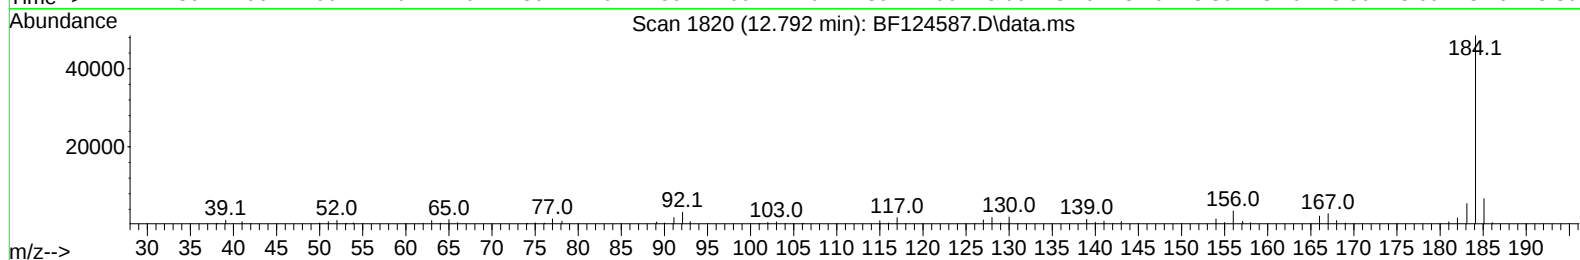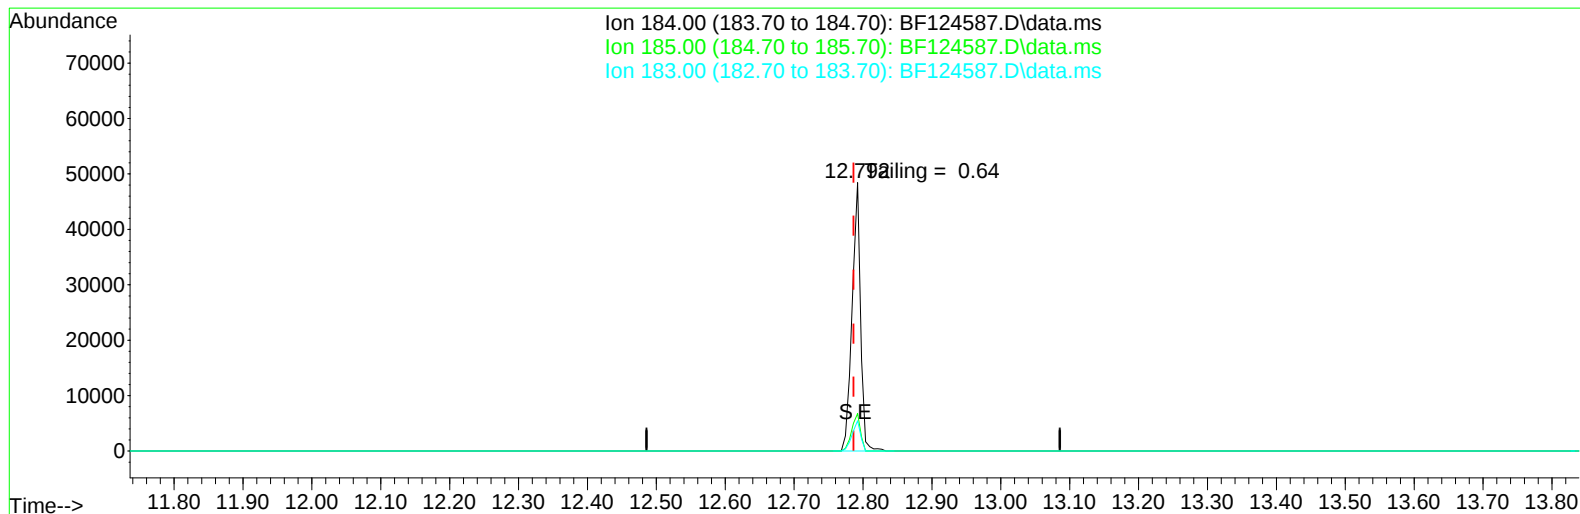

TIC: BF124587.D\data.ms

(77) Benzidine

12.792min (+ 0.006) 0.00 ng

response 41171

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.95
183.00	10.10	11.31
0.00	0.00	0.00