
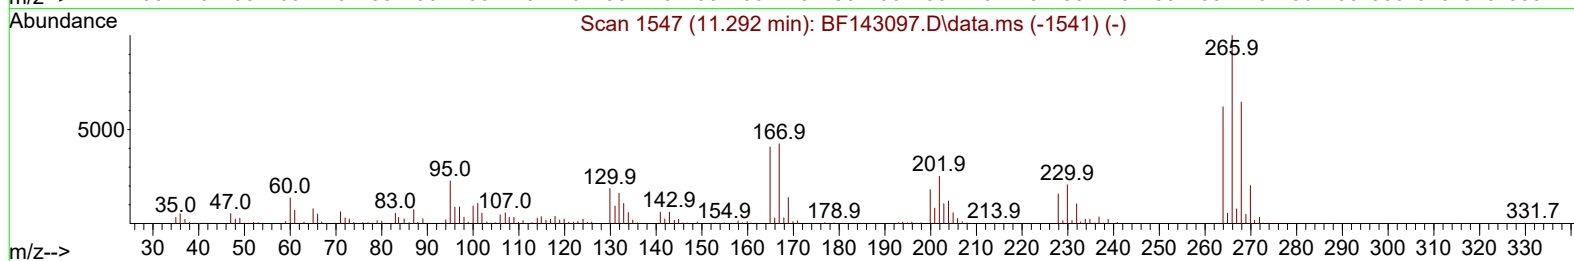
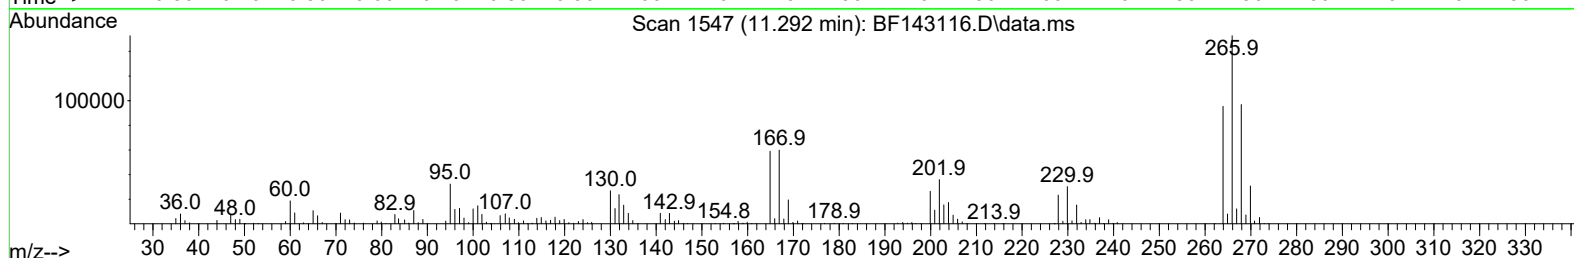


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143116.D
Acq On : 16 Jul 2025 19:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 17 03:11:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 15 17:53:25 2025
Response via : Initial Calibration

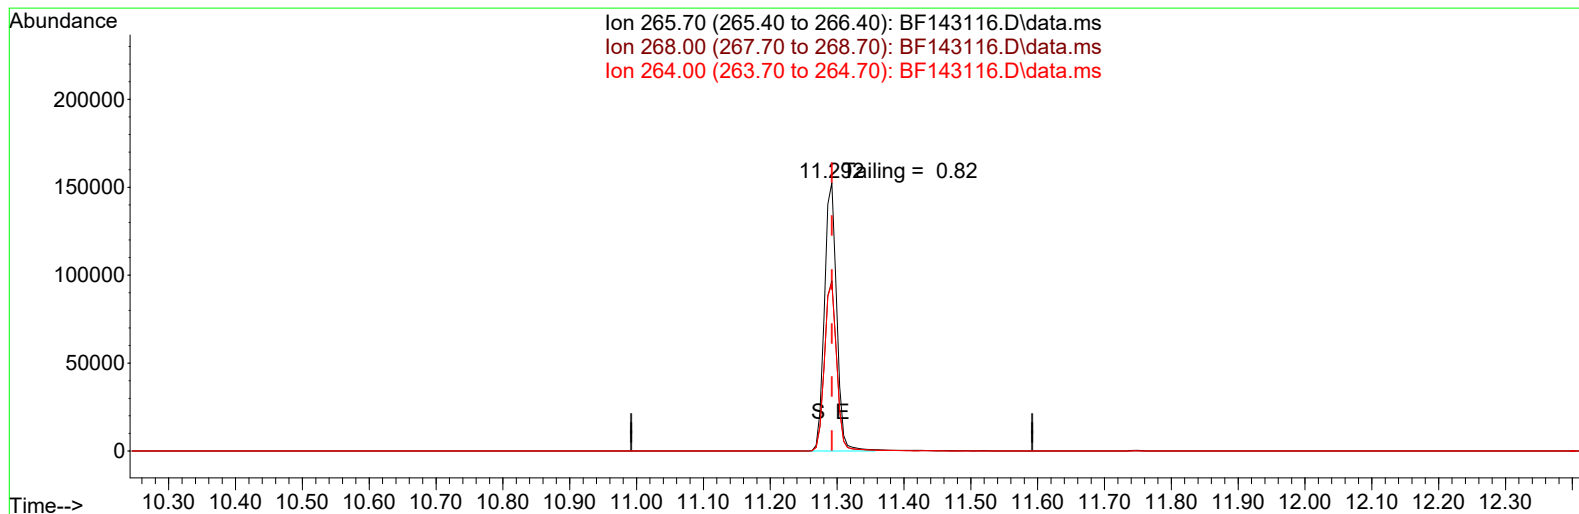

TIC: BF143116.D\data.ms

(70) Pentachlorophenol (C)




11.292min (-0.000) 32920.43 ng

response 195924

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	63.41
264.00	62.10	62.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143116.D
Acq On : 16 Jul 2025 19:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 17 03:11:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 15 17:53:25 2025
Response via : Initial Calibration

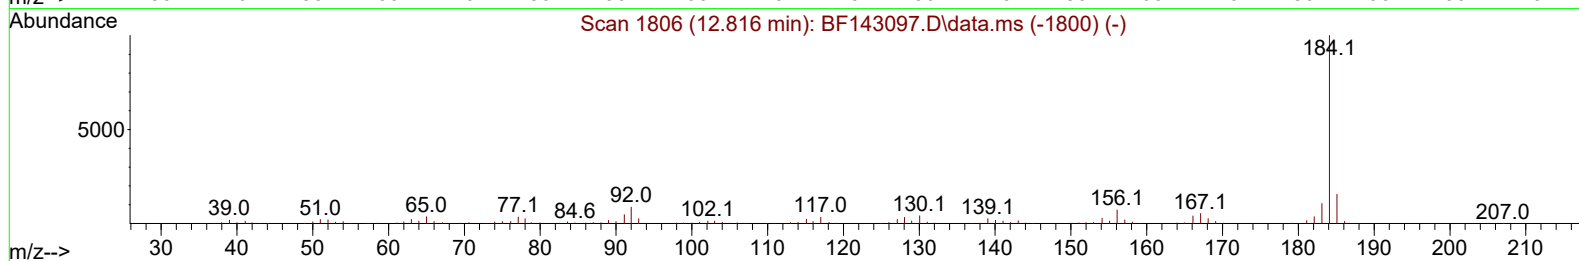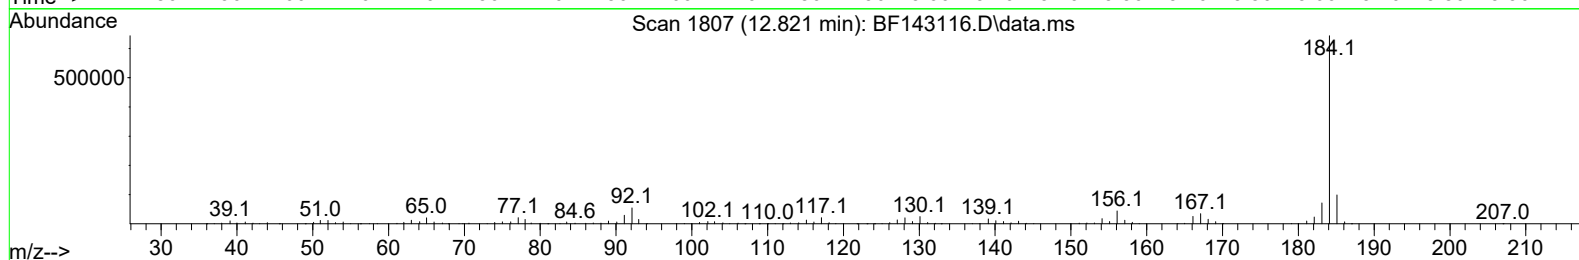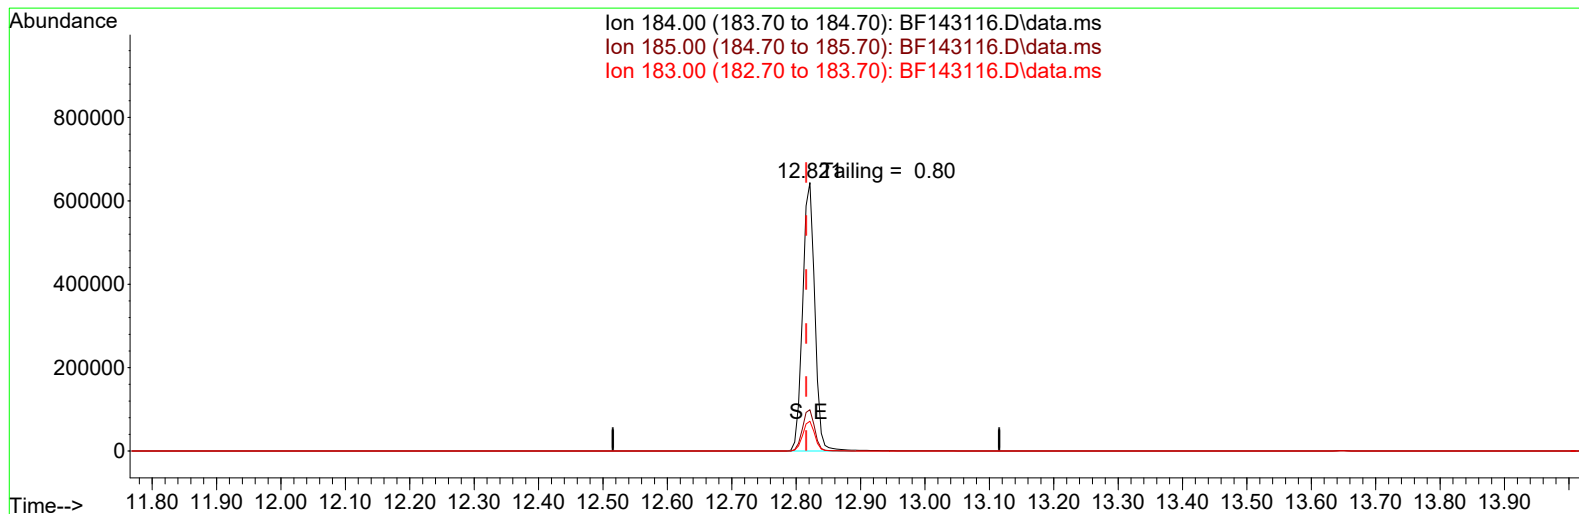

TIC: BF143116.D\data.ms

(77) Benzidine

12.821min (+ 0.006) 0.00 ng

response 848698

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.39
183.00	10.70	11.10
0.00	0.00	0.00