

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
 Data File : BF143133.D
 Acq On : 17 Jul 2025 03:32
 Operator : RC/JU
 Sample : Q2555-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-29-070925

Manual Integrations
 APPROVED

Reviewed By :Rahul
 Chavli

07/17/2025
 Supervised By :Jagrut
 Upadhyay

Quant Time: Jul 17 04:45:42 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 15 17:53:25 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.969	152	148153	20.000	ng	0.00
21) Naphthalene-d8	8.245	136	532010	20.000	ng	0.00
39) Acenaphthene-d10	10.004	164	233880	20.000	ng	0.00
64) Phenanthrene-d10	11.486	188	324353	20.000	ng	0.00
76) Chrysene-d12	14.127	240	293654	20.000	ng	0.00
86) Perylene-d12	15.633	264	265449	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.592	112	640693	68.325	ng	0.00
7) Phenol-d6	6.581	99	820567	69.616	ng	0.00
23) Nitrobenzene-d5	7.522	82	513304	54.126	ng	0.00
42) 2,4,6-Tribromophenol	10.786	330	120229	57.653	ng	0.00
45) 2-Fluorobiphenyl	9.322	172	859190	48.833	ng	0.00
79) Terphenyl-d14	13.068	244	594491	29.594	ng	0.00
Target Compounds						
32) Benzoic acid	7.922	122	10466	8.654	ng	Qvalue 91
75) Fluoranthene	12.698	202	38282	2.405	ng	99
84) Bis(2-ethylhexyl)phtha...	14.110	149	10200	4.559	ng	# 99
88) Benzo(b)fluoranthene	15.186	252	46105m	3.011	ng	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143133.D
Acq On : 17 Jul 2025 03:32
Operator : RC/JU
Sample : Q2555-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-29-070925


Quant Time: Jul 17 04:45:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 15 17:53:25 2025
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Rahul
Chavli

07/17/2025
Supervised By :Jagrut
Upadhyay


07/17/2025

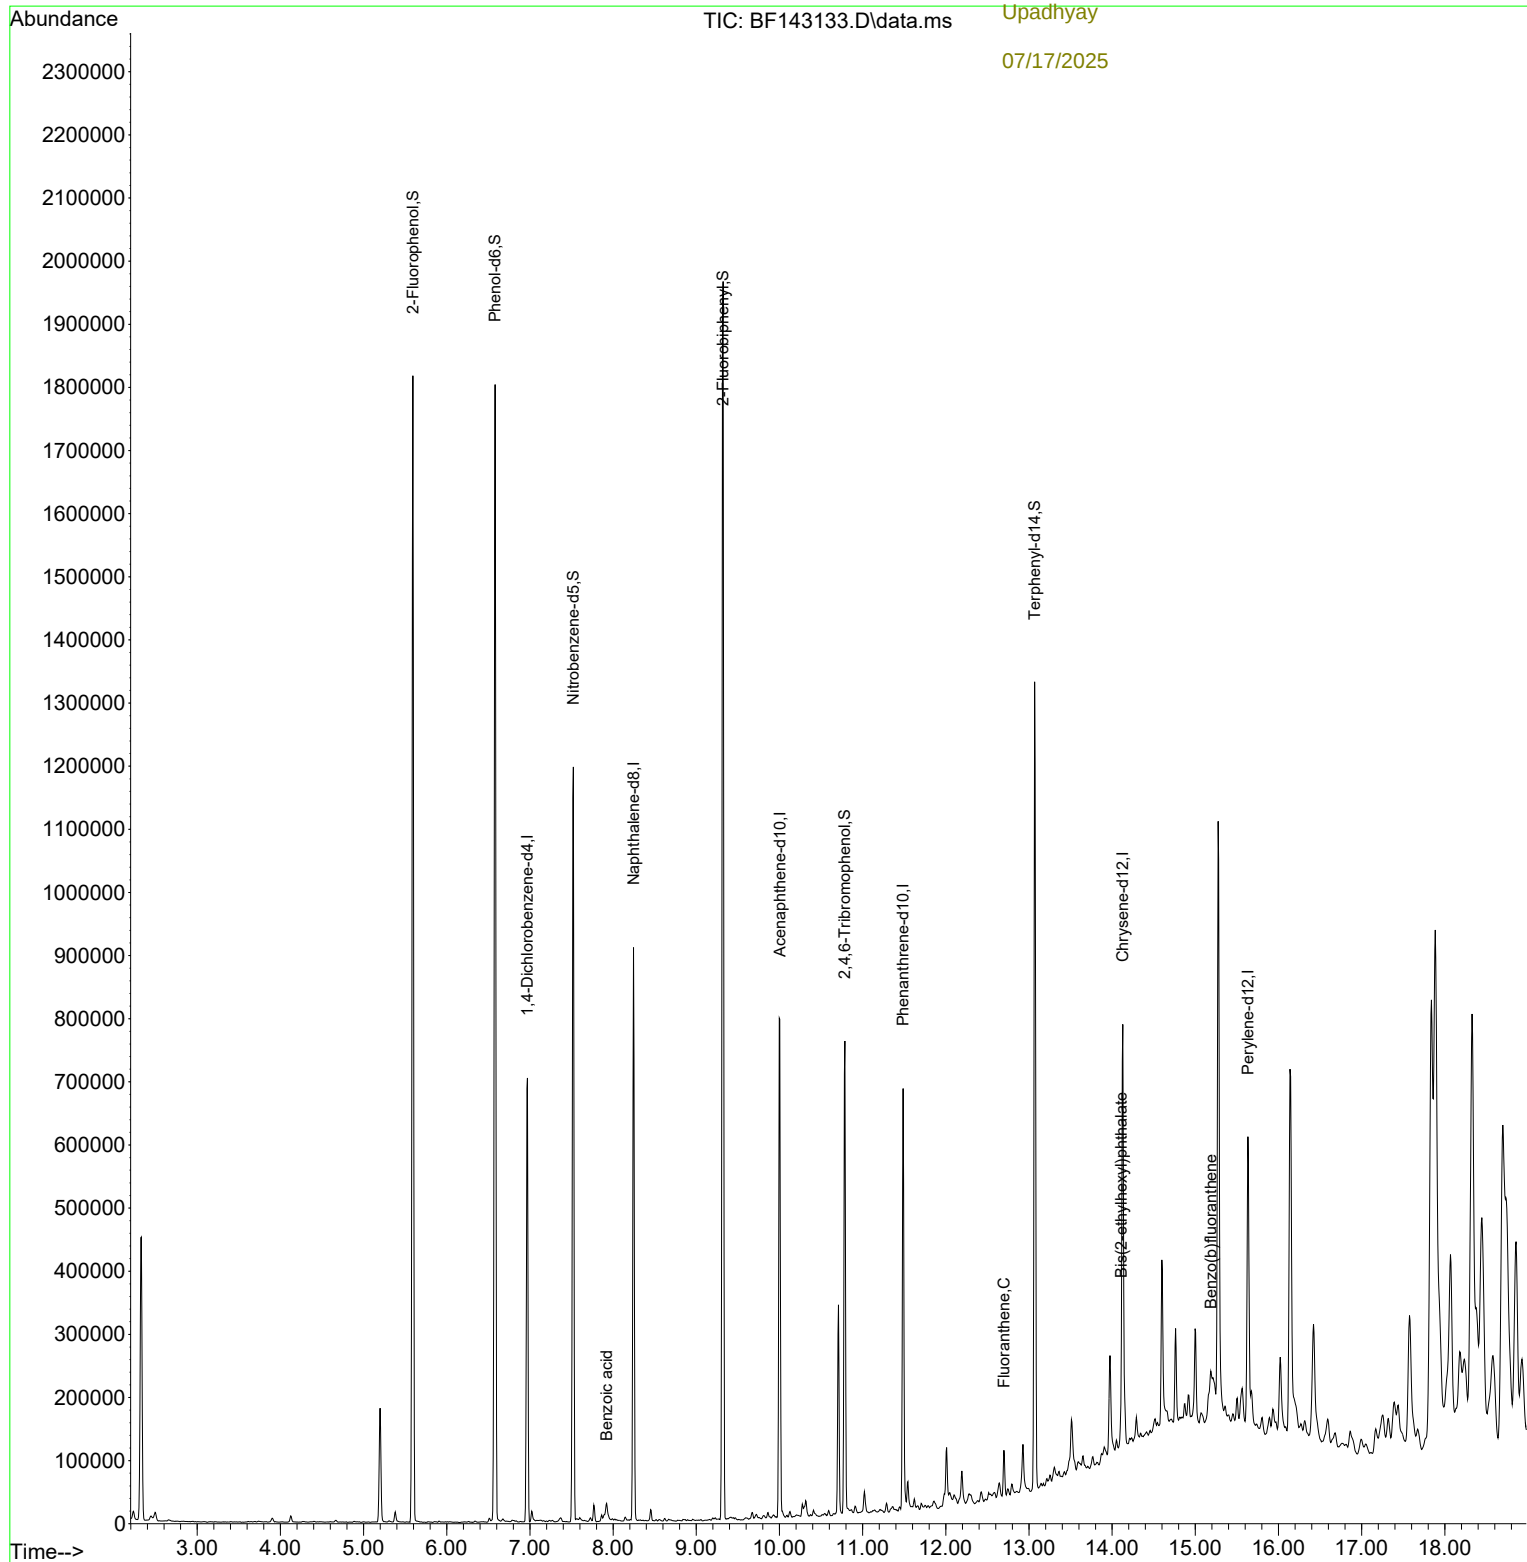



#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.969 min Scan# 812
Delta R.T. -0.000 min
Lab File: BF143133.D
Acq: 17 Jul 2025 03:32

Instrument :
BNA_F
ClientSampleId :
OU4-TS-29-070925






Tgt Ion:152 Resp: 14815
Ion Ratio Lower Upper
152 100
150 154.7 126.5 189.7
115 60.0 47.0 70.6

Manual Integrations
APPROVED


Reviewed By :Rahul
Chavli

07/17/2025
Supervised By :Jagrut
Upadhyay



07/17/2025

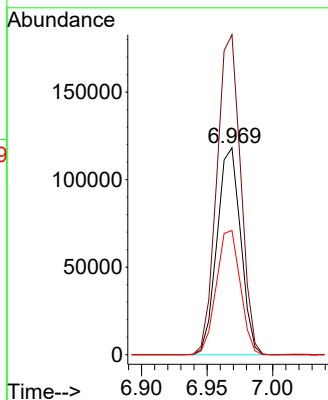


#5
2-Fluorophenol
Concen: 68.325 ng
RT: 5.592 min Scan# 578
Delta R.T. 0.006 min
Lab File: BF143133.D
Acq: 17 Jul 2025 03:32




Tgt Ion:112 Resp: 640693
Ion Ratio Lower Upper
112 100
64 66.1 54.6 82.0
63 33.1 27.3 40.9

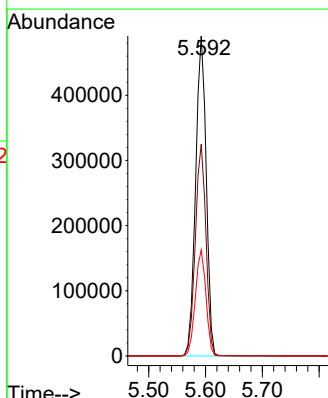



#7
Phenol-d6
Concen: 69.616 ng
RT: 6.581 min Scan# 74
Delta R.T. -0.006 min
Lab File: BF143133.D
Acq: 17 Jul 2025 03:32

Instrument :
BNA_F
ClientSampleId :
OU4-TS-29-070925






Tgt Ion: 99 Resp: 82056
Ion Ratio Lower Upper
99 100
42 21.1 17.2 25.8
71 34.1 27.4 41.0

Manual Integrations
APPROVED

Reviewed By :Rahul
Chavli




07/17/2025
Supervised By :Jagrut
Upadhyay


07/17/2025

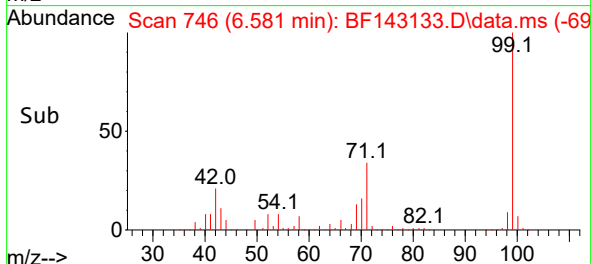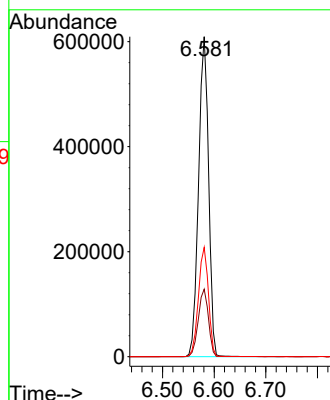

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.245 min Scan# 1029
Delta R.T. -0.006 min
Lab File: BF143133.D
Acq: 17 Jul 2025 03:32


Tgt Ion:136 Resp: 532010
Ion Ratio Lower Upper
136 100
137 10.9 8.9 13.3
54 10.1 8.3 12.5
68 6.8 5.3 7.9

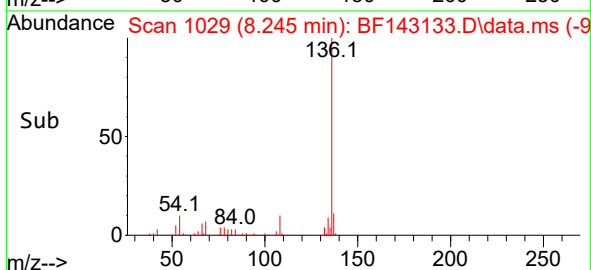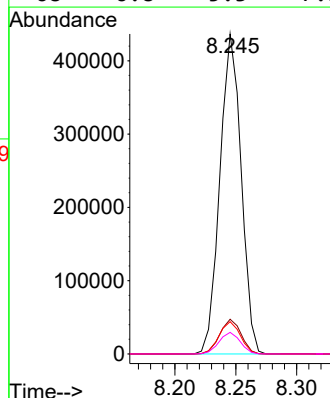



#23
Nitrobenzene-d5
Concen: 54.126 ng
RT: 7.522 min Scan# 907
Delta R.T. -0.006 min
Lab File: BF143133.D
Acq: 17 Jul 2025 03:32

Instrument :
BNA_F
ClientSampleId :
OU4-TS-29-070925






Tgt Ion: 82 Resp: 513304
Ion Ratio Lower Upper
82 100
128 42.4 33.3 49.9
54 58.9 47.4 71.2

Manual Integrations
APPROVED

Reviewed By :Rahul
Chavli




07/17/2025
Supervised By :Jagrut
Upadhyay


07/17/2025

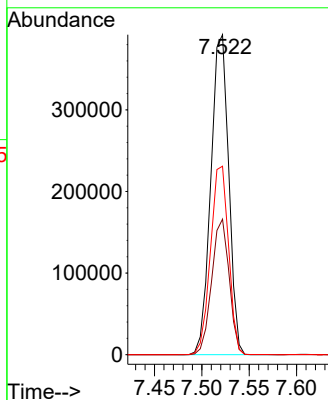

#32
Benzoic acid
Concen: 8.654 ng
RT: 7.922 min Scan# 974
Delta R.T. -0.065 min
Lab File: BF143133.D
Acq: 17 Jul 2025 03:32


Tgt Ion:122 Resp: 10466
Ion Ratio Lower Upper
122 100
105 113.1 105.4 145.4
77 90.9 78.6 118.6

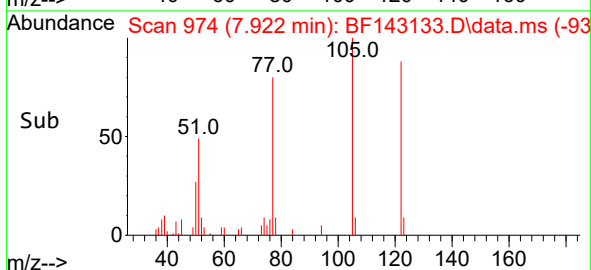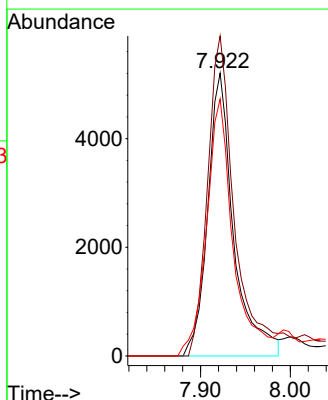



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.004 min Scan# 11
Delta R.T. -0.000 min
Lab File: BF143133.D
Acq: 17 Jul 2025 03:32

Instrument :
BNA_F
ClientSampleId :
OU4-TS-29-070925






Tgt Ion:164 Resp: 233880
Ion Ratio Lower Upper
164 100
162 99.3 79.0 118.6
160 44.8 35.8 53.6

Manual Integrations
APPROVED

Reviewed By :Rahul
Chavli




07/17/2025
Supervised By :Jagrut
Upadhyay


07/17/2025

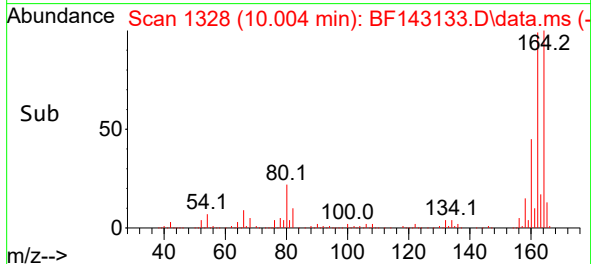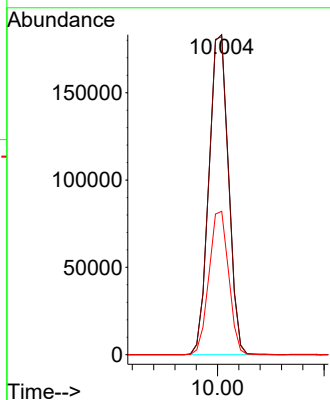

#42
2,4,6-Tribromophenol
Concen: 57.653 ng
RT: 10.786 min Scan# 1461
Delta R.T. -0.006 min
Lab File: BF143133.D
Acq: 17 Jul 2025 03:32

Tgt Ion:330 Resp: 120229
Ion Ratio Lower Upper
330 100
332 98.2 77.9 116.9
141 32.1 25.9 38.9

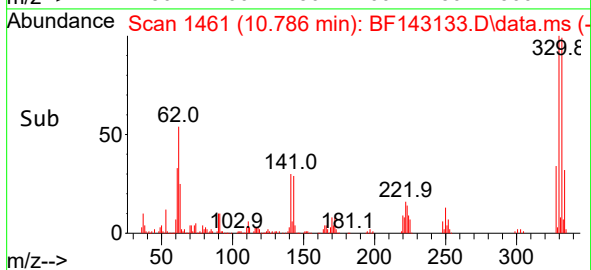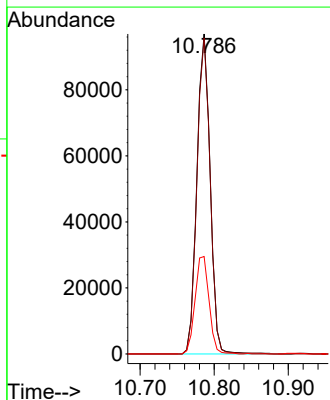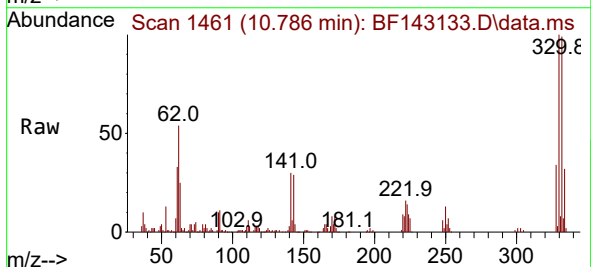



#45

2-Fluorobiphenyl

Concen: 48.833 ng

RT: 9.322 min Scan# 1

Delta R.T. -0.006 min

Lab File: BF143133.D


Acq: 17 Jul 2025 03:32

Instrument :

BNA_F

ClientSampleId :

OU4-TS-29-070925



Tgt Ion:172 Resp: 859190

Ion Ratio Lower Upper

172 100

171 34.9 28.2 42.4

170 22.9 18.6 28.0

Manual Integrations



APPROVED

Reviewed By :Rahul
Chavli

07/17/2025

Supervised By :Jagrut
Upadhyay

07/17/2025

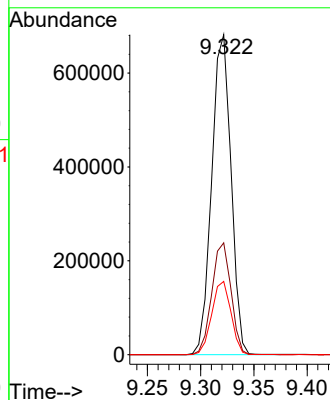

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.486 min Scan# 1580

Delta R.T. -0.006 min

Lab File: BF143133.D

Acq: 17 Jul 2025 03:32




Tgt Ion:188 Resp: 324353


Ion Ratio Lower Upper

188 100

94 10.5 8.6 13.0


80 11.6 9.3 13.9

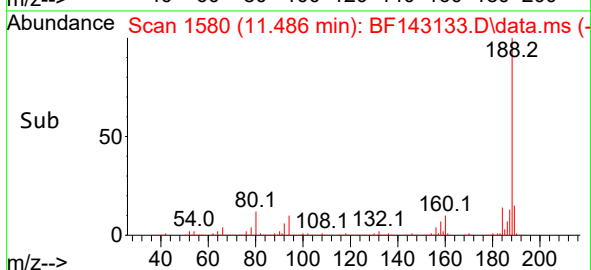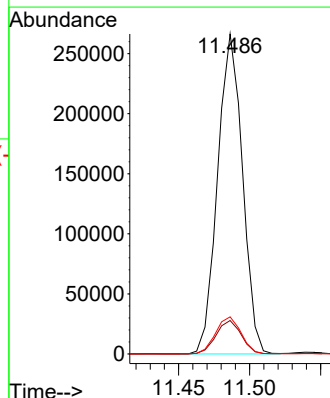



#75
Fluoranthene
Concen: 2.405 ng
RT: 12.698 min Scan# 1786
Delta R.T. -0.006 min
Lab File: BF143133.D
Acq: 17 Jul 2025 03:32

Instrument :
BNA_F
ClientSampleId :
OU4-TS-29-070925





Tgt Ion:202 Resp: 3828
Ion Ratio Lower Upper
202 100
101 12.7 0.0 32.4
203 17.1 0.0 37.4

Manual Integrations
APPROVED

Reviewed By :Rahul
Chavli




07/17/2025
Supervised By :Jagrut
Upadhyay


07/17/2025

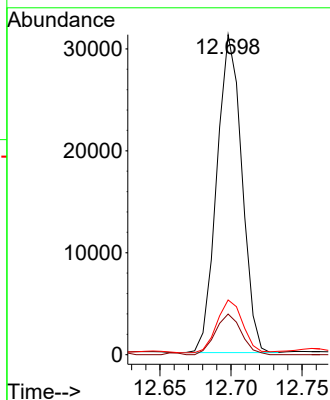

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.127 min Scan# 2029
Delta R.T. -0.000 min
Lab File: BF143133.D
Acq: 17 Jul 2025 03:32


Tgt Ion:240 Resp: 293654
Ion Ratio Lower Upper
240 100
120 11.7 10.0 15.0
236 25.2 20.0 30.0

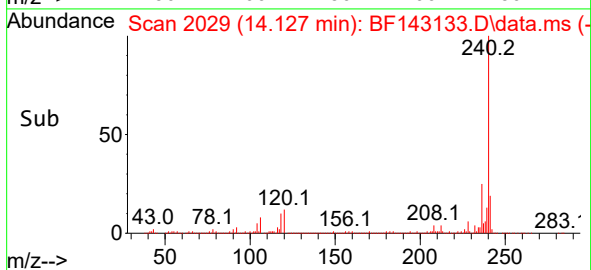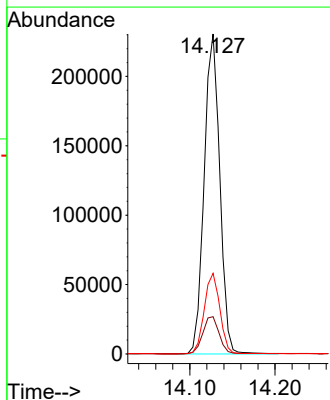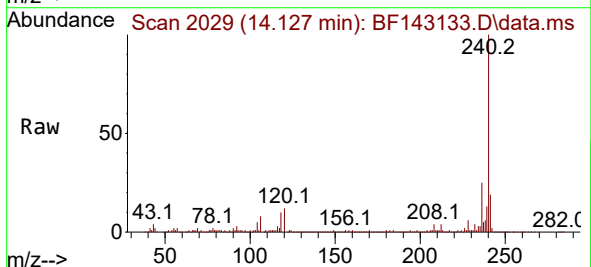



#79
 Terphenyl-d14
 Concen: 29.594 ng
 RT: 13.068 min Scan# 1849
 Delta R.T. -0.006 min
 Lab File: BF143133.D
 Acq: 17 Jul 2025 03:32

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-29-070925






Tgt Ion:244 Resp: 59449
 Ion Ratio Lower Upper
 244 100
 212 6.6 5.2 7.8
 122 11.7 8.8 13.2

Manual Integrations
 APPROVED

Reviewed By :Rahul
 Chavli




07/17/2025
 Supervised By :Jagrut
 Upadhyay


07/17/2025

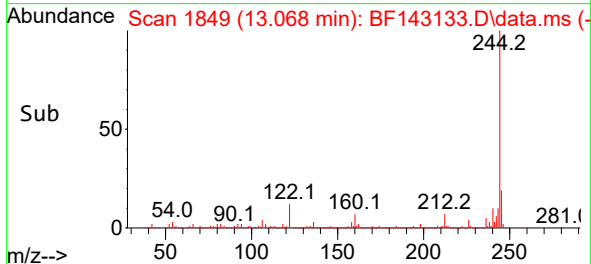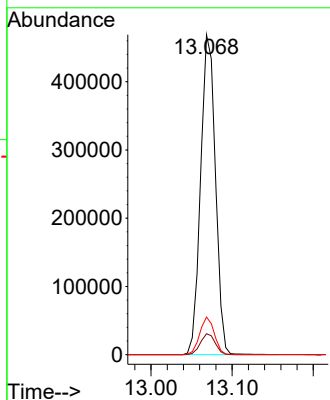

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 4.559 ng
 RT: 14.110 min Scan# 2026
 Delta R.T. -0.000 min
 Lab File: BF143133.D
 Acq: 17 Jul 2025 03:32


Tgt Ion:149 Resp: 10200
 Ion Ratio Lower Upper
 149 100
 167 28.0 21.9 32.9
 279 5.1 3.4 5.0#

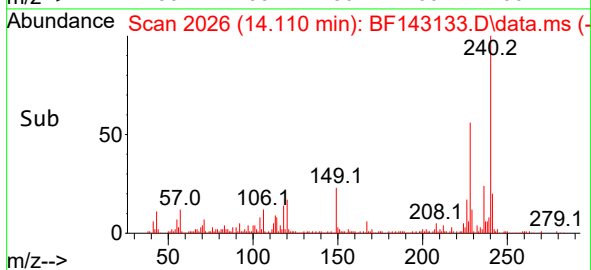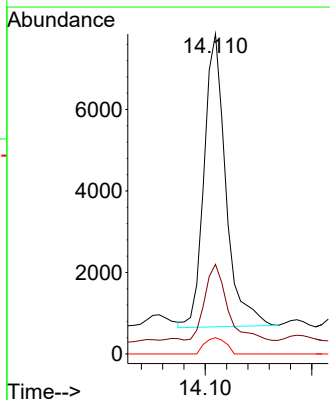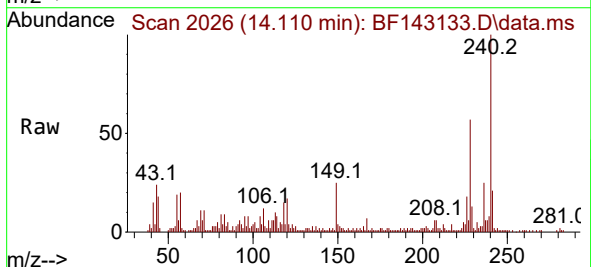



#86
Perylene-d12
Concen: 20.000 ng
RT: 15.633 min Scan# 21
Delta R.T. -0.006 min
Lab File: BF143133.D
Acq: 17 Jul 2025 03:32

Instrument :
BNA_F
ClientSampleId :
OU4-TS-29-070925






Tgt Ion:264 Resp: 265449
Ion Ratio Lower Upper
264 100
260 23.5 18.5 27.7
265 22.0 17.5 26.3

Manual Integrations
APPROVED


Reviewed By :Rahul
Chavli

07/17/2025
Supervised By :Jagrut
Upadhyay

07/17/2025

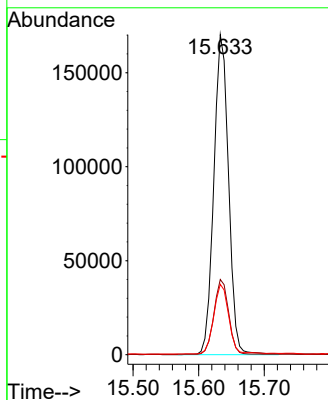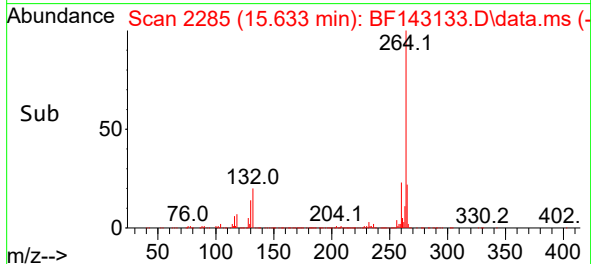

#88
Benzo(b)fluoranthene
Concen: 3.011 ng m
RT: 15.186 min Scan# 2209
Delta R.T. -0.006 min
Lab File: BF143133.D
Acq: 17 Jul 2025 03:32



Tgt Ion:252 Resp: 46105
Ion Ratio Lower Upper
252 100
253 24.7 17.5 26.3
125 16.3 8.6 13.0#

