

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
 Data File : BF143133.D
 Acq On : 17 Jul 2025 03:32
 Operator : RC/JU
 Sample : Q2555-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-29-070925

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143133.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.328	15	23	30	rVB	448736	731493	29.30%	2.148%
2	2.493	46	51	58	rVB	13589	27310	1.09%	0.080%
3	5.198	504	511	520	rBV	180327	267709	10.72%	0.786%
4	5.592	572	578	583	rBV	1815948	2371082	94.97%	6.963%
5	6.581	739	746	751	rBV	1798913	2430762	97.36%	7.139%
6	6.969	806	812	817	rVB	703361	897720	35.96%	2.636%
7	7.022	817	821	829	rBV	17050	27796	1.11%	0.082%
8	7.522	899	906	911	rBV	1195850	1573990	63.05%	4.622%
9	7.769	944	948	953	rVB	26258	31578	1.26%	0.093%
10	7.922	966	974	983	rVB2	25862	56758	2.27%	0.167%
11	8.245	1024	1029	1037	rVB	907556	1113100	44.58%	3.269%
12	9.322	1206	1212	1217	rBV	1961207	2496584	100.00%	7.332%
13	9.998	1322	1327	1332	rBV	791184	1025961	41.09%	3.013%
14	10.316	1379	1381	1389	rVB3	24424	32494	1.30%	0.095%
15	10.710	1443	1448	1455	rVB	330373	403783	16.17%	1.186%
16	10.786	1455	1461	1466	rBV	748216	962083	38.54%	2.825%
17	11.022	1497	1501	1510	rVB2	33357	50706	2.03%	0.149%
18	11.486	1575	1580	1587	rBV	665893	847164	33.93%	2.488%
19	11.545	1587	1590	1596	rVB2	40383	54852	2.20%	0.161%
20	12.010	1660	1669	1673	rBV3	92947	166104	6.65%	0.488%
21	12.192	1696	1700	1708	rVB4	51503	80242	3.21%	0.236%
22	12.645	1772	1777	1782	rVB4	21015	37290	1.49%	0.110%
23	12.698	1782	1786	1791	rBV	72740	93401	3.74%	0.274%
24	12.792	1799	1802	1808	rBV4	17389	29060	1.16%	0.085%
25	12.927	1820	1825	1834	rVB	70141	109885	4.40%	0.323%
26	13.068	1844	1849	1857	rBV	1278510	1626775	65.16%	4.777%
27	13.510	1920	1924	1934	rVB3	79690	161120	6.45%	0.473%
28	13.974	1998	2003	2013	rBV2	155618	278373	11.15%	0.818%
29	14.127	2023	2029	2040	rVB	664197	1015156	40.66%	2.981%
30	14.598	2105	2109	2118	rBV	259785	418420	16.76%	1.229%
31	14.762	2133	2137	2143	rBV	146941	198055	7.93%	0.582%
32	14.998	2174	2177	2185	rVB	148847	219673	8.80%	0.645%
33	15.274	2219	2224	2235	rVB	933375	1476372	59.14%	4.336%
34	15.633	2280	2285	2290	rBV	445663	689960	27.64%	2.026%
35	16.021	2346	2351	2360	rBV	111402	210570	8.43%	0.618%
36	16.139	2365	2371	2389	rBV	572941	1232096	49.35%	3.618%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143133.D
Acq On : 17 Jul 2025 03:32
Operator : RC/JU
Sample : Q2555-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-29-070925

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	16.421	2413	2419	2435	rVB3	186638	496300	19.88%	1.458%
38	17.574	2609	2615	2628	rVB4	190951	485028	19.43%	1.424%
39	17.839	2651	2660	2664	rBV2	682157	1895499	75.92%	5.567%
40	17.886	2664	2668	2685	rVB3	767015	2248275	90.05%	6.603%
41	18.068	2694	2699	2707	rVB	249681	584528	23.41%	1.717%
42	18.180	2714	2718	2723	rBV4	69258	153771	6.16%	0.452%
43	18.327	2735	2743	2750	rBV	605842	1643882	65.85%	4.828%
44	18.445	2757	2763	2774	rVB5	310512	953608	38.20%	2.801%
45	18.698	2797	2806	2811	rBV2	491480	1538343	61.62%	4.518%
46	18.856	2826	2833	2840	rBV2	251098	606354	24.29%	1.781%




Sum of corrected areas: 34051065

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143133.D
Acq On : 17 Jul 2025 03:32
Operator : RC/JU
Sample : Q2555-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-29-070925

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

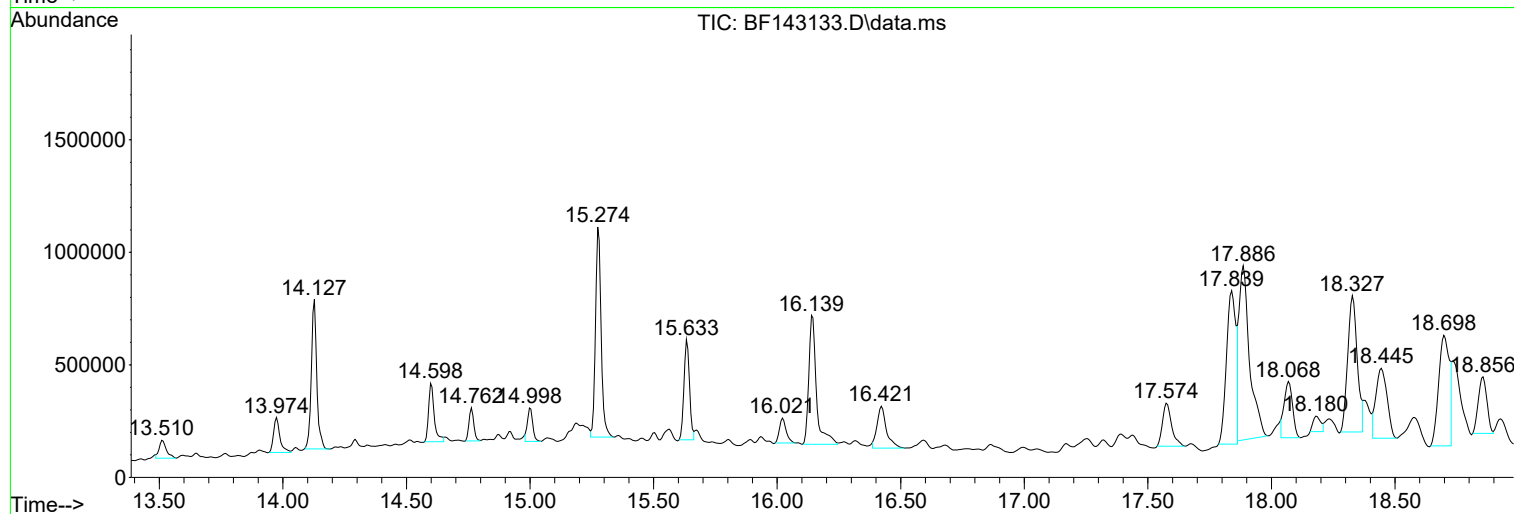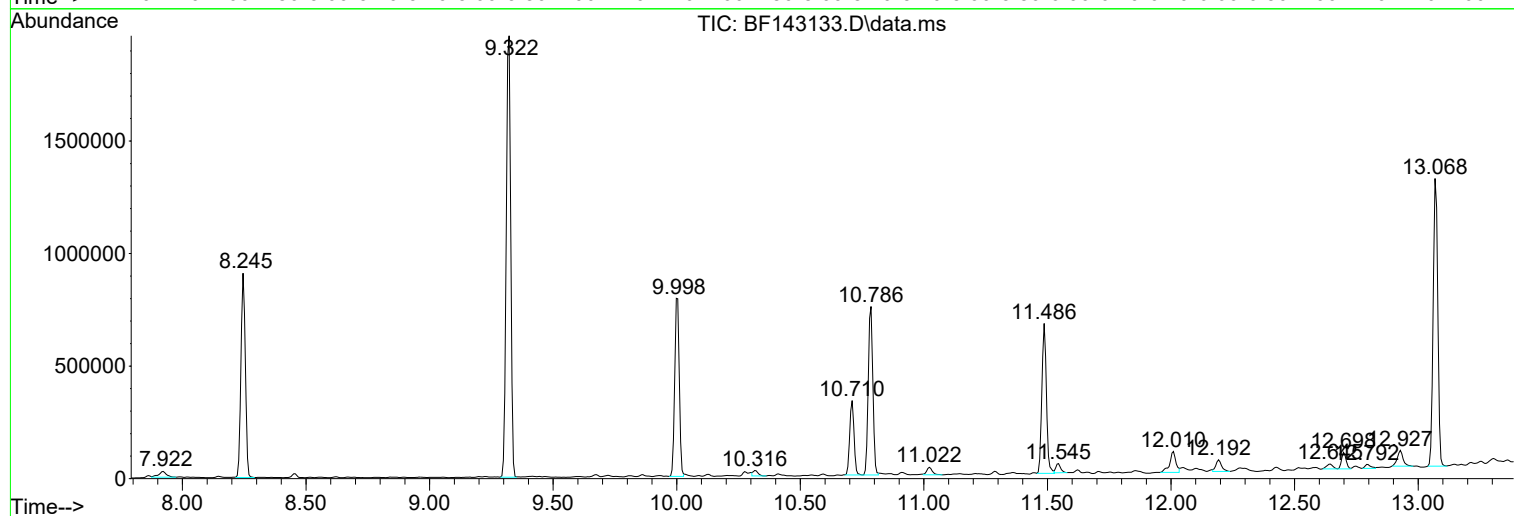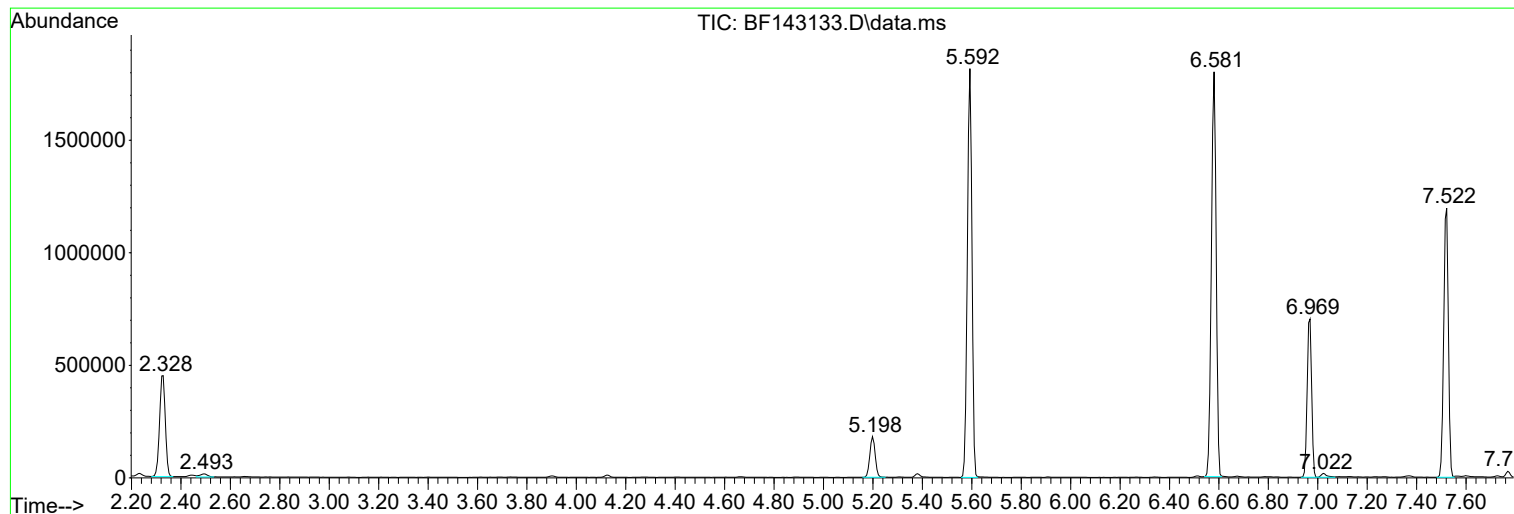

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143133.D
Acq On : 17 Jul 2025 03:32
Operator : RC/JU
Sample : Q2555-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-29-070925

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071625\
Data File : BF143133.D
Acq On : 17 Jul 2025 03:32
Operator : RC/JU
Sample : Q2555-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-29-070925

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------