
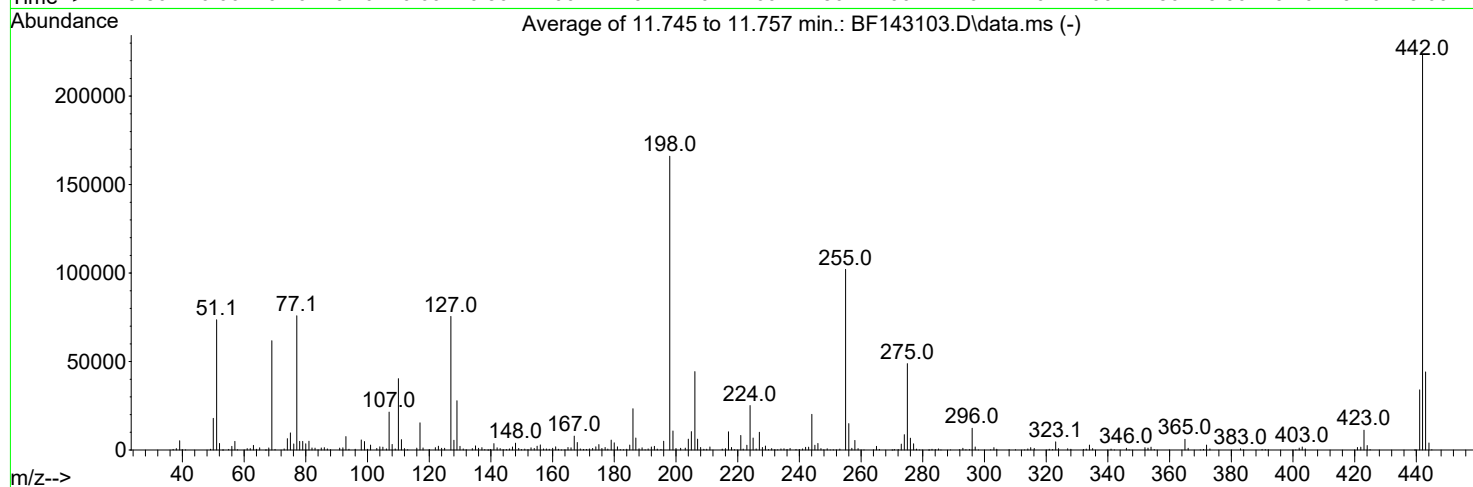


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF071625\  
Data File : BF143103.D  
Acq On : 16 Jul 2025 09:06  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF071525.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Jul 15 17:53:25 2025

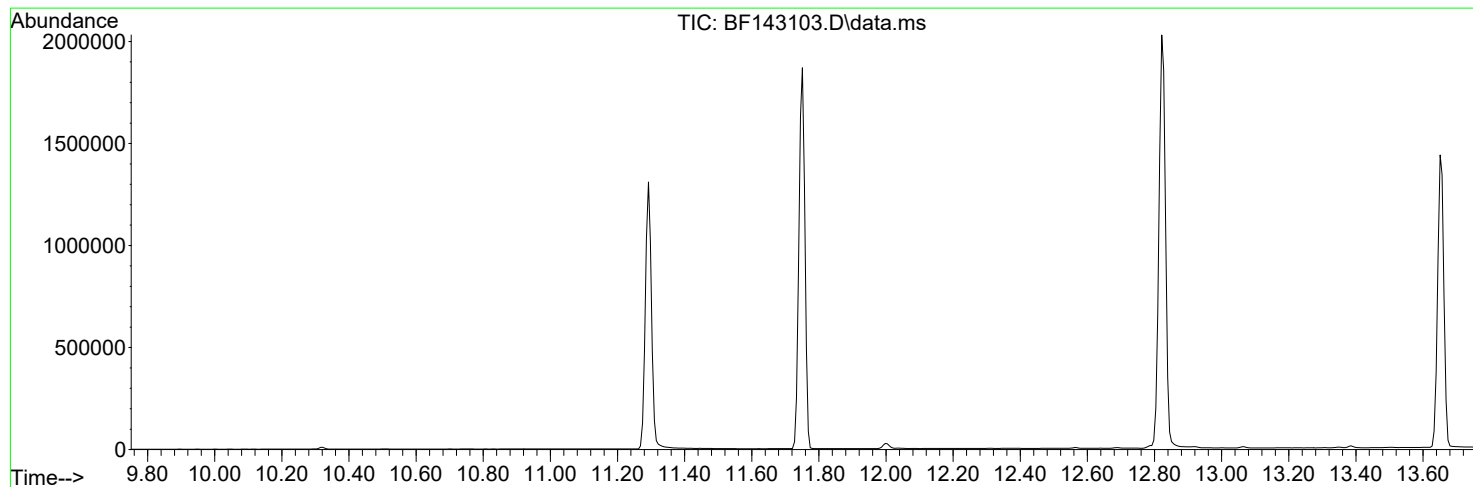

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1617

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 68          | 69           | 0.00         | 2            | 1.9       | 1154    | PASS             |
| 69          | 69           | 100          | 100          | 100.0     | 61736   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 361     | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 166040  | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 10739   | PASS             |
| 365         | 198          | 1            | 100          | 3.7       | 6100    | PASS             |
| 441         | 443          | 0.01         | 150          | 77.0      | 33984   | PASS             |
| 442         | 442          | 100          | 100          | 100.0     | 223147  | PASS             |
| 443         | 442          | 15           | 24           | 19.8      | 44128   | PASS             |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 7/16/2025     | BNA_F            | <u>BF143103.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 313998           | 13.651             |
| DDD           | 3323             | 13.386             |
| DDE           | 0                | 13.01              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 3323          | 317321           | 1.05               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF071625\  
Data File : BF143103.D  
Acq On : 16 Jul 2025 09:06  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jul 16 11:19:42 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF071525.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jul 15 17:53:25 2025  
Response via : Initial Calibration

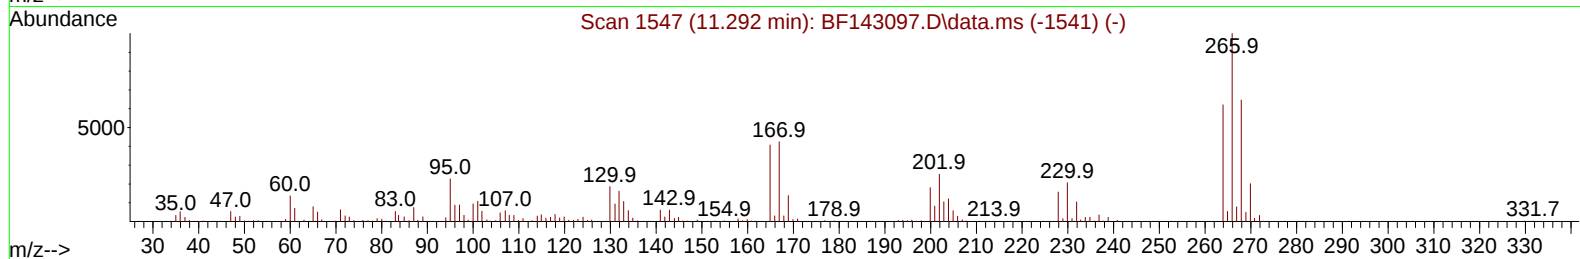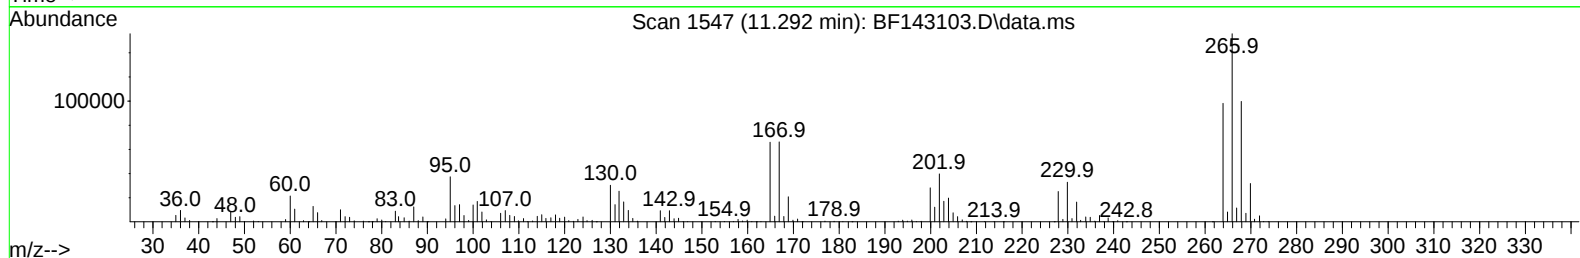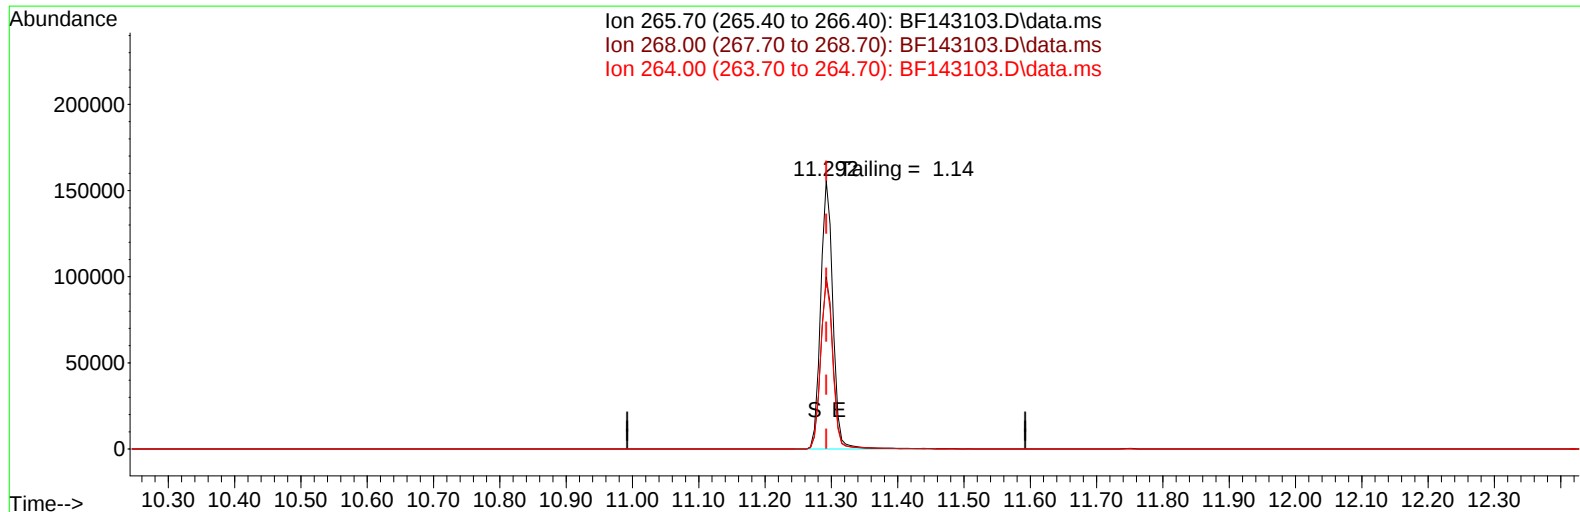

TIC: BF143103.D\data.ms

**(70) Pentachlorophenol (C)**

**11.292min (-0.000) 57968.33 ng**




**response 199936**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.70  | 64.06  |
| 264.00 | 62.10  | 62.99  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF071625\  
Data File : BF143103.D  
Acq On : 16 Jul 2025 09:06  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jul 16 11:19:42 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF071525.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jul 15 17:53:25 2025  
Response via : Initial Calibration

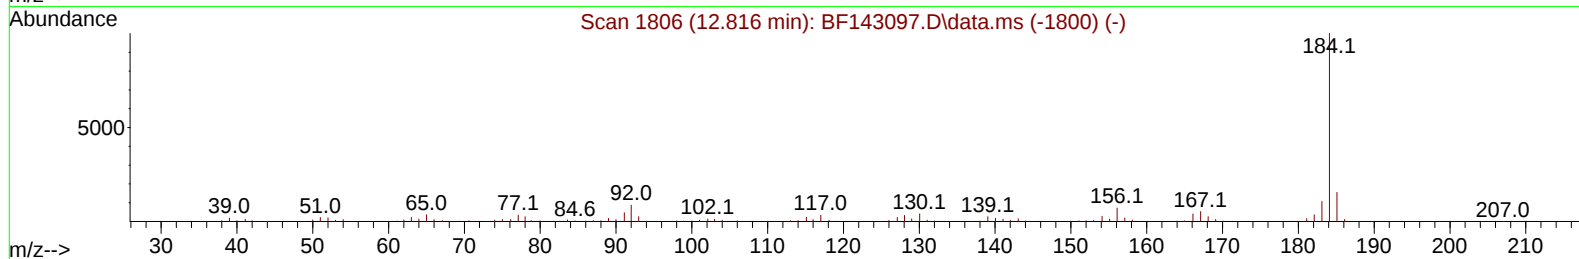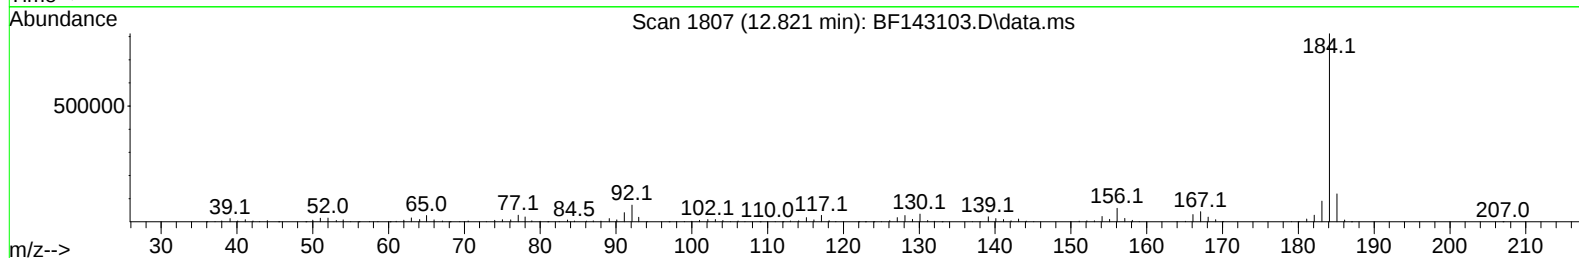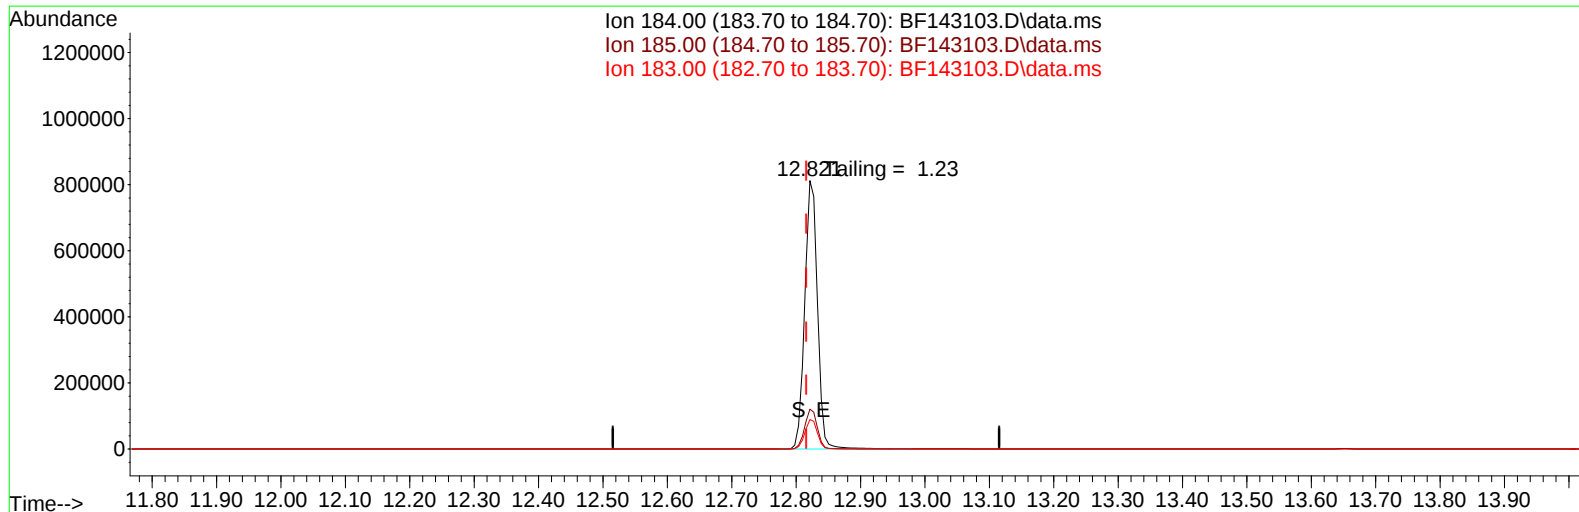

TIC: BF143103.D\data.ms

(77) Benzidine

12.821min (+ 0.006) 53995.93 ng

response 1120309

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.84  |
| 183.00 | 10.70  | 11.01  |
| 0.00   | 0.00   | 0.00   |