
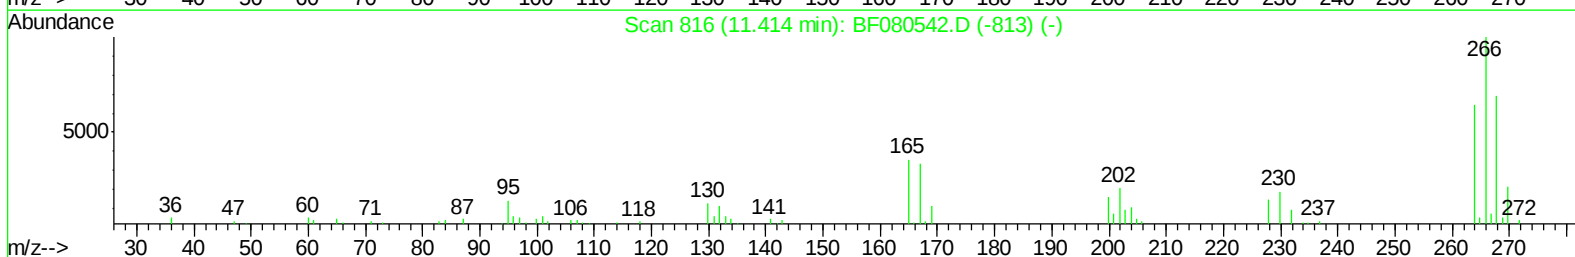
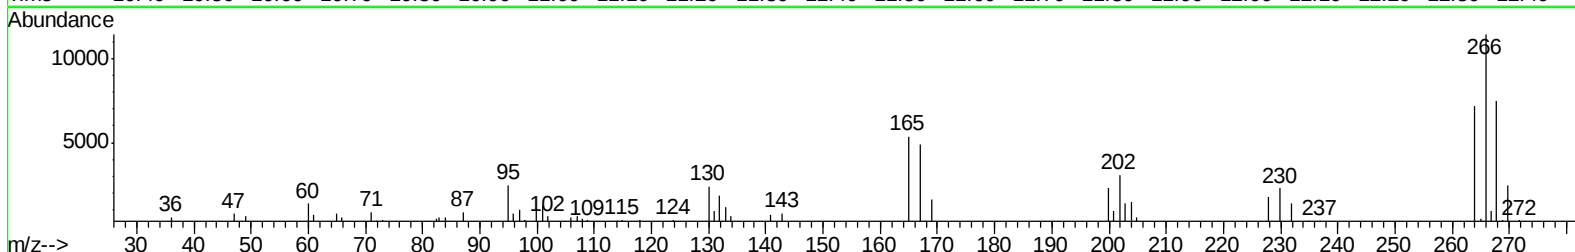


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071715\
Data File : BF080534.D
Acq On : 17 Jul 2015 15:23
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 00:46:12 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 18 00:40:00 2015
Response via : Initial Calibration

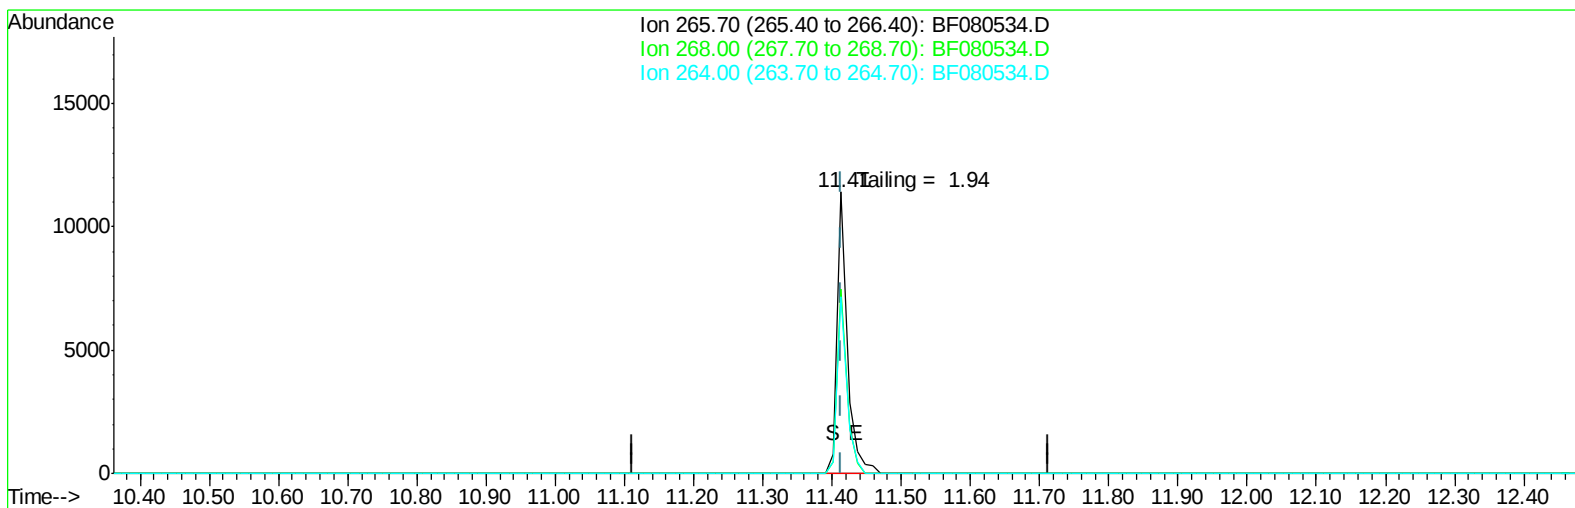

TIC: BF080534.D

(69) Pentachlorophenol (C)




11.414min (+0.001) 0.00ng

response 11425

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	65.59
264.00	64.20	62.93
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071715\
Data File : BF080534.D
Acq On : 17 Jul 2015 15:23
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 00:46:12 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 18 00:40:00 2015
Response via : Initial Calibration

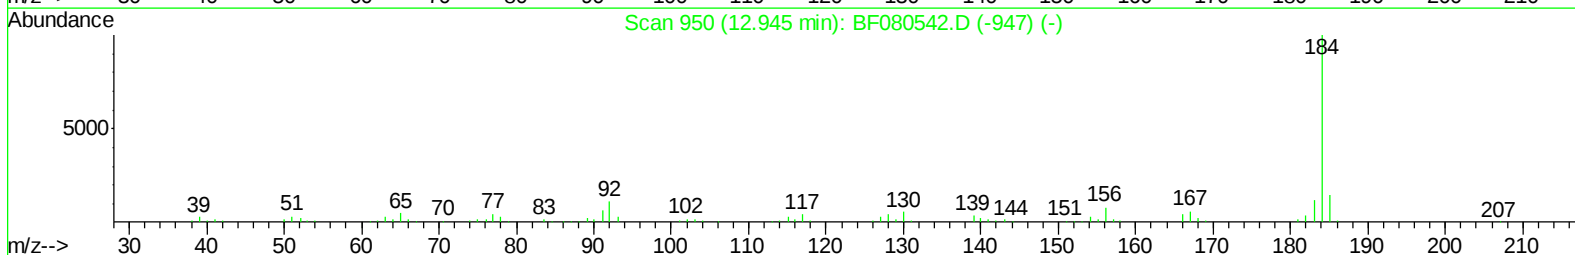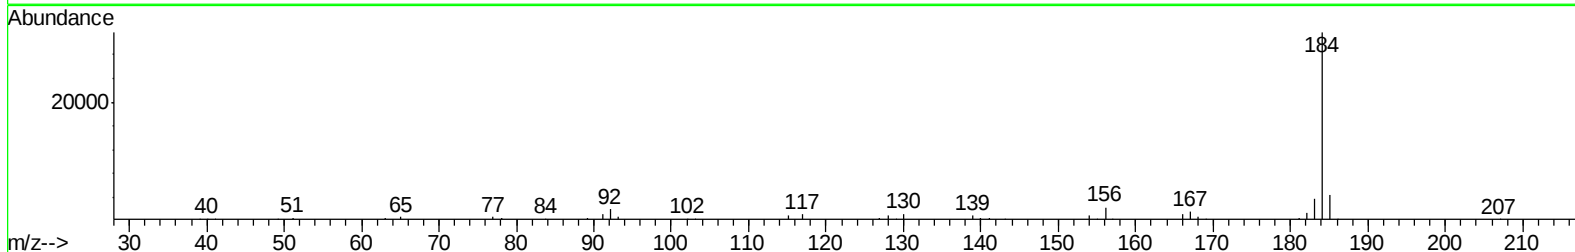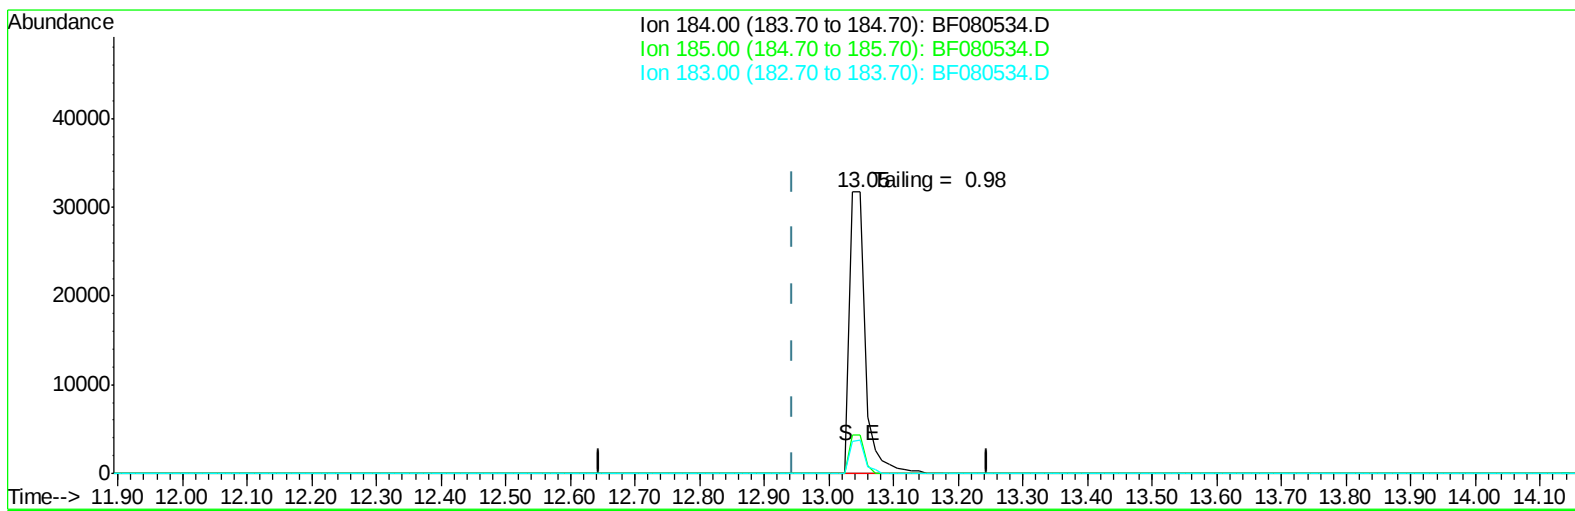

TIC: BF080534.D

(76) Benzidine

13.048min (+0.103) 0.00ng

response 52617

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	13.59
183.00	11.60	11.84
0.00	0.00	0.00