

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071715\
 Data File : BF080550.D
 Acq On : 17 Jul 2015 23:20
 Operator : TP/UM
 Sample : G2996-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SOUTH-EAST-WALL1-071415

Quant Time: Jul 18 07:06:05 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 18 00:40:00 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.07	152	49735	20.00	ng	0.00
21) Naphthalene-d8	8.35	136	201247	20.00	ng	0.00
38) Acenaphthene-d10	10.11	164	85873	20.00	ng	0.00
63) Phenanthrene-d10	11.60	188	177540	20.00	ng	0.00
75) Chrysene-d12	14.34	240	141045	20.00	ng	-0.01
86) Perylene-d12	15.99	264	126998	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	417235	130.80	ng	0.00
7) Phenol-d6	6.70	99	509644	140.39	ng	0.00
23) Nitrobenzene-d5	7.63	82	294057	93.16	ng	0.00
41) 2,4,6-Tribromophenol	10.90	330	113164	147.27	ng	0.00
44) 2-Fluorobiphenyl	9.42	172	526458	86.11	ng	0.00
78) Terphenyl-d14	13.19	244	460266	72.87	ng	-0.01
Target Compounds						
49) Dimethylphthalate	9.82	163	109964	19.24	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071715\
Data File : BF080550.D
Acq On : 17 Jul 2015 23:20
Operator : TP/UM
Sample : G2996-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SOUTH-EAST-WALL1-071415

Quant Time: Jul 18 07:06:05 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 18 00:40:00 2015
Response via : Initial Calibration

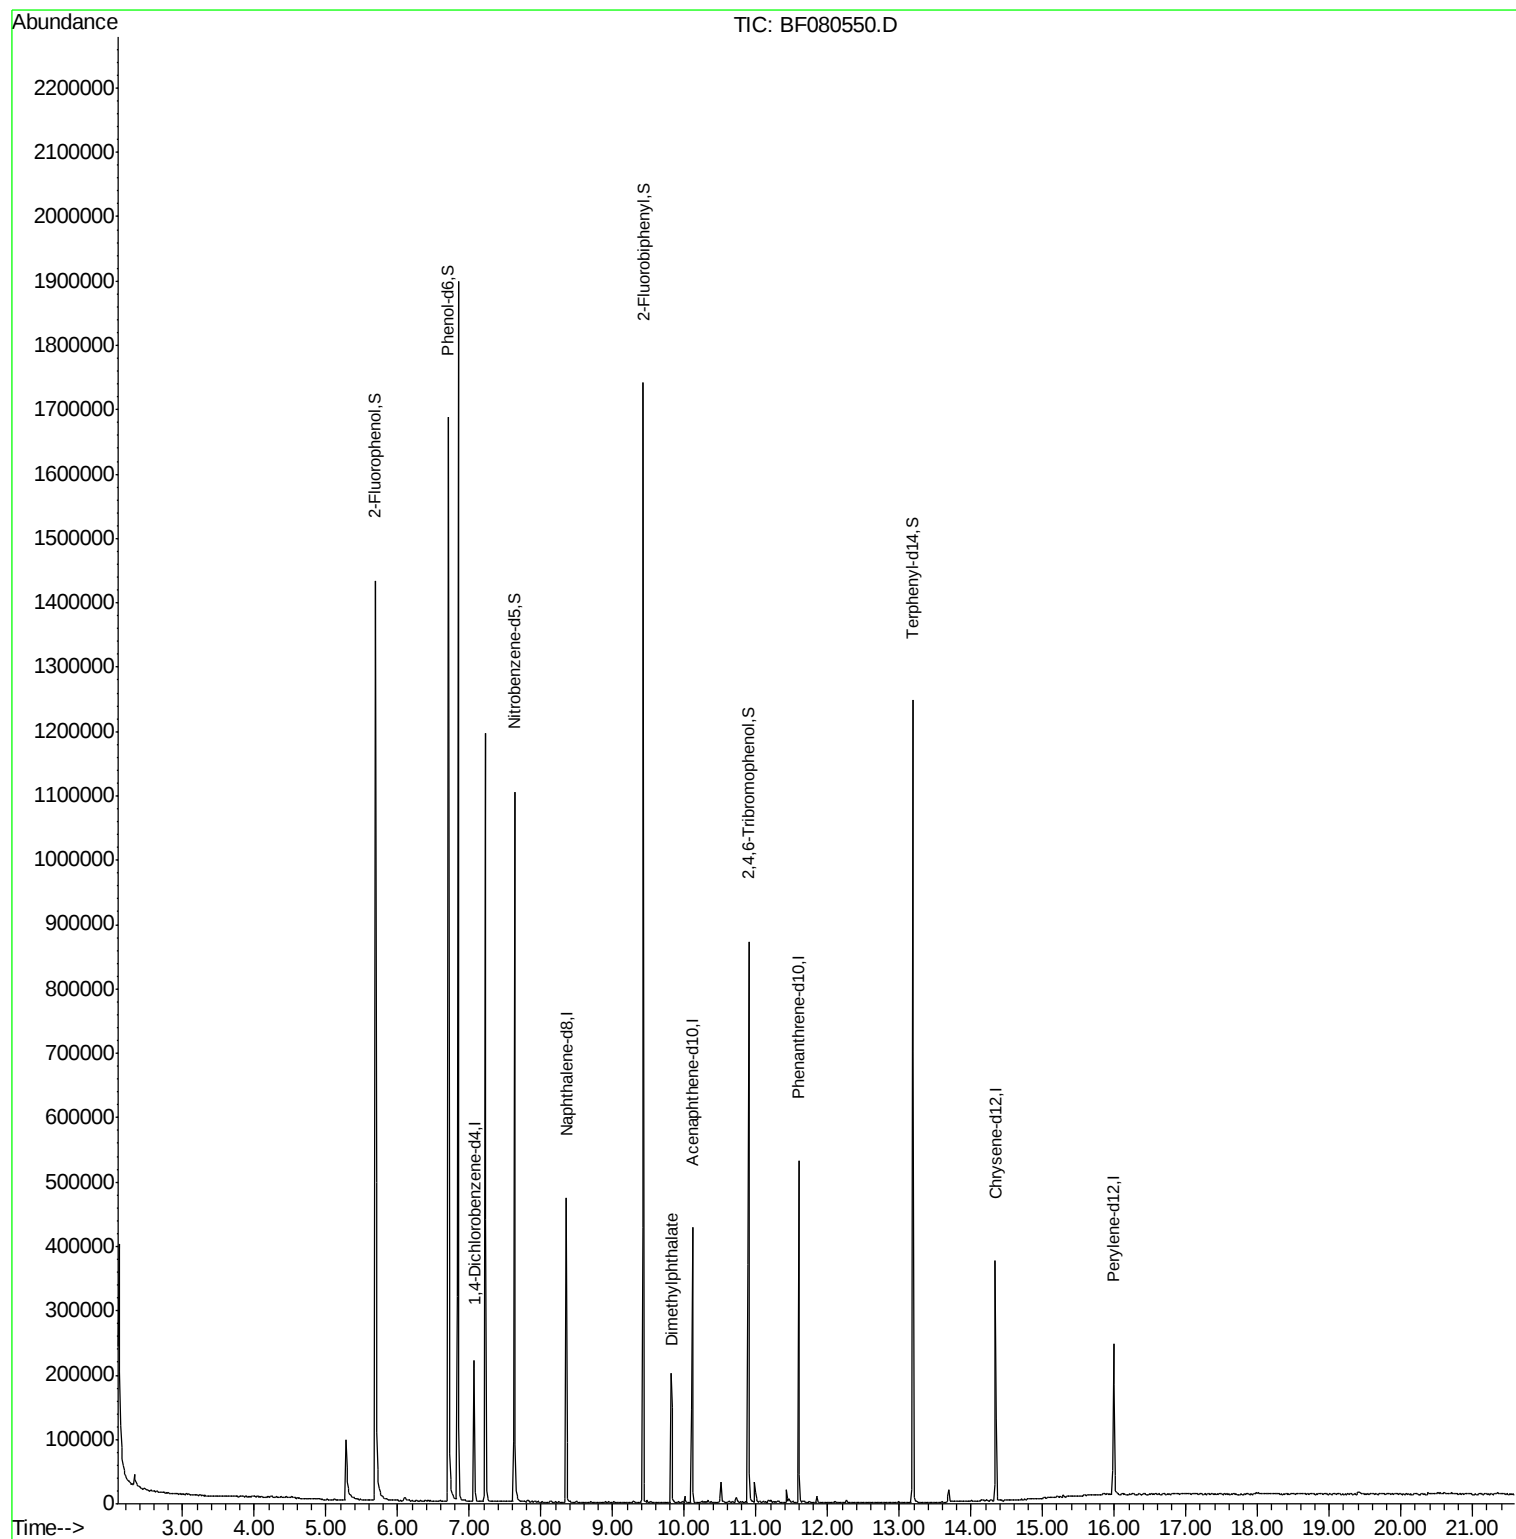

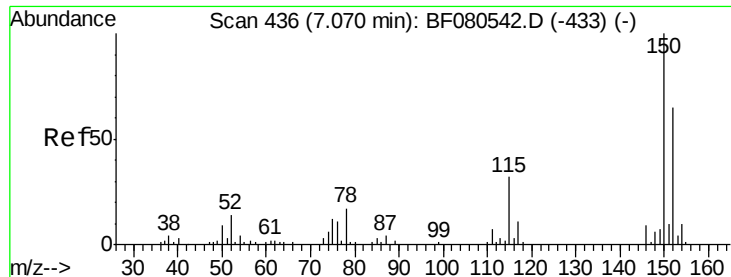


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.07 min Scan# 436
Delta R.T. -0.00 min
Lab File: BF080550.D
Acq: 17 Jul 2015 23:20

Instrument :
BNA_F
ClientSampleId :
SOUTH-EAST-WALL1-071415

Tgt Ion:152 Resp: 49735
Ion Ratio Lower Upper
152 100
150 151.9 123.0 184.4
115 50.5 39.9 59.9

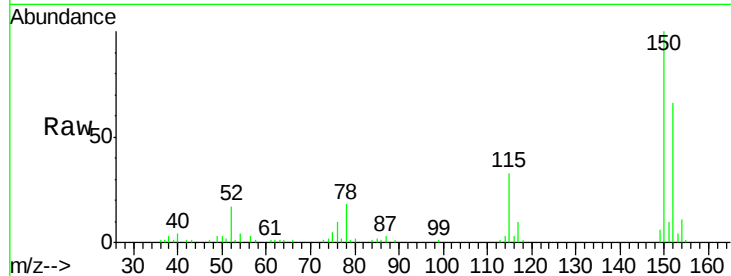


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

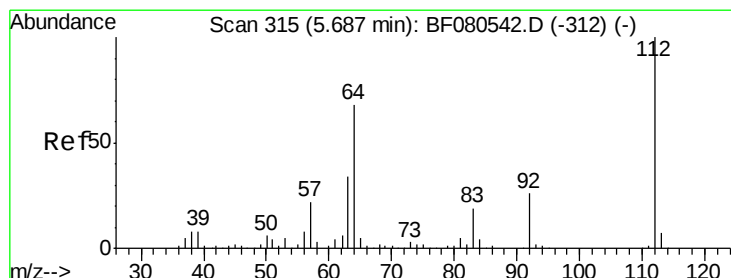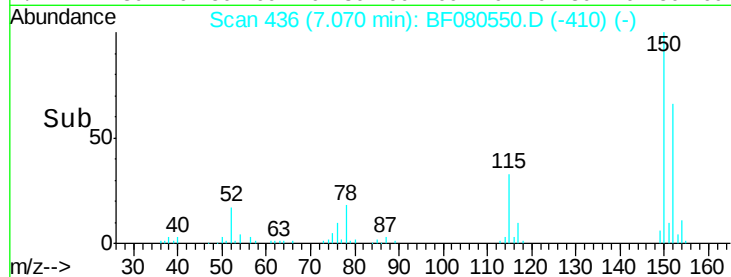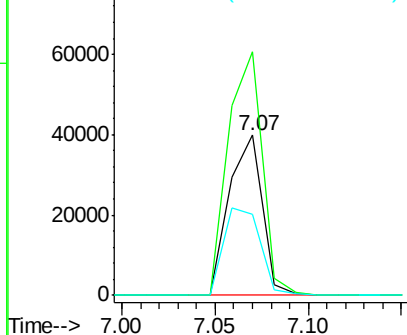



#5


2-Fluorophenol
Concen: 130.80 ng
RT: 5.69 min Scan# 315
Delta R.T. 0.00 min
Lab File: BF080550.D
Acq: 17 Jul 2015 23:20

Tgt Ion:112 Resp: 417235
Ion Ratio Lower Upper
112 100
64 66.2 54.1 81.1
63 35.4 27.6 41.4

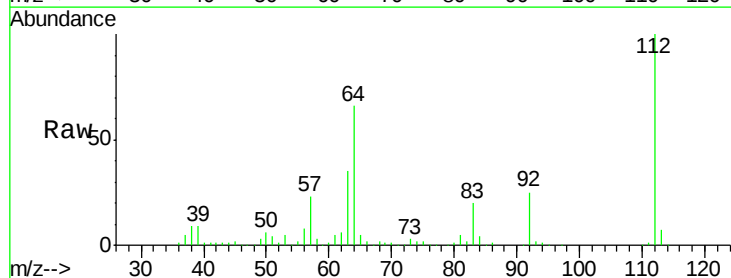

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

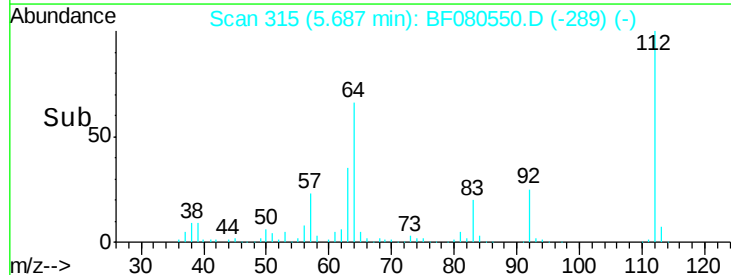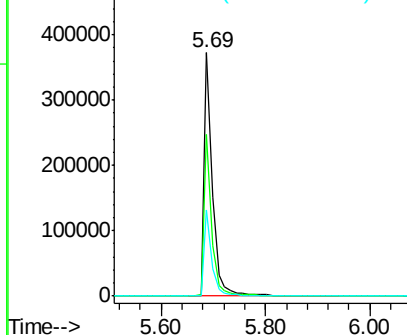

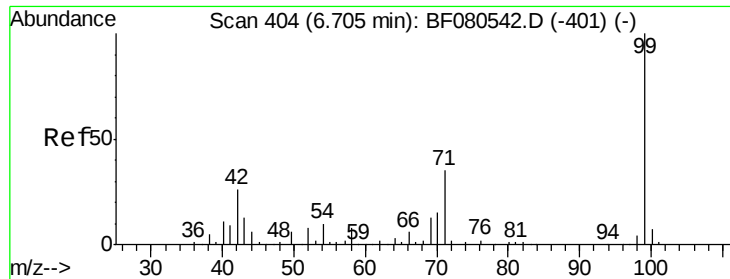

#7

Phenol-d6

Concen: 140.39 ng

RT: 6.70 min Scan# 404

Delta R.T. -0.00 min

Lab File: BF080550.D

Acq: 17 Jul 2015 23:20

Instrument :

BNA_F

ClientSampleId :

SOUTH-EAST-WALL1-071415


Tgt Ion: 99 Resp: 509644

Ion Ratio Lower Upper

99 100

42 25.3 21.0 31.4




71 35.0 28.4 42.6

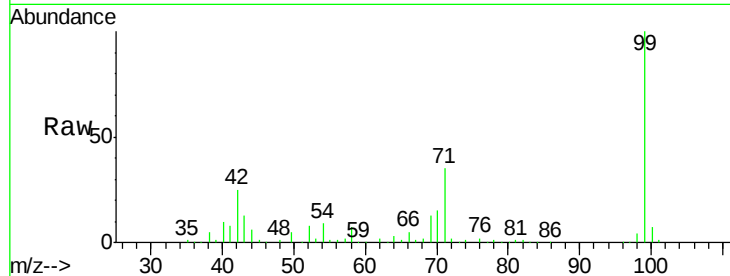

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

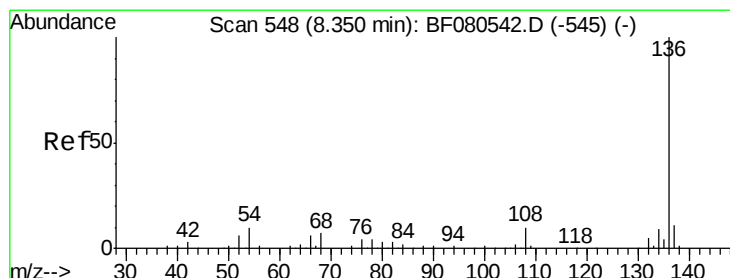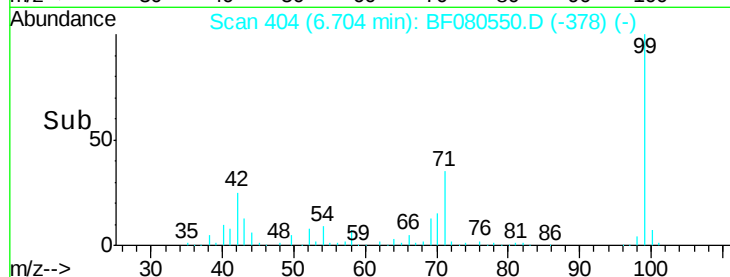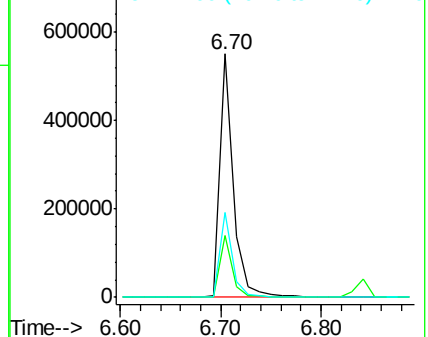

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.35 min Scan# 548

Delta R.T. -0.00 min

Lab File: BF080550.D

Acq: 17 Jul 2015 23:20

Tgt Ion: 136 Resp: 201247


Ion Ratio Lower Upper

136 100

137 11.3 8.7 13.1

54 9.9 8.3 12.5

68 5.9 5.4 8.2


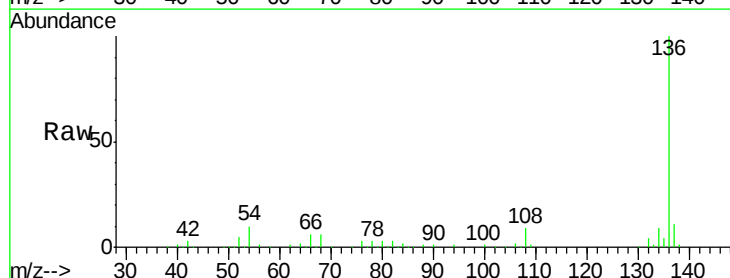



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

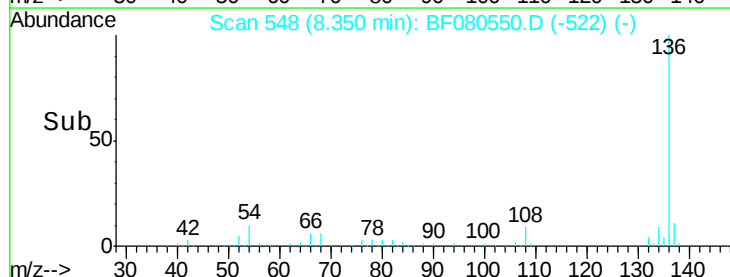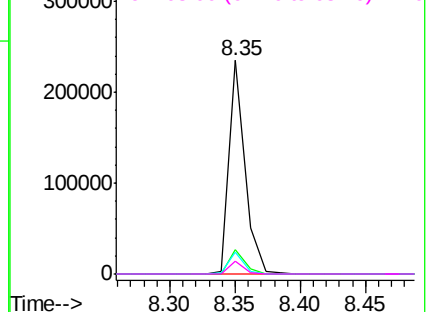


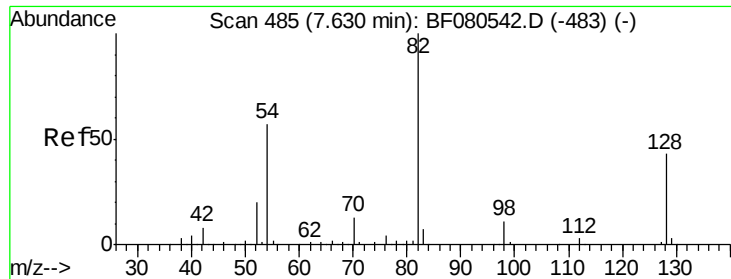




#23
 Nitrobenzene-d5
 Concen: 93.16 ng
 RT: 7.63 min Scan# 485
 Delta R.T. -0.00 min
 Lab File: BF080550.D
 Acq: 17 Jul 2015 23:20

Instrument :
 BNA_F
 ClientSampleId :
 SOUTH-EAST-WALL1-071415

Tgt Ion: 82 Resp: 294057
 Ion Ratio Lower Upper
 82 100
 128 46.1 34.6 51.8
 54 57.8 45.8 68.6

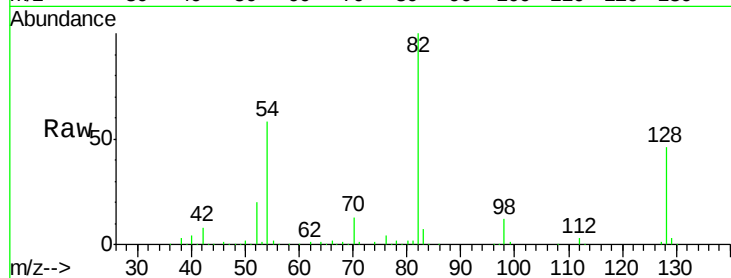


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

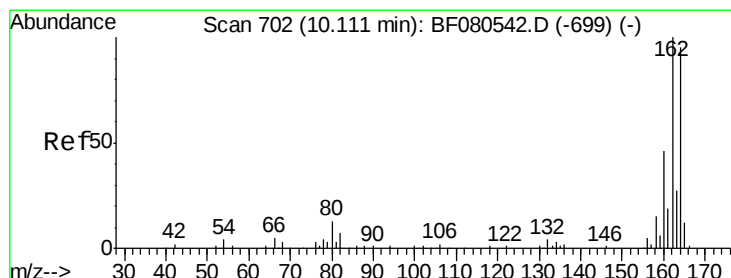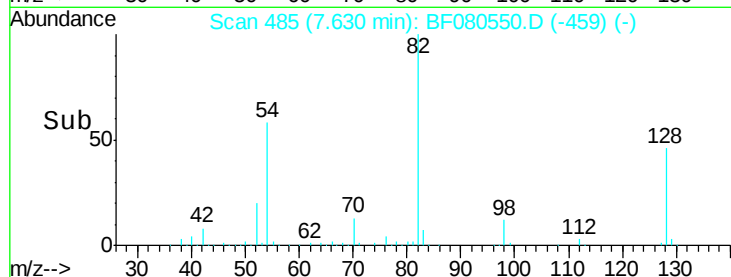
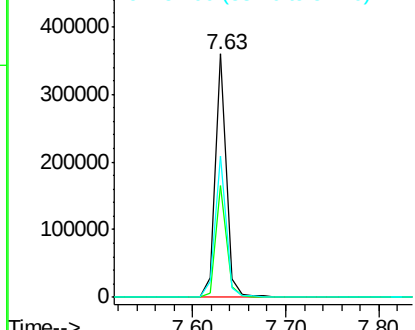



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.11 min Scan# 702
 Delta R.T. -0.00 min
 Lab File: BF080550.D
 Acq: 17 Jul 2015 23:20

Tgt Ion: 164 Resp: 85873
 Ion Ratio Lower Upper
 164 100
 162 107.1 84.1 126.1
 160 48.9 38.8 58.2

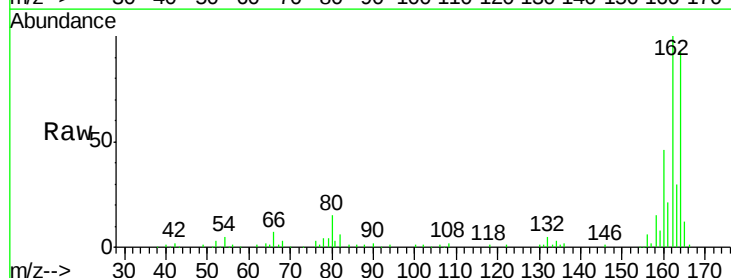

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

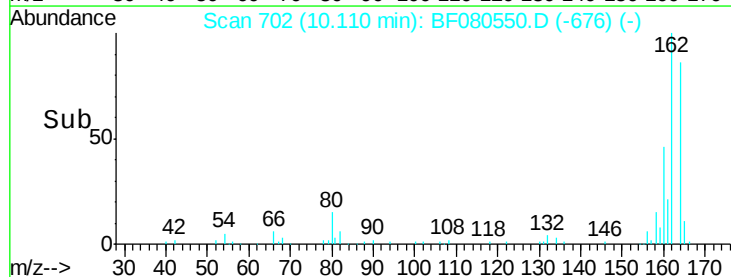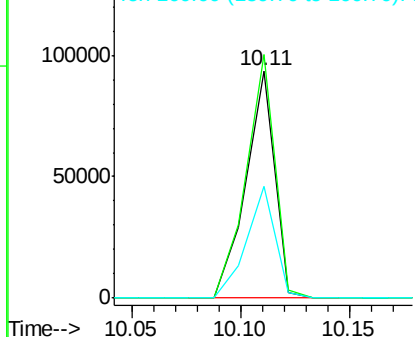


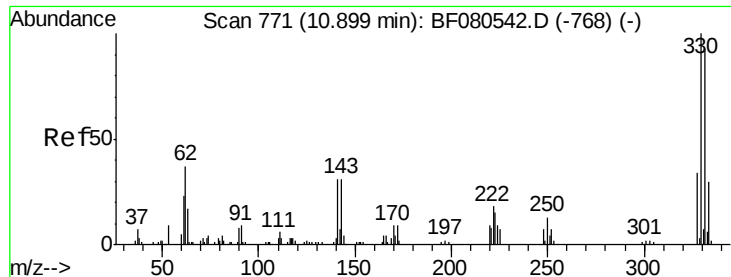




#41
 2,4,6-Tribromophenol
 Concen: 147.27 ng
 RT: 10.90 min Scan# 771
 Delta R.T. -0.00 min
 Lab File: BF080550.D
 Acq: 17 Jul 2015 23:20

Instrument :
 BNA_F
 ClientSampleId :
 SOUTH-EAST-WALL1-071415

Tgt Ion:330 Resp: 113164
 Ion Ratio Lower Upper
 330 100
 332 93.6 74.3 111.5
 141 34.9 29.0 43.4

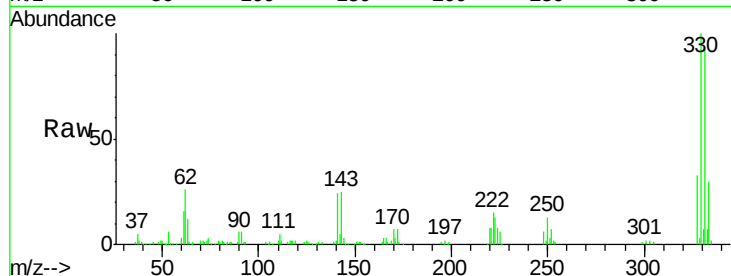


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

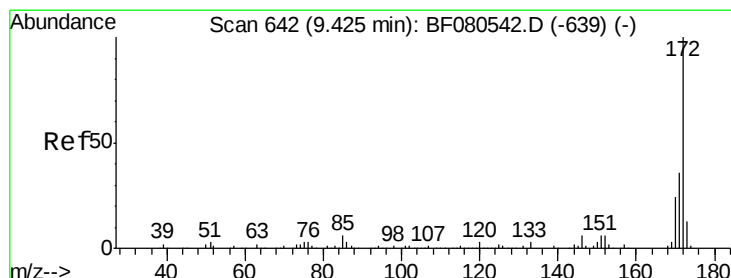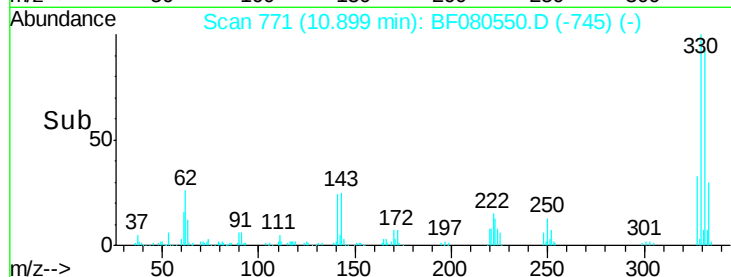
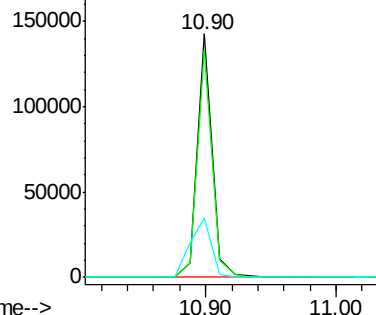



#44
 2-Fluorobiphenyl
 Concen: 86.11 ng
 RT: 9.42 min Scan# 642
 Delta R.T. -0.00 min
 Lab File: BF080550.D
 Acq: 17 Jul 2015 23:20

Tgt Ion:172 Resp: 526458
 Ion Ratio Lower Upper
 172 100
 171 35.9 28.8 43.2
 170 24.0 19.0 28.4

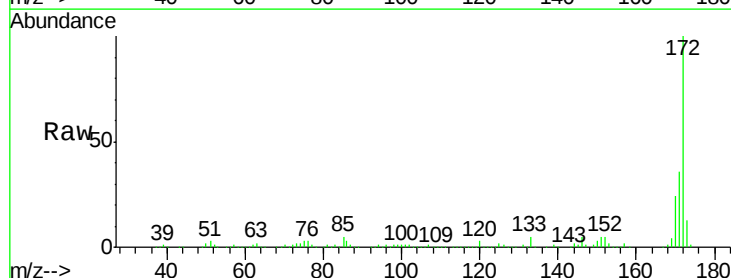

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

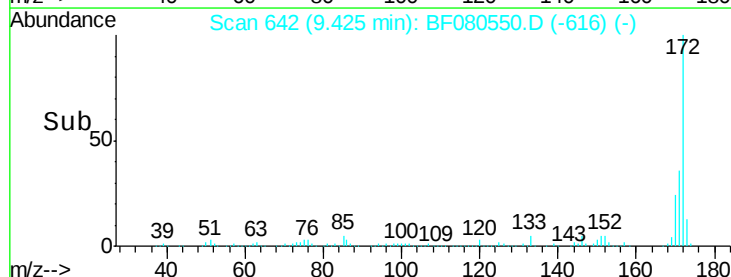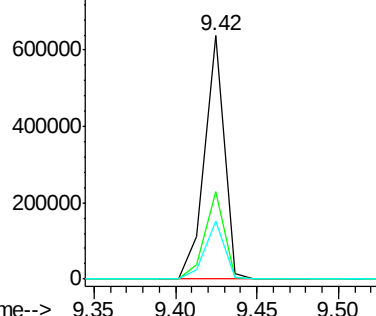

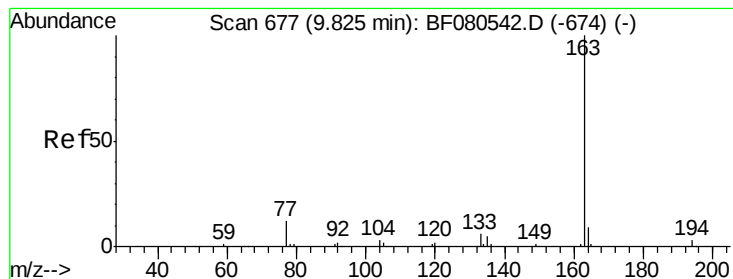

#49

Dimethylphthalate

Concen: 19.24 ng

RT: 9.82 min Scan# 677

Delta R.T. -0.00 min

Lab File: BF080550.D

Acq: 17 Jul 2015 23:20

Instrument :

BNA_F

ClientSampleId :

SOUTH-EAST-WALL1-071415


Tgt Ion:163 Resp: 109964

Ion Ratio Lower Upper

163 100

194 4.0 2.7 4.1




164 8.8 7.4 11.2

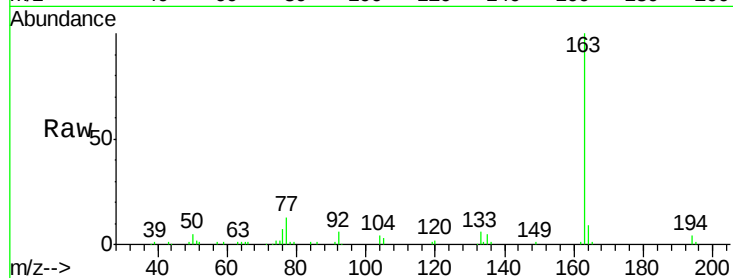

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

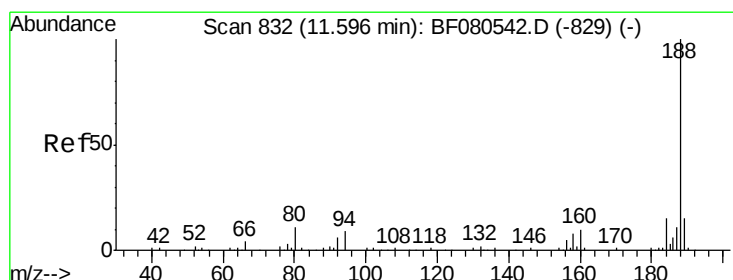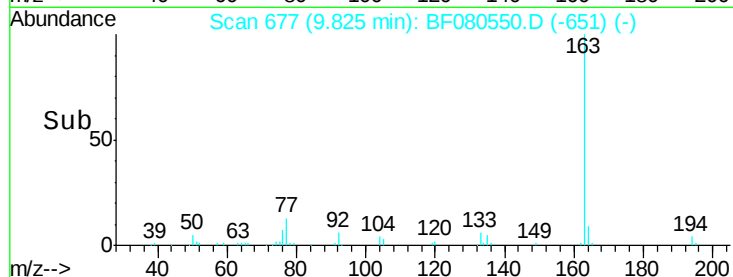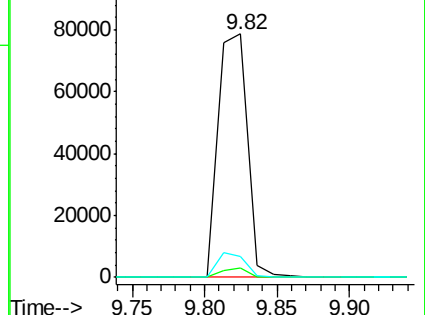

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.60 min Scan# 832

Delta R.T. -0.00 min

Lab File: BF080550.D

Acq: 17 Jul 2015 23:20


Tgt Ion:188 Resp: 177540

Ion Ratio Lower Upper

188 100

94 9.1 7.6 11.4



80 9.4 8.6 12.8

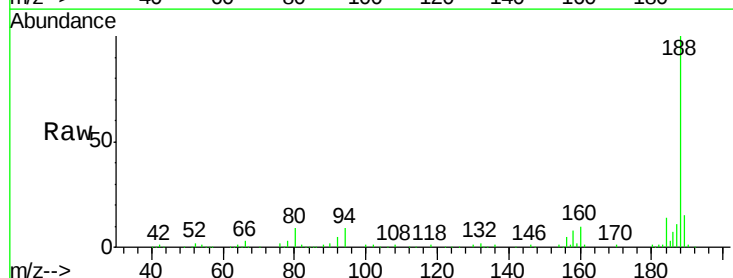


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

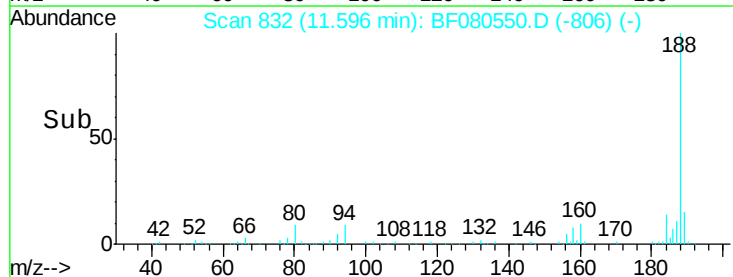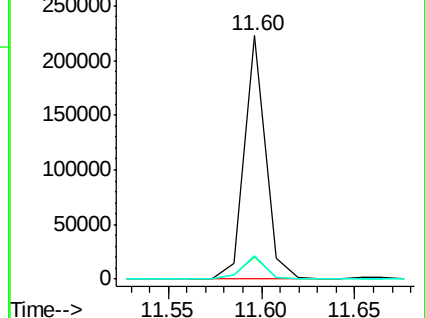

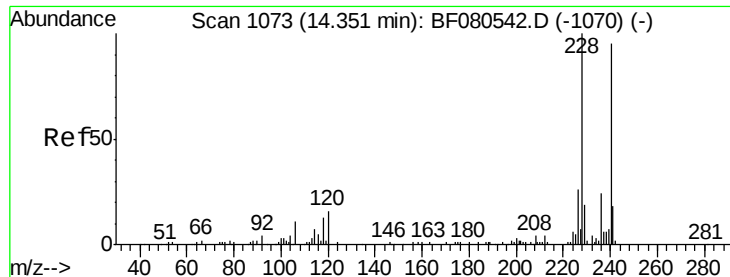

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.34 min Scan# 1072

Delta R.T. -0.01 min

Lab File: BF080550.D

Acq: 17 Jul 2015 23:20

Instrument :

BNA_F

ClientSampleId :

SOUTH-EAST-WALL1-071415


Tgt Ion:240 Resp: 141045

Ion Ratio Lower Upper

240 100

120 13.3 13.6 20.4#




236 25.4 20.2 30.4

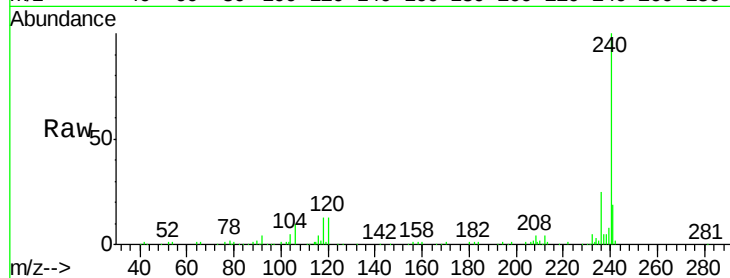

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

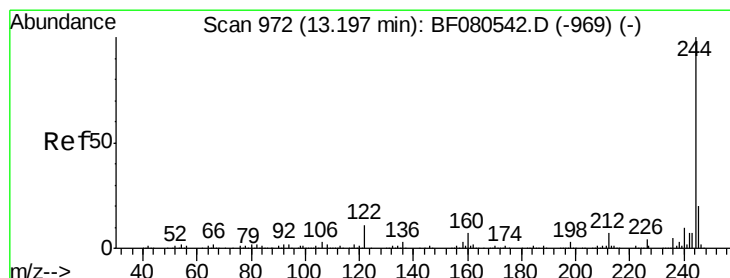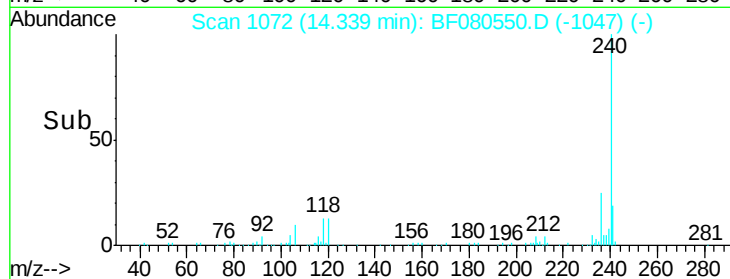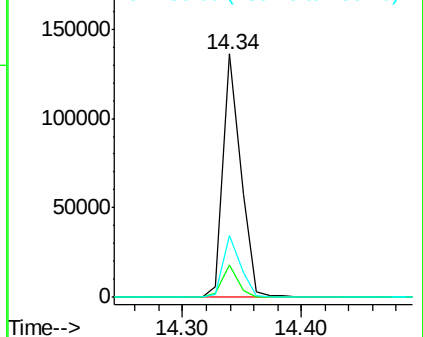

#78

Terphenyl-d14

Concen: 72.87 ng

RT: 13.19 min Scan# 971

Delta R.T. -0.01 min

Lab File: BF080550.D

Acq: 17 Jul 2015 23:20


Tgt Ion:244 Resp: 460266

Ion Ratio Lower Upper

244 100

212 7.6 5.5 8.3



122 18.8 9.0 13.4#

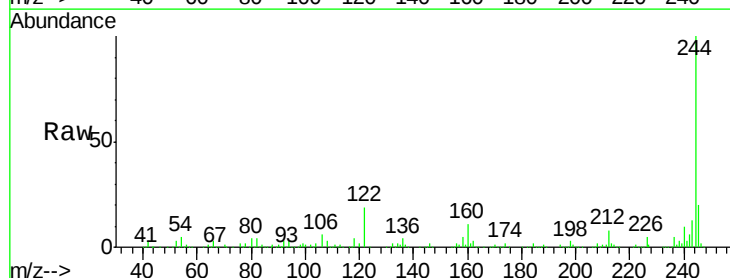


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

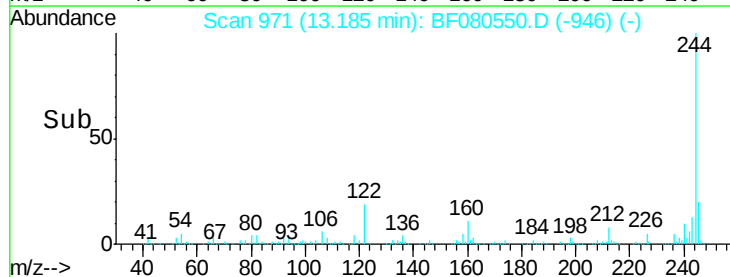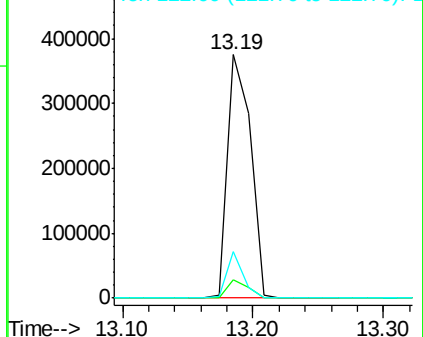

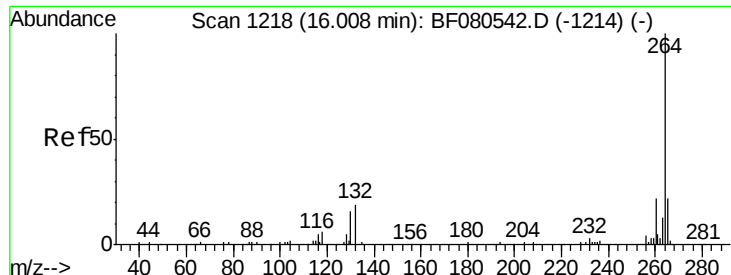

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.99 min Scan# 1216
Delta R.T. -0.02 min
Lab File: BF080550.D
Acq: 17 Jul 2015 23:20

Instrument :
BNA_F
ClientSampleId :
SOUTH-EAST-WALL1-071415

Tgt Ion: 264 Resp: 126998
Ion Ratio Lower Upper
264 100
260 23.8 17.8 26.8
265 22.3 17.2 25.8

