
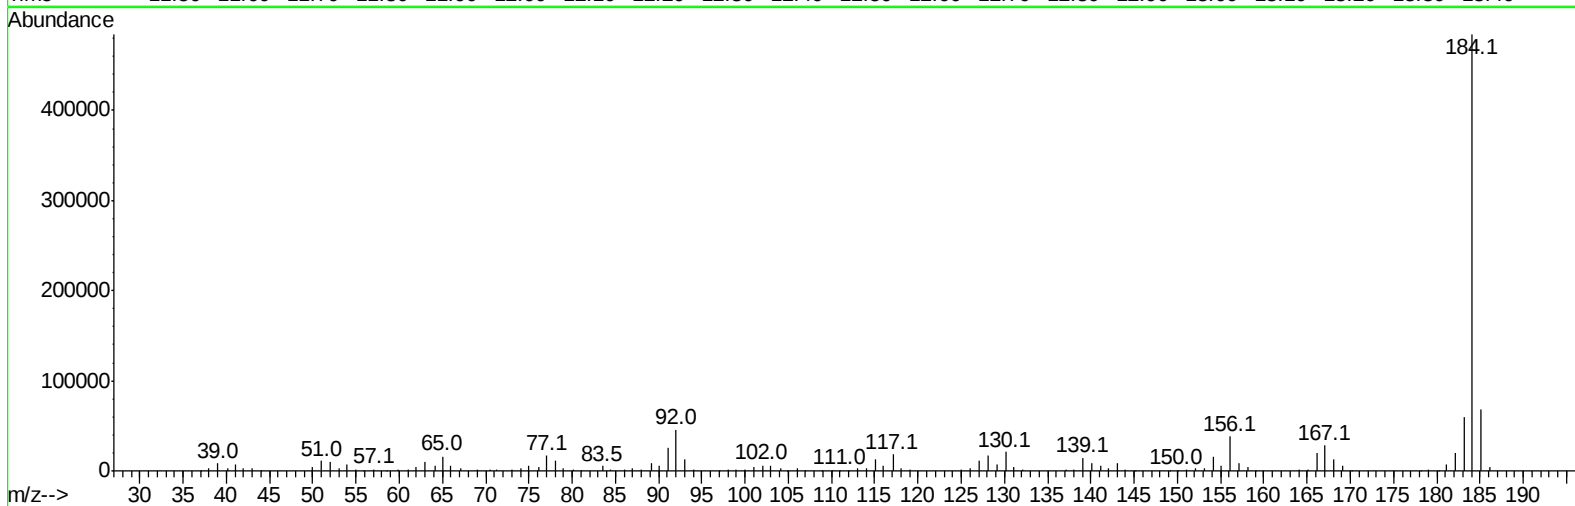


Data Path : Z:\HPCHEM1\BNA F\DATA\BF071717\
Data File : BF096809.D
Acq On : 17 Jul 2017 10:21
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 05:06:41 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 13 14:49:34 2017
Response via : Initial Calibration

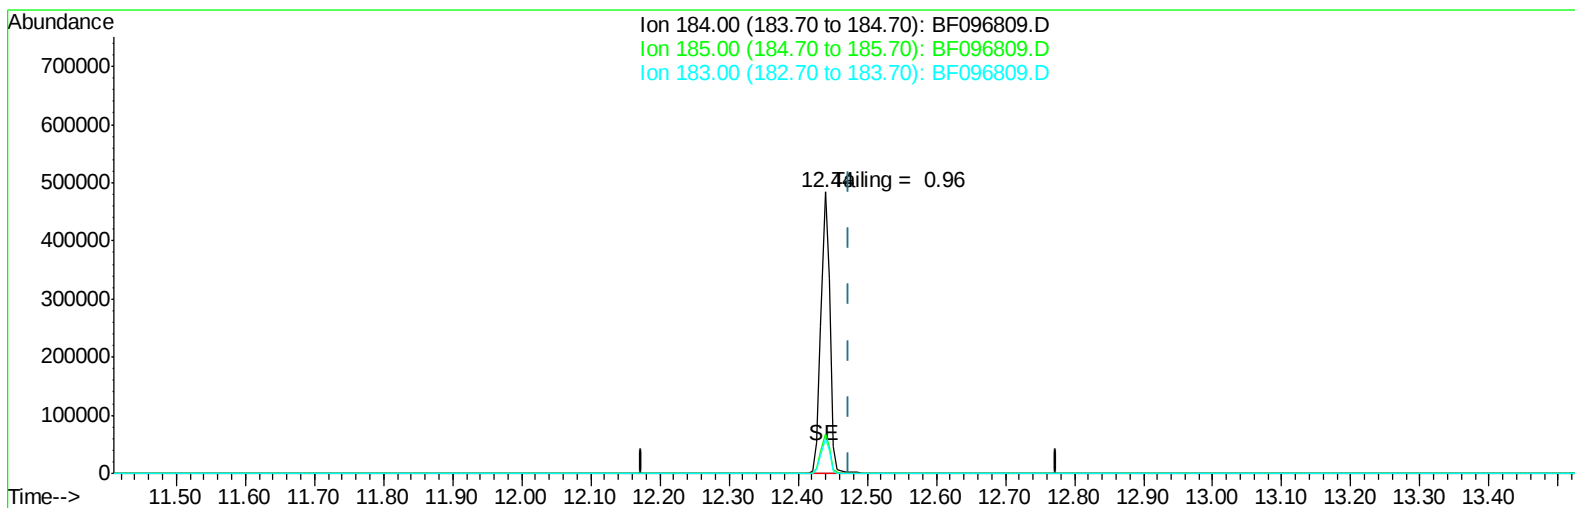

TIC: BF096809.D

(76) Benzidine



12.439min (-0.036) 0.00ng

response 422884

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.19#
183.00	12.20	12.23
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF071717\
Data File : BF096809.D
Acq On : 17 Jul 2017 10:21
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 05:06:41 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 13 14:49:34 2017
Response via : Initial Calibration

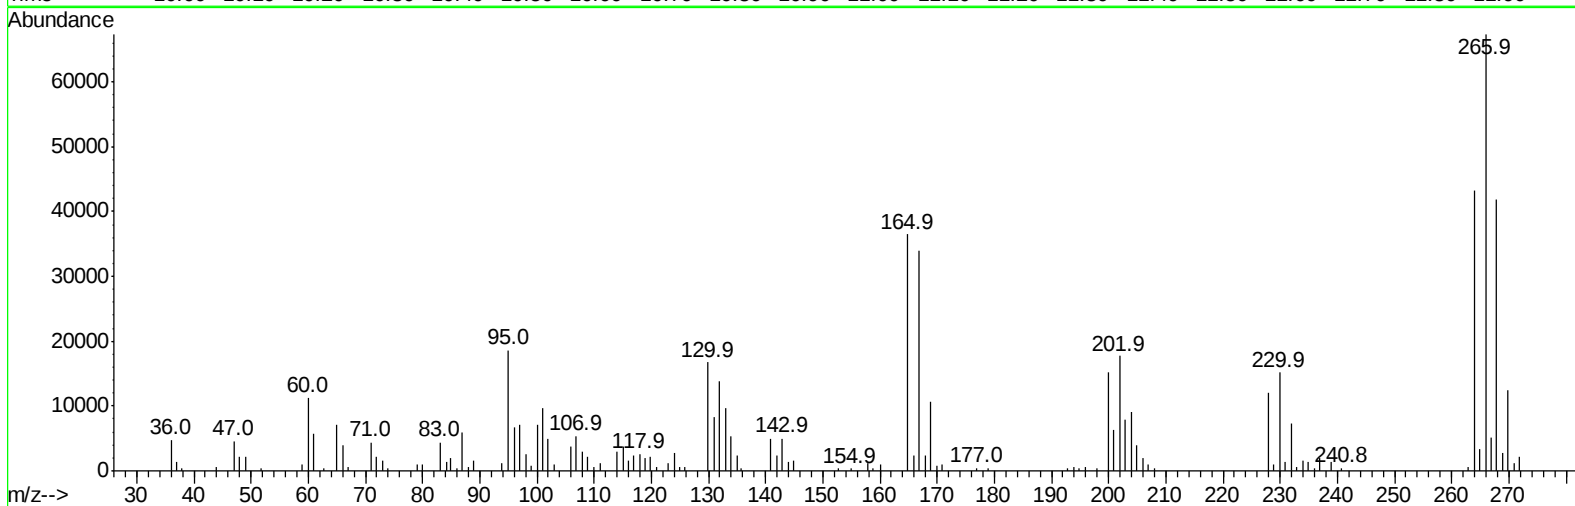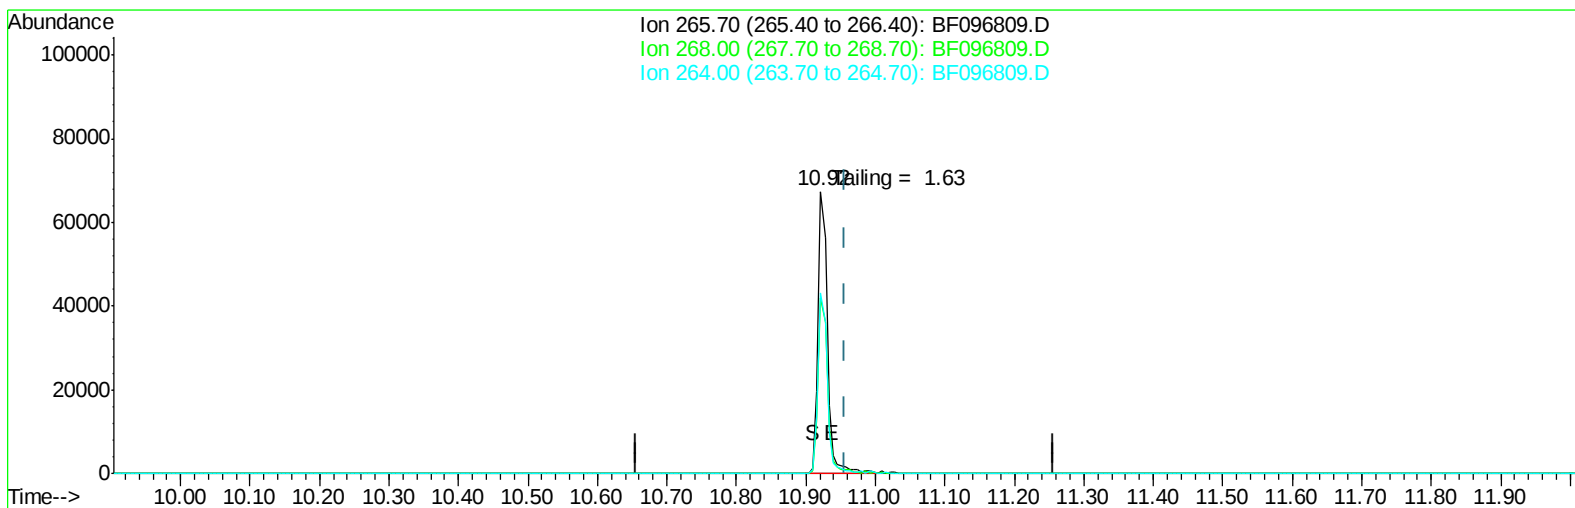

TIC: BF096809.D

(69) Pentachlorophenol (C)

10.921min (-0.036) 41430.65ng

response 61222

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.30
264.00	64.60	64.15
0.00	0.00	0.00