


Data Path : Z:\HPCHEM1\BNA F\Data\BF071717\
 Data File : BF096809.D
 Acq On : 17 Jul 2017 10:21
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 18 13:33:22 2017

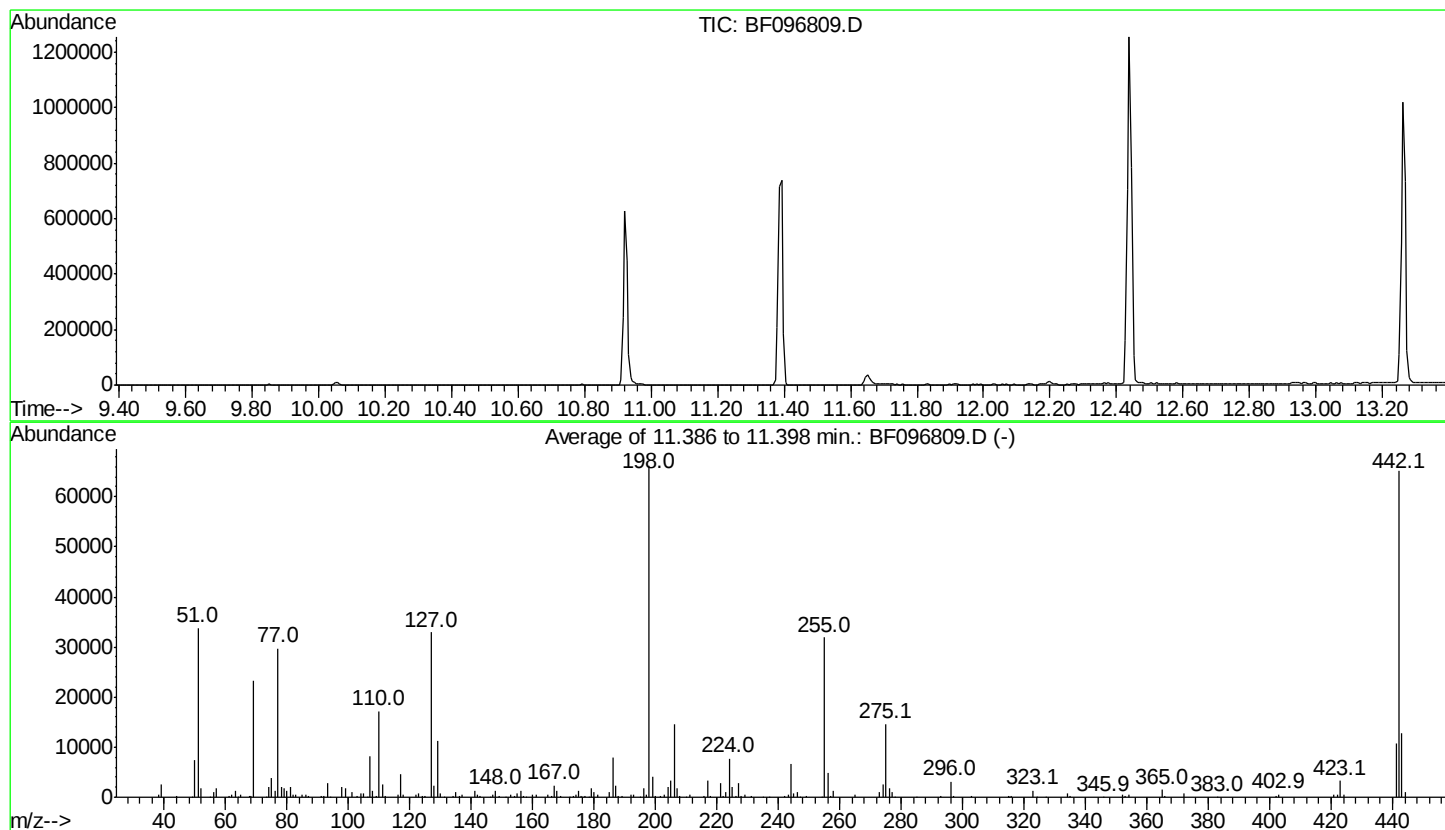

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.0	33742	PASS
68	69	0.00	2	1.0	240	PASS
69	198	0.00	100	35.0	23165	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.7	32934	PASS
197	198	0.00	2	0.9	614	PASS
198	198	100	100	100.0	66216	PASS
199	198	5	9	6.3	4198	PASS
275	198	10	60	22.2	14678	PASS
365	198	1	100	2.2	1434	PASS
441	442	0.01	24	16.5	10769	PASS
442	198	50	100	98.6	65314	PASS
443	442	15	24	19.6	12770	PASS