


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071718\
Data File : BF107436.D
Acq On : 17 Jul 2018 9:10
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071618.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 17 11:29:08 2018

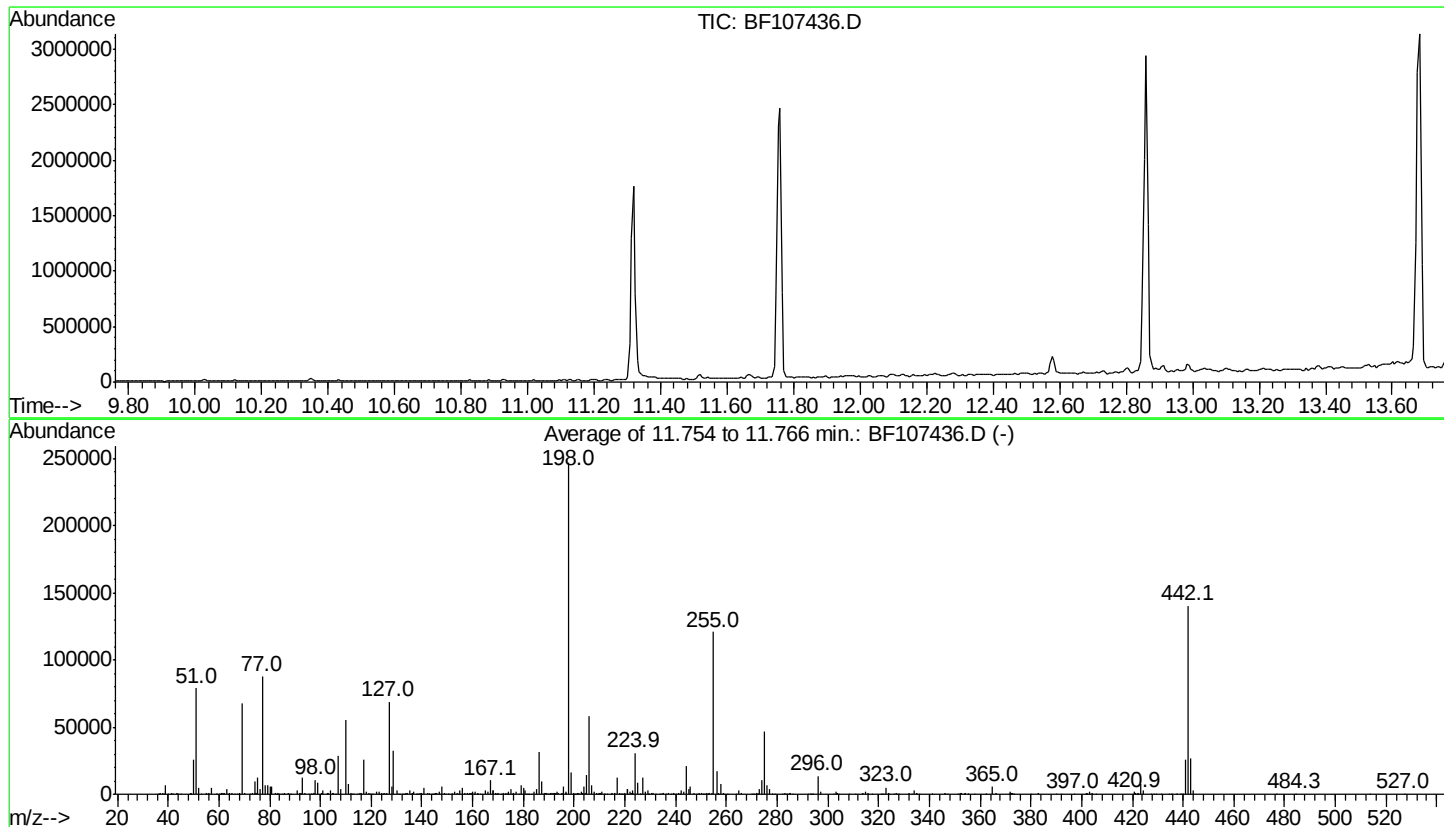

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	78994	PASS
68	69	0.00	2	2.0	1343	PASS
69	198	0.00	100	27.6	68075	PASS
70	69	0.00	2	1.3	864	PASS
127	198	10	80	27.9	68912	PASS
197	198	0.00	2	0.7	1625	PASS
198	198	100	100	100.0	246834	PASS
199	198	5	9	6.7	16571	PASS
275	198	10	60	18.8	46418	PASS
365	198	1	100	2.2	5353	PASS
441	198	0.01	100	10.4	25616	PASS
442	198	50	100	56.9	140554	PASS
443	442	15	24	19.3	27120	PASS