
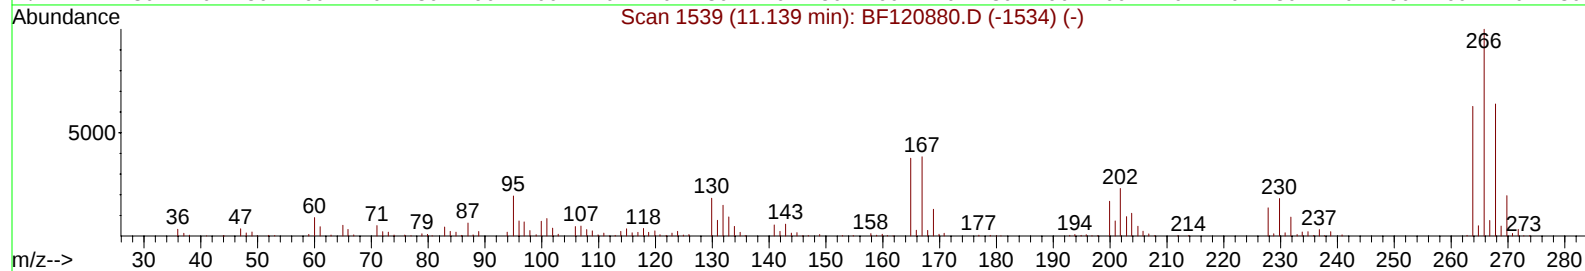
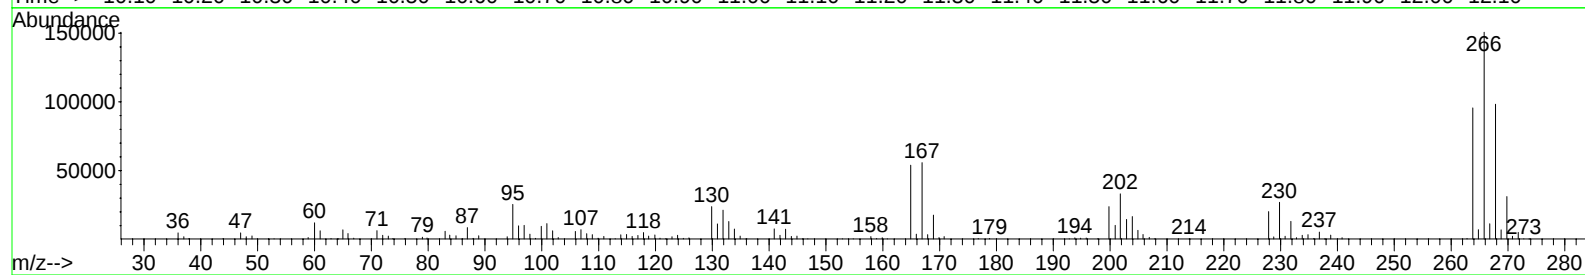


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071720\
 Data File : BF120910.D
 Acq On : 17 Jul 2020 8:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 17 13:23:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 16 14:20:32 2020
 Response via : Initial Calibration

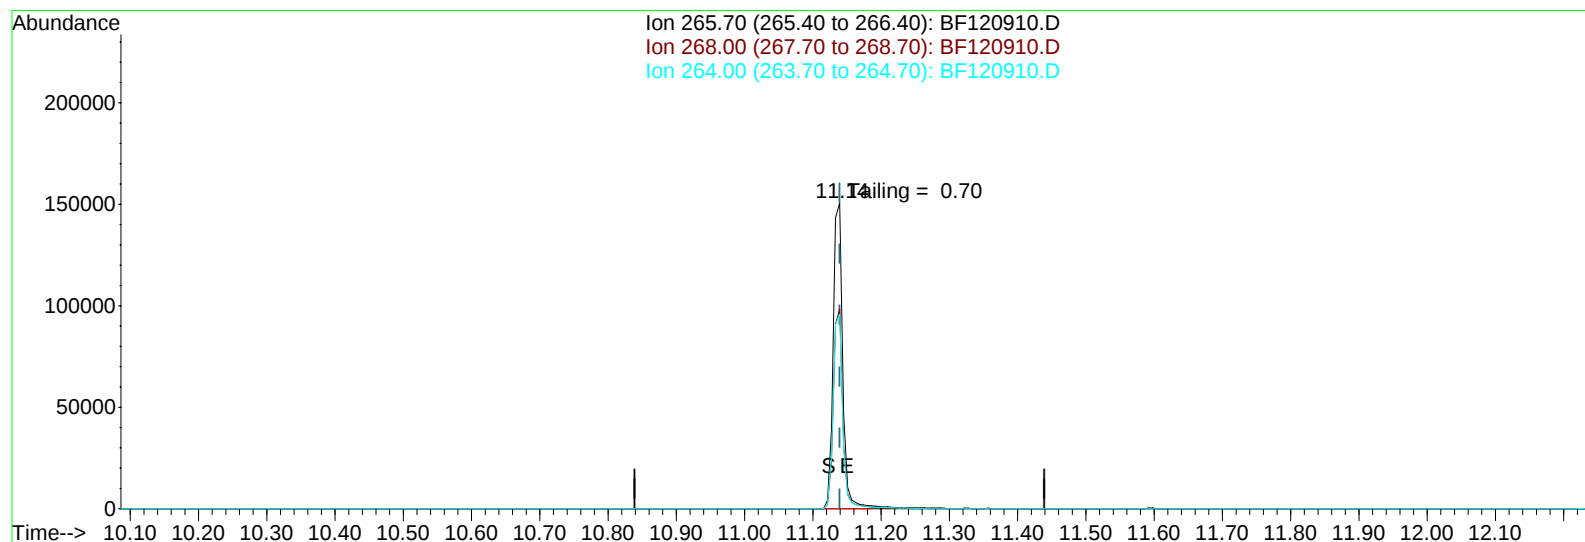

TIC: BF120910.D

(70) Pentachlorophenol (C)




11.139min (+0.000) 165758.36ng

response 146595

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.23
264.00	62.70	63.50
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071720\
 Data File : BF120910.D
 Acq On : 17 Jul 2020 8:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 17 13:23:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 16 14:20:32 2020
 Response via : Initial Calibration

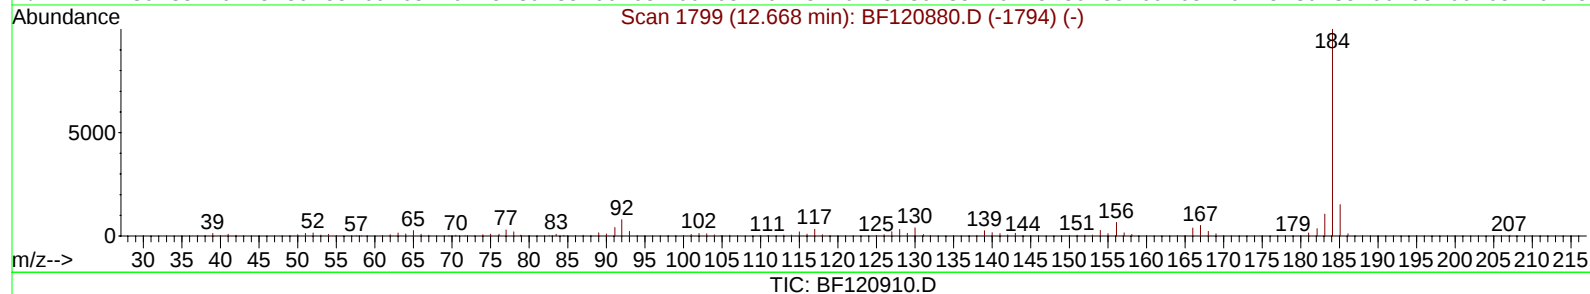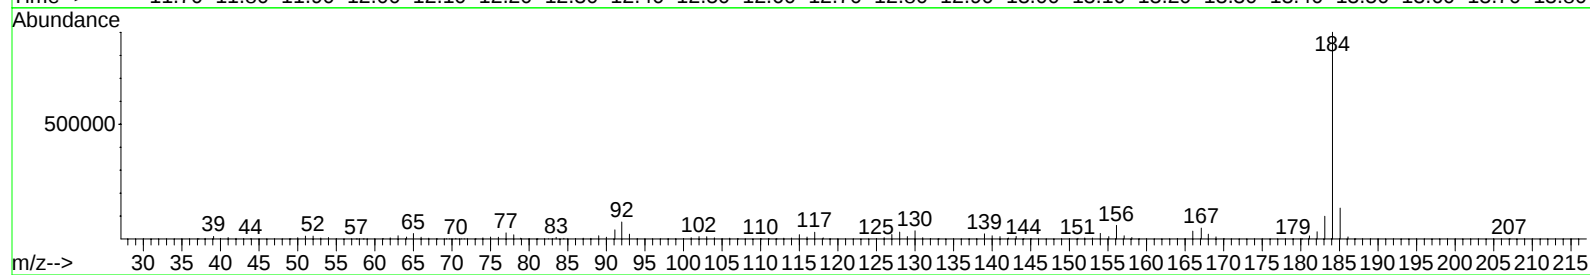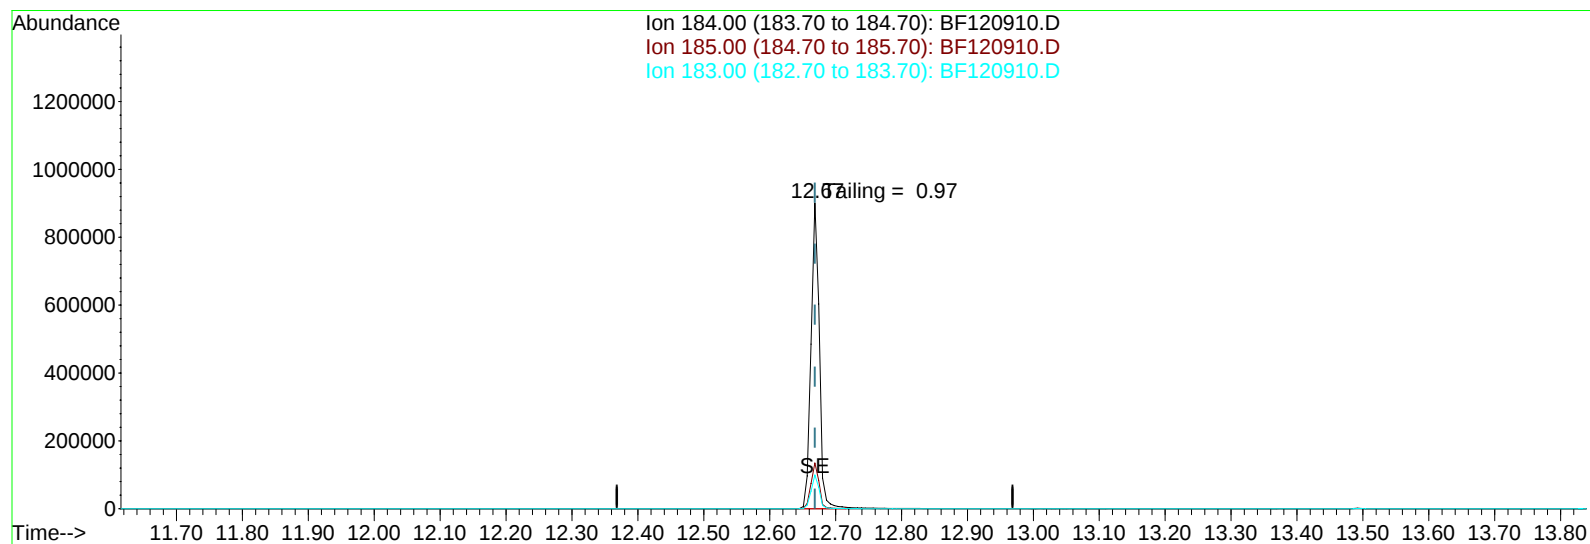

(77) Benzidine

12.669min (+0.000) 78316.64ng

response 805102

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.95
183.00	10.60	11.05
0.00	0.00	0.00