

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071720\
 Data File : BF120913.D
 Acq On : 17 Jul 2020 10:22
 Operator : JU/CG
 Sample : PB130249BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB130249BL

Quant Time: Jul 17 10:53:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 16 14:20:32 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	178697	20.00	ng	0.00
21) Naphthalene-d8	8.10	136	673762	20.00	ng	0.00
39) Acenaphthene-d10	9.85	164	342111	20.00	ng	0.00
64) Phenanthrene-d10	11.33	188	648068	20.00	ng	0.00
76) Chrysene-d12	13.97	240	517353	20.00	ng	0.00
86) Perylene-d12	15.42	264	475786	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.43	112	1187513	108.94	ng	0.01
7) Phenol-d6	6.45	99	1421990	100.99	ng	0.00
23) Nitrobenzene-d5	7.37	82	903372	77.58	ng	0.00
42) 2,4,6-Tribromophenol	10.64	330	398315	106.37	ng	0.00
45) 2-Fluorobiphenyl	9.17	172	1586664	69.25	ng	0.00
79) Terphenyl-d14	12.92	244	1573852	66.13	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071720\
Data File : BF120913.D
Acq On : 17 Jul 2020 10:22
Operator : JU/CG
Sample : PB130249BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130249BL

Quant Time: Jul 17 10:53:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 16 14:20:32 2020
Response via : Initial Calibration

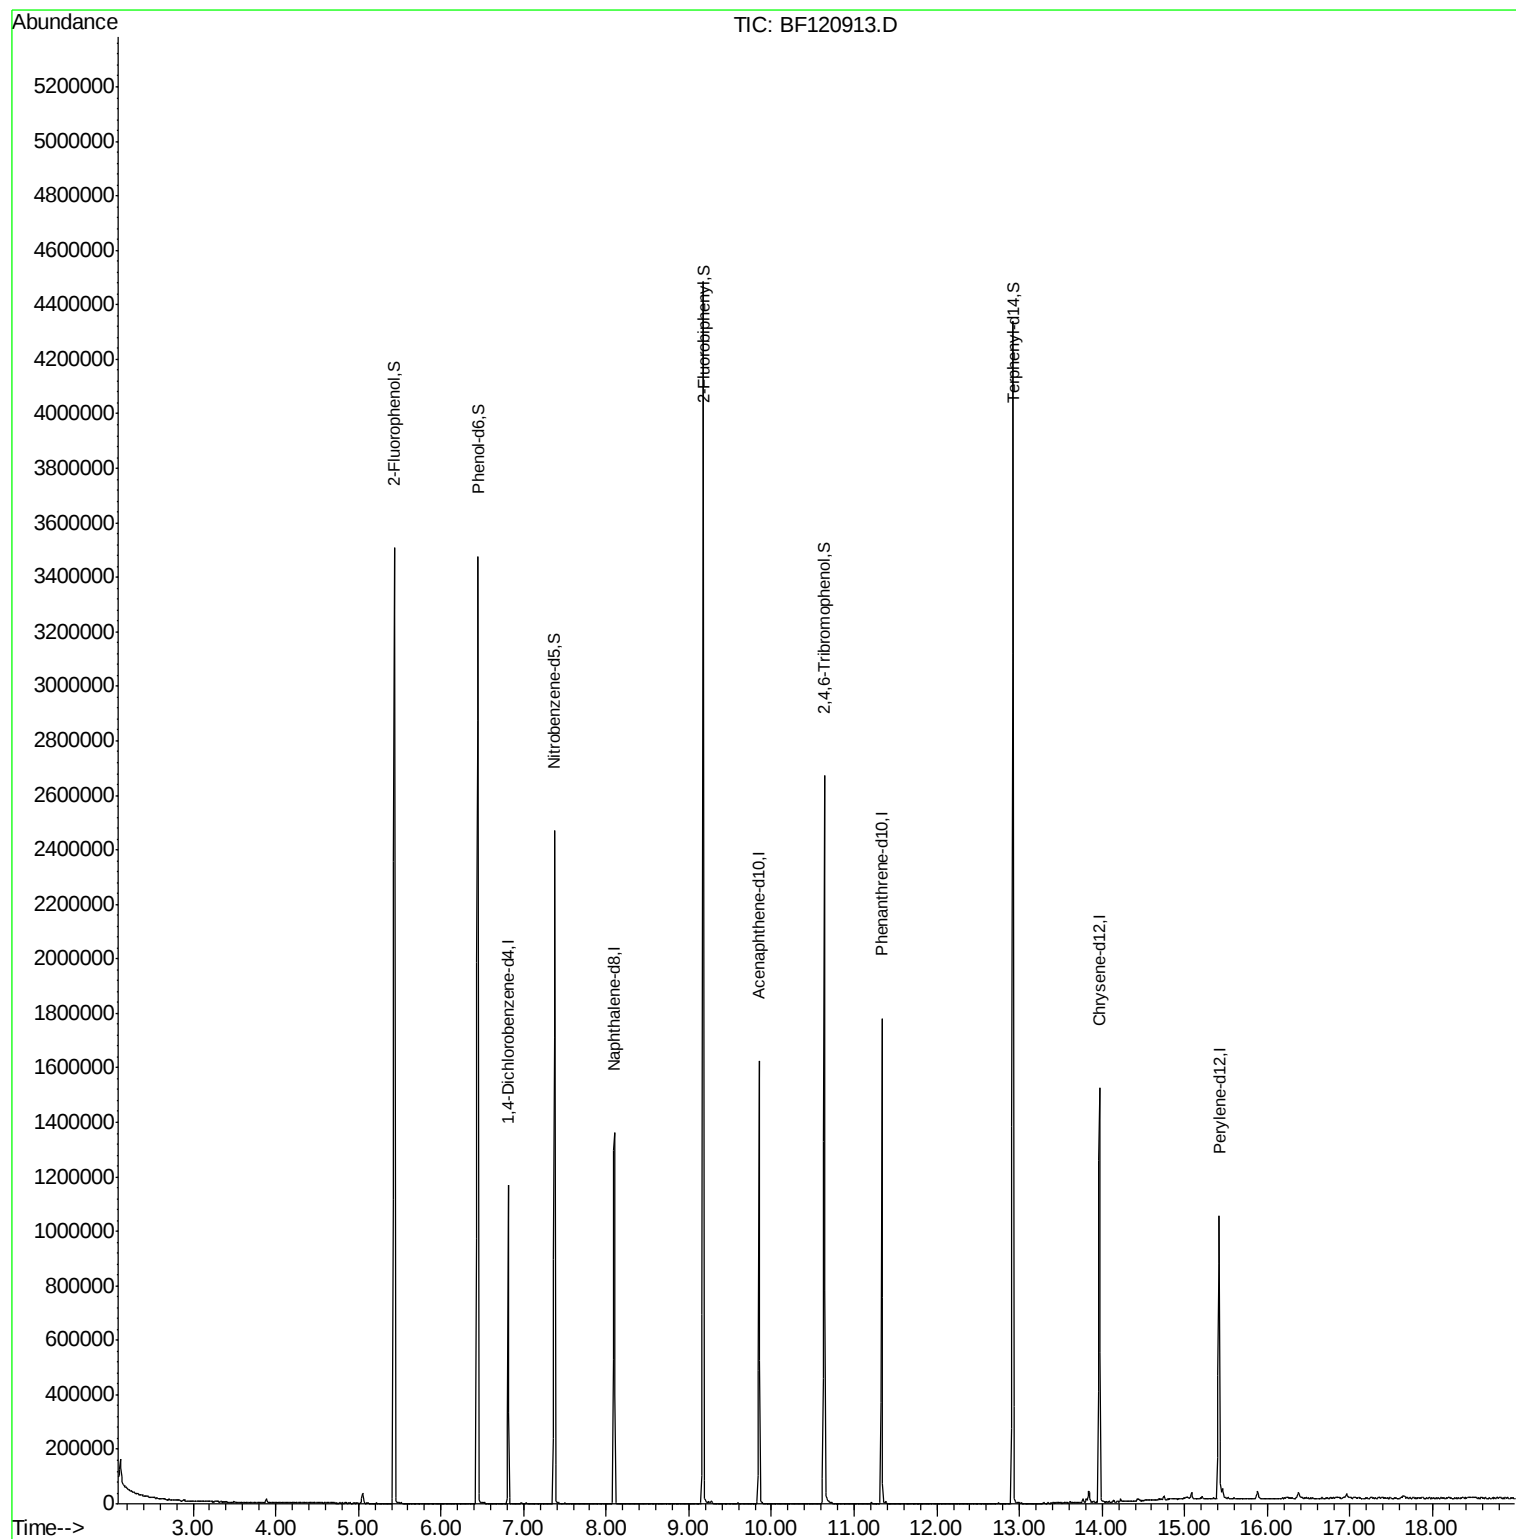

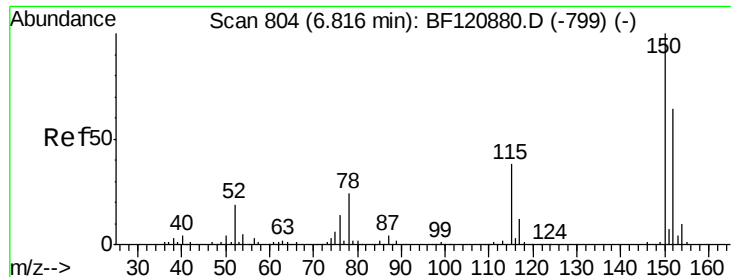

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 6.82 min Scan# 804

Delta R.T. 0.00 min

Lab File: BF120913.D

Acq: 17 Jul 2020 10:22

Instrument :

BNA_F

ClientSampleId :

PB130249BL


Tot Ion:152 Resp: 178697

Ion Ratio Lower Upper

152 100

150 156.1 125.0 187.6




115 56.5 47.0 70.4

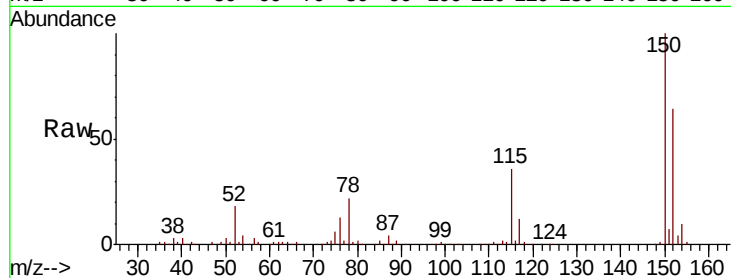

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

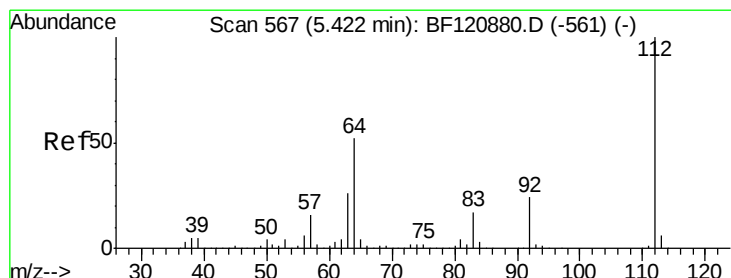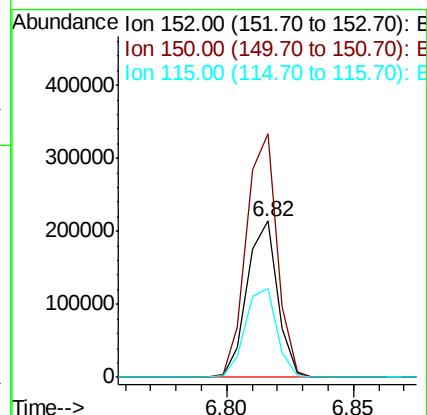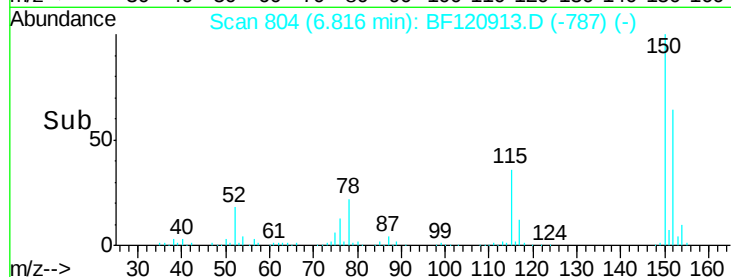

#5

2-Fluorophenol

Concen: 108.942 ng

RT: 5.43 min Scan# 569

Delta R.T. 0.01 min

Lab File: BF120913.D

Acq: 17 Jul 2020 10:22


Tgt Ion:112 Resp: 1187513

Ion Ratio Lower Upper

112 100

64 55.6 41.3 61.9



63 28.0 21.1 31.7

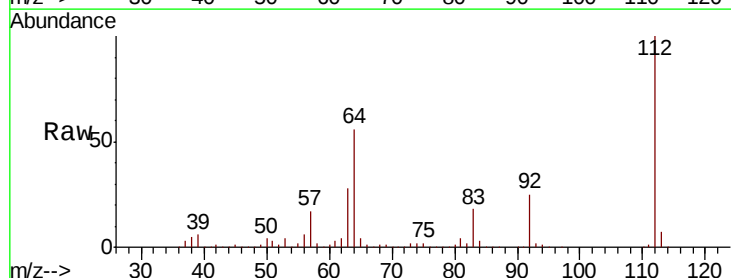

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

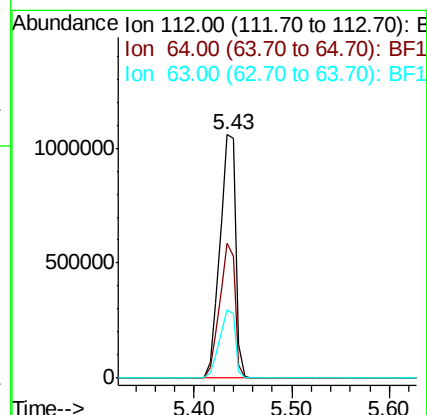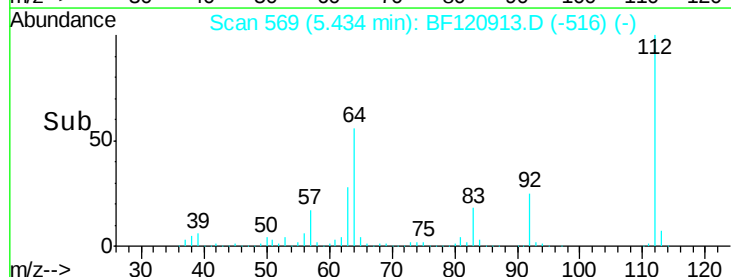



#7

Phenol-d6

Concen: 100.989 ng

RT: 6.45 min Scan# 741

Delta R.T. 0.00 min

Lab File: BF120913.D

Acq: 17 Jul 2020 10:22

Instrument :


BNA_F

ClientSampleId :

PB130249BL

Tot Ion: 99 Resp: 1421990

Ion	Ratio	Lower	Upper
99	100		
42	17.1	13.1	19.7
71	31.5	24.2	36.4



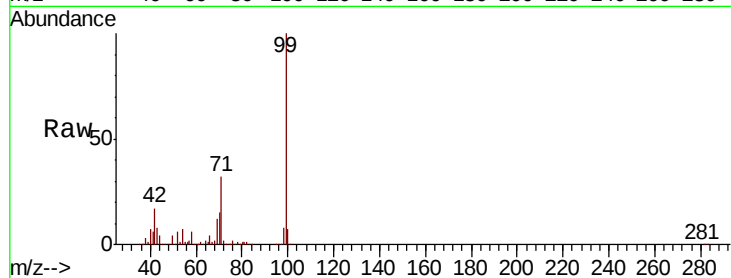


Abundance

Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

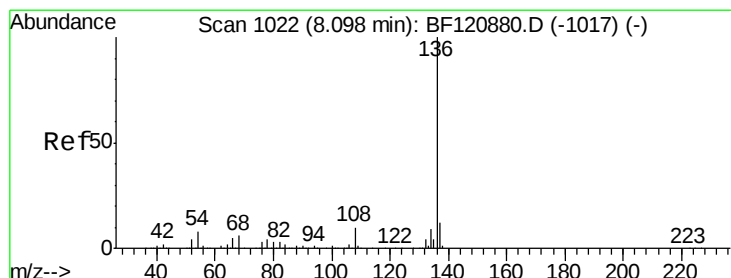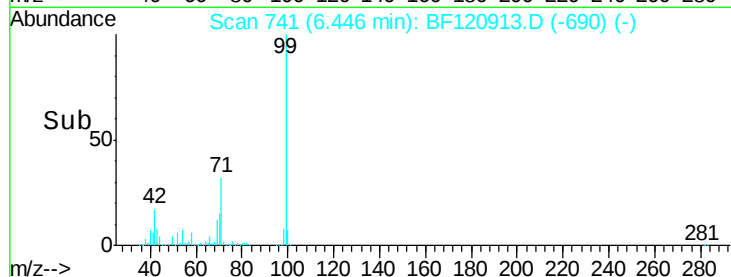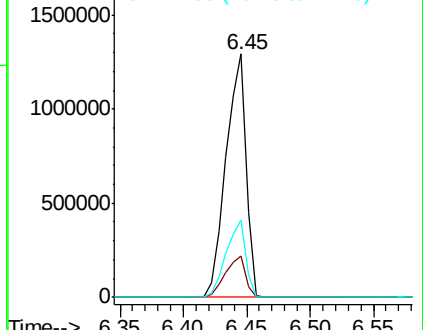

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.10 min Scan# 1022


Delta R.T. 0.00 min

Lab File: BF120913.D

Acq: 17 Jul 2020 10:22

Tgt Ion: 136 Resp: 673762

Ion	Ratio	Lower	Upper
136	100		
137	11.0	9.3	13.9
54	7.1	6.3	9.5
68	5.5	5.0	7.4

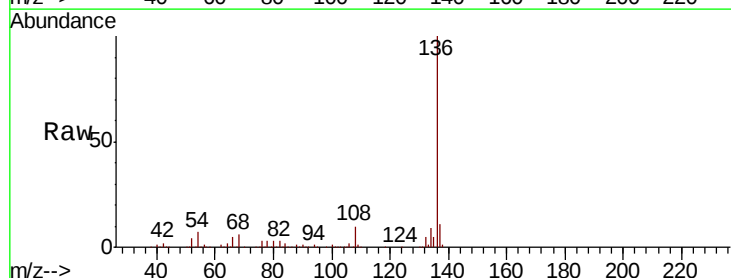



Abundance

Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

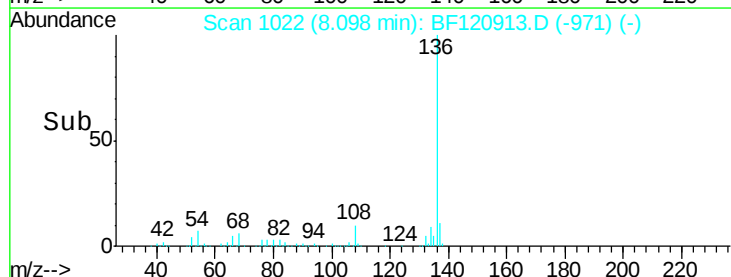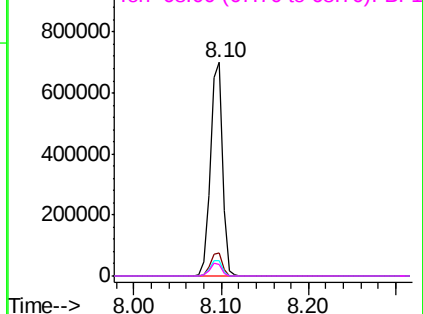







#23
 Nitrobenzene-d5
 Concen: 77.582 ng
 RT: 7.37 min Scan# 899
 Delta R.T. -0.01 min
 Lab File: BF120913.D
 Acq: 17 Jul 2020 10:22

Instrument :
 BNA_F
 ClientSampleId :
 PB130249BL

Tot Ion: 82 Resp: 903372
 Ion Ratio Lower Upper
 82 100
 128 47.1 38.2 57.4
 54 48.8 38.7 58.1

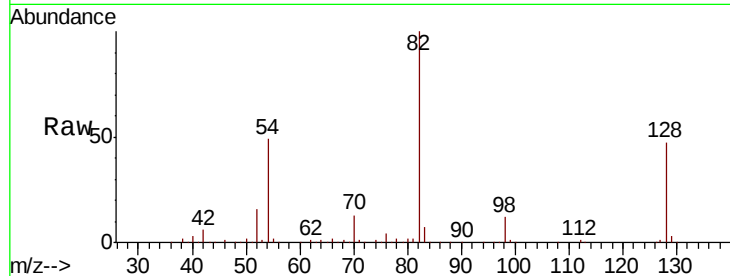


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

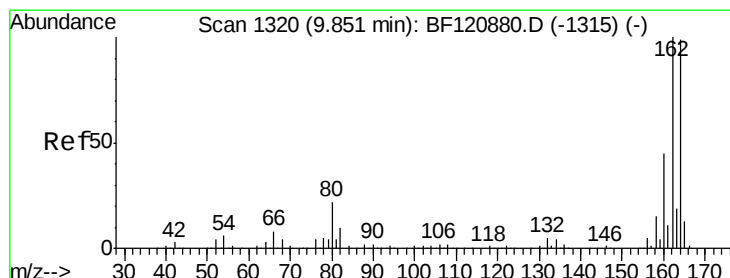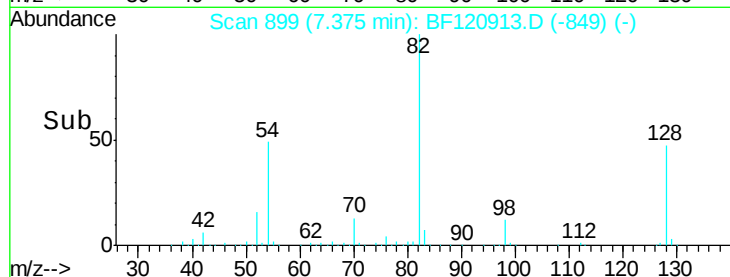
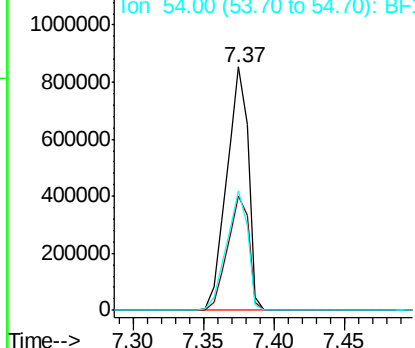



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.85 min Scan# 1320
 Delta R.T. 0.00 min
 Lab File: BF120913.D
 Acq: 17 Jul 2020 10:22

Tgt Ion:164 Resp: 342111
 Ion Ratio Lower Upper
 164 100
 162 101.4 81.2 121.8
 160 47.1 36.9 55.3

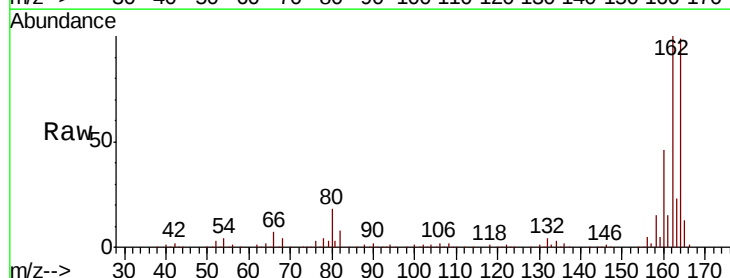

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



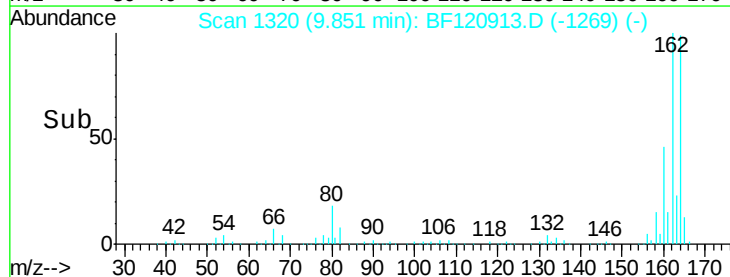
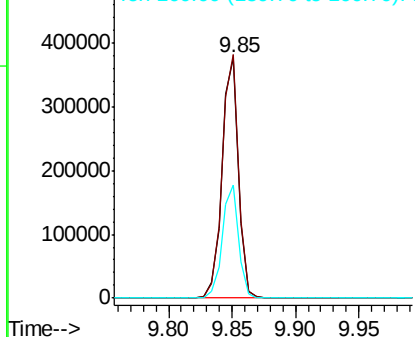


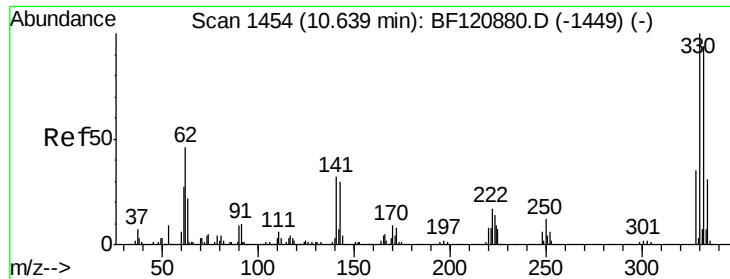

#42
 2,4,6-Tribromophenol
 Concen: 106.366 ng
 RT: 10.64 min Scan# 1454
 Delta R.T. 0.00 min
 Lab File: BF120913.D
 Acq: 17 Jul 2020 10:22




Instrument :
 BNA_F
 ClientSampleId :
 PB130249BL


Tot Ion	Ratio	Lower	Upper
330	100		
332	97.3	75.5	113.3
141	30.1	25.7	38.5

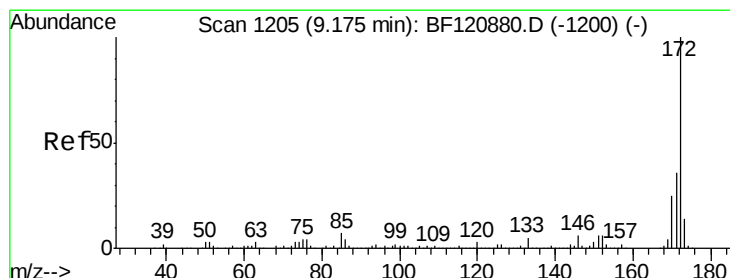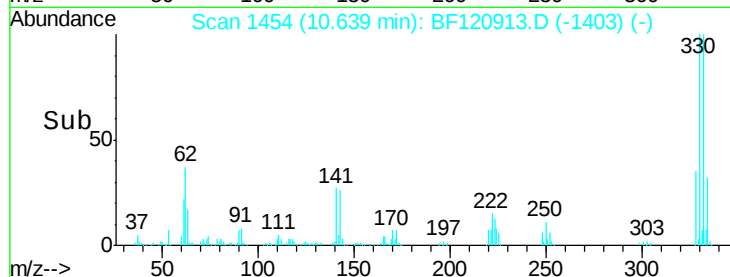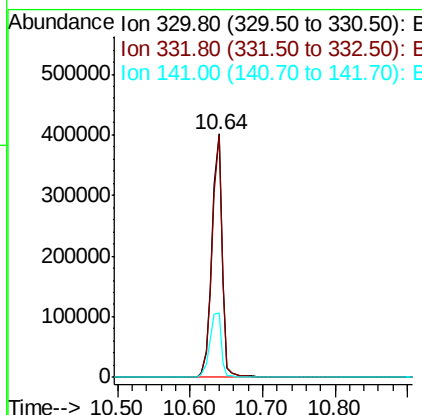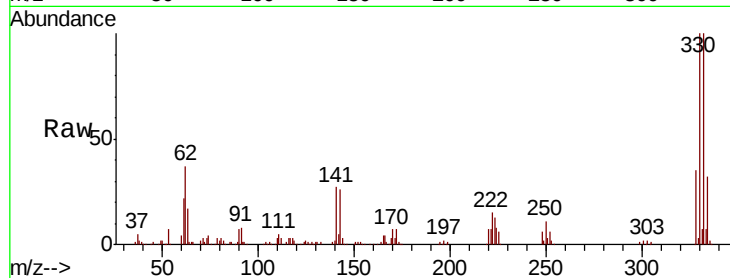

#45
 2-Fluorobiphenyl
 Concen: 69.245 ng
 RT: 9.17 min Scan# 1205
 Delta R.T. 0.00 min
 Lab File: BF120913.D
 Acq: 17 Jul 2020 10:22

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	29.0	43.4
170	24.6	19.6	29.4


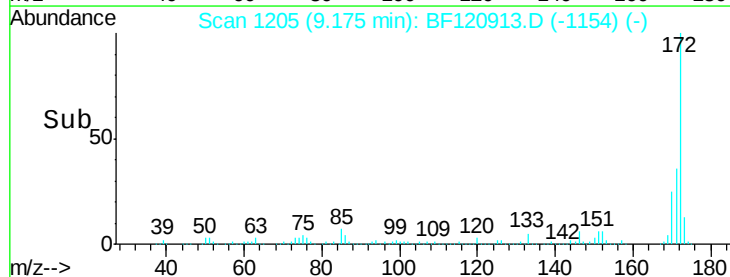
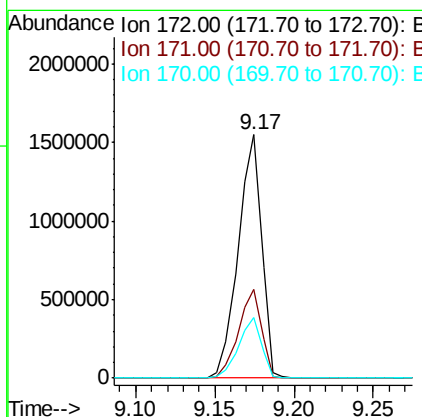
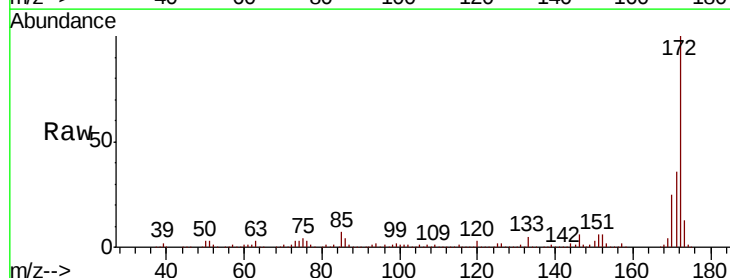


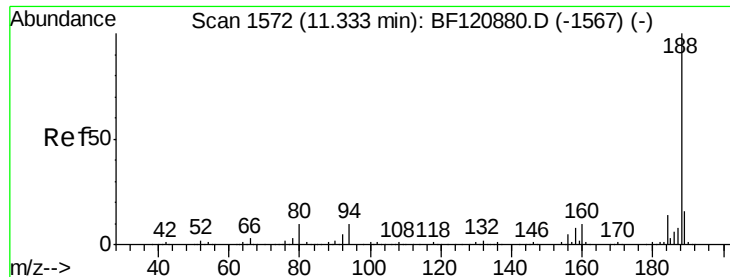

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.33 min Scan# 1572
Delta R.T. 0.00 min
Lab File: BF120913.D
Acq: 17 Jul 2020 10:22




Instrument :
BNA_F
ClientSampleId :
PB130249BL

Tot Ion:188 Resp: 648068
Ion Ratio Lower Upper
188 100
94 9.3 8.0 12.0
80 9.4 8.3 12.5

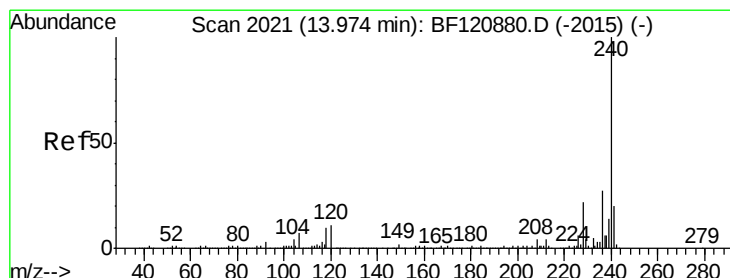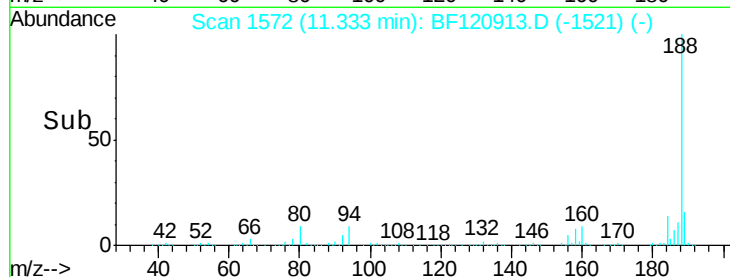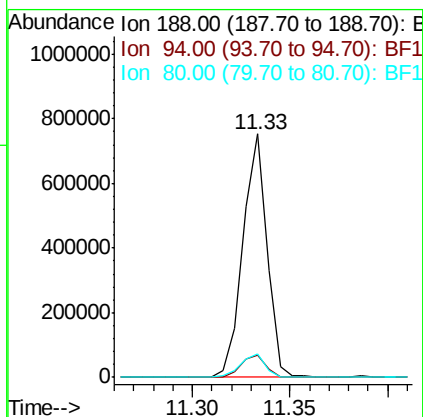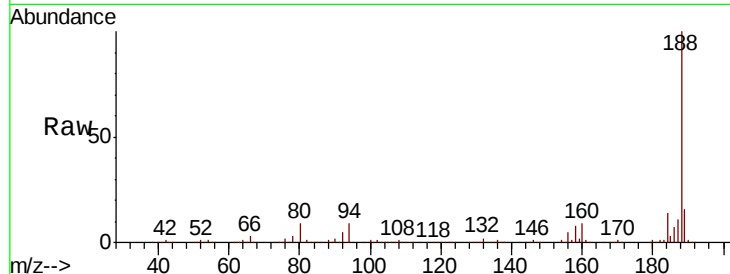

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.97 min Scan# 2020
Delta R.T. -0.01 min
Lab File: BF120913.D
Acq: 17 Jul 2020 10:22

Tgt Ion:240 Resp: 517353
Ion Ratio Lower Upper
240 100
120 10.5 9.0 13.4
236 26.3 21.7 32.5

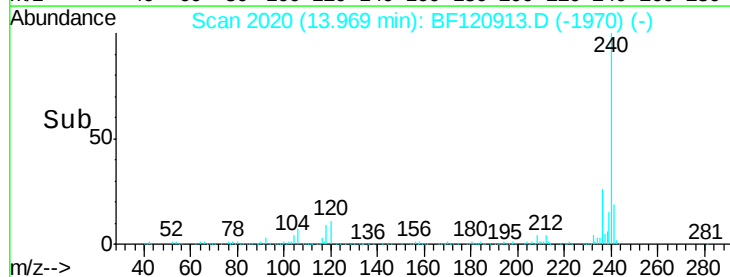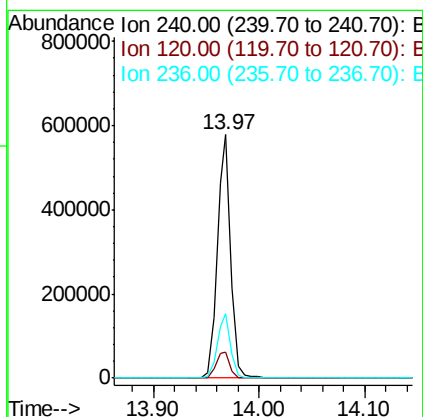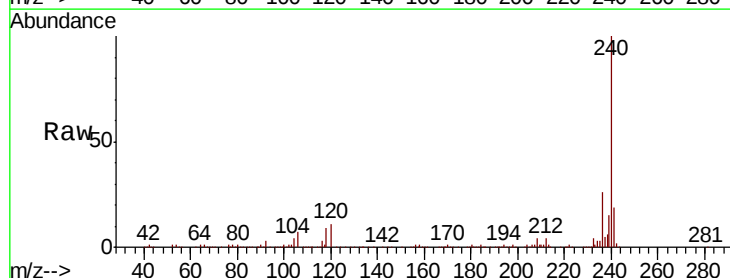



#79

Terphenyl-d14

Concen: 66.129 ng

RT: 12.92 min Scan# 1842

Delta R.T. 0.00 min

Lab File: BF120913.D

Acq: 17 Jul 2020 10:22

Instrument :

BNA_F

ClientSampleId :

PB130249BL


Tot Ion:244 Resp: 1573852

Ion Ratio Lower Upper

244 100

212 7.2 5.6 8.4




122 11.1 8.9 13.3

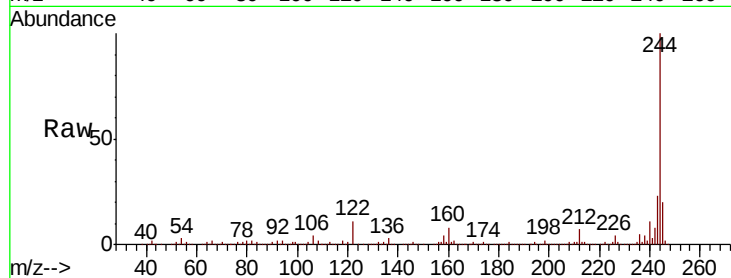

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

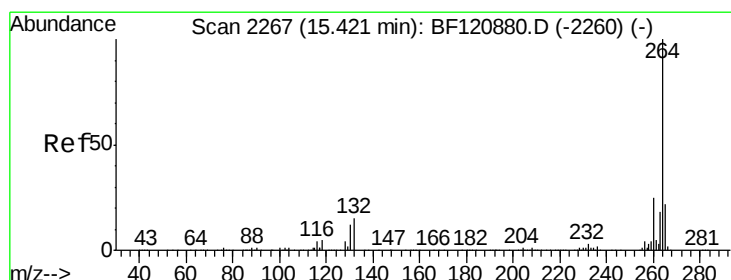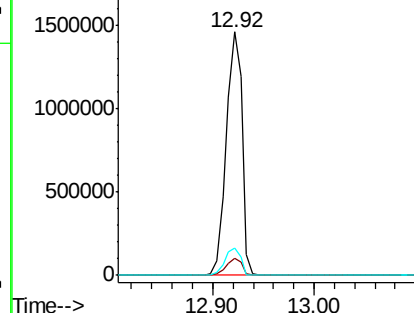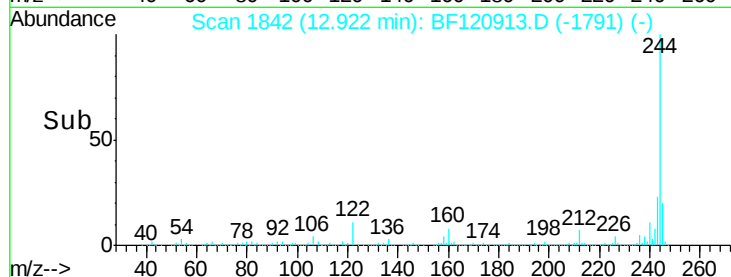

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.42 min Scan# 2266

Delta R.T. -0.01 min

Lab File: BF120913.D

Acq: 17 Jul 2020 10:22


Tgt Ion:264 Resp: 475786

Ion Ratio Lower Upper

264 100

260 24.3 20.0 30.0

265 21.0 17.4 26.2

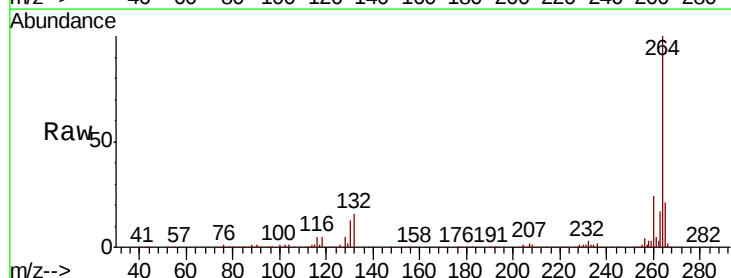

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

