


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071720\
 Data File : BF120910.D
 Acq On : 17 Jul 2020 8:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 16 14:20:32 2020

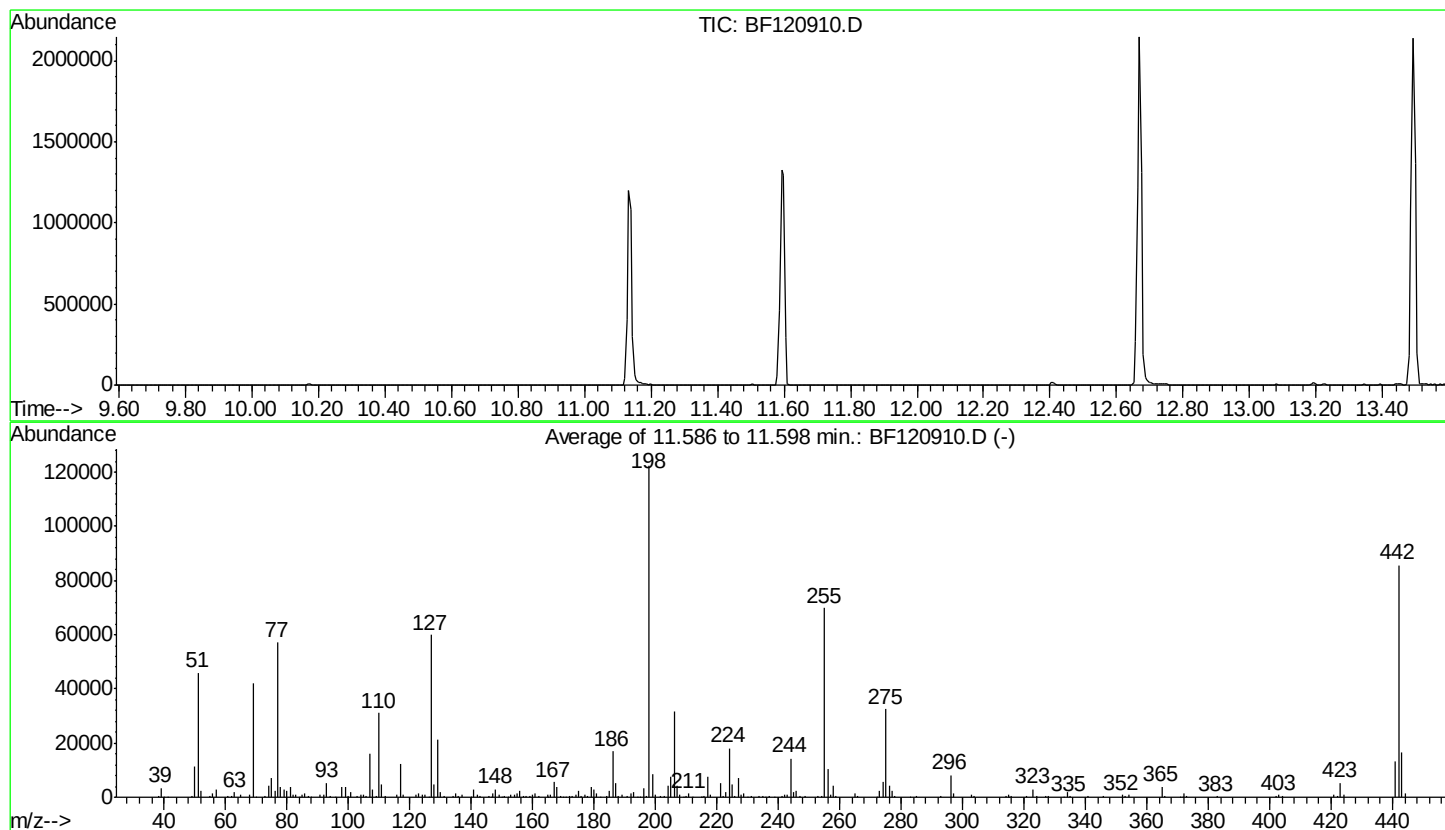

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	45906	PASS
68	69	0.00	2	1.9	819	PASS
69	198	0.00	100	34.5	42213	PASS
70	69	0.00	2	0.5	210	PASS
127	198	10	80	49.0	59994	PASS
197	198	0.00	2	0.6	721	PASS
198	198	100	100	100.0	122389	PASS
199	198	5	9	7.0	8551	PASS
275	198	10	60	26.6	32587	PASS
365	198	1	100	3.1	3782	PASS
441	198	0.01	100	10.9	13346	PASS
442	198	50	100	70.1	85753	PASS
443	442	15	24	19.3	16573	PASS