
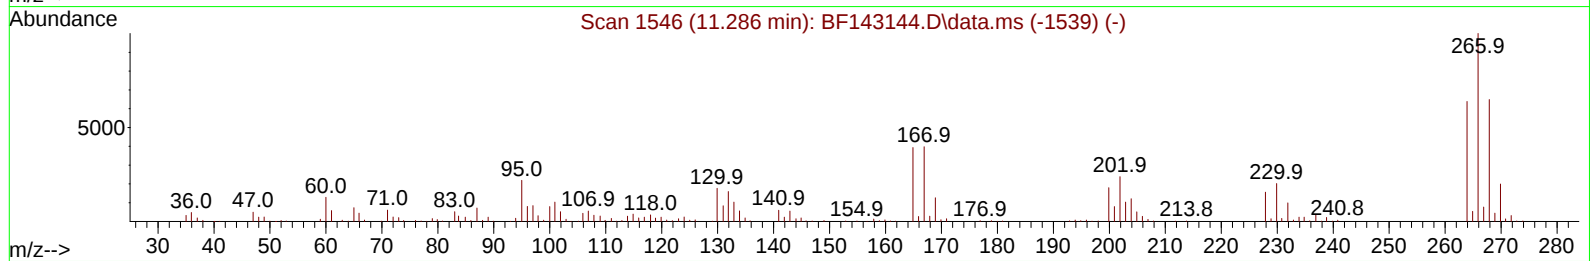
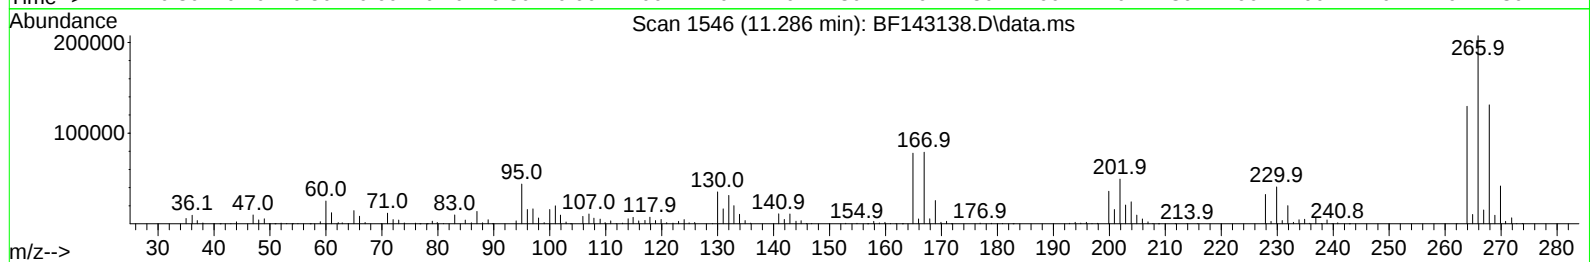


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071725\
Data File : BF143138.D
Acq On : 17 Jul 2025 09:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 17 16:32:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

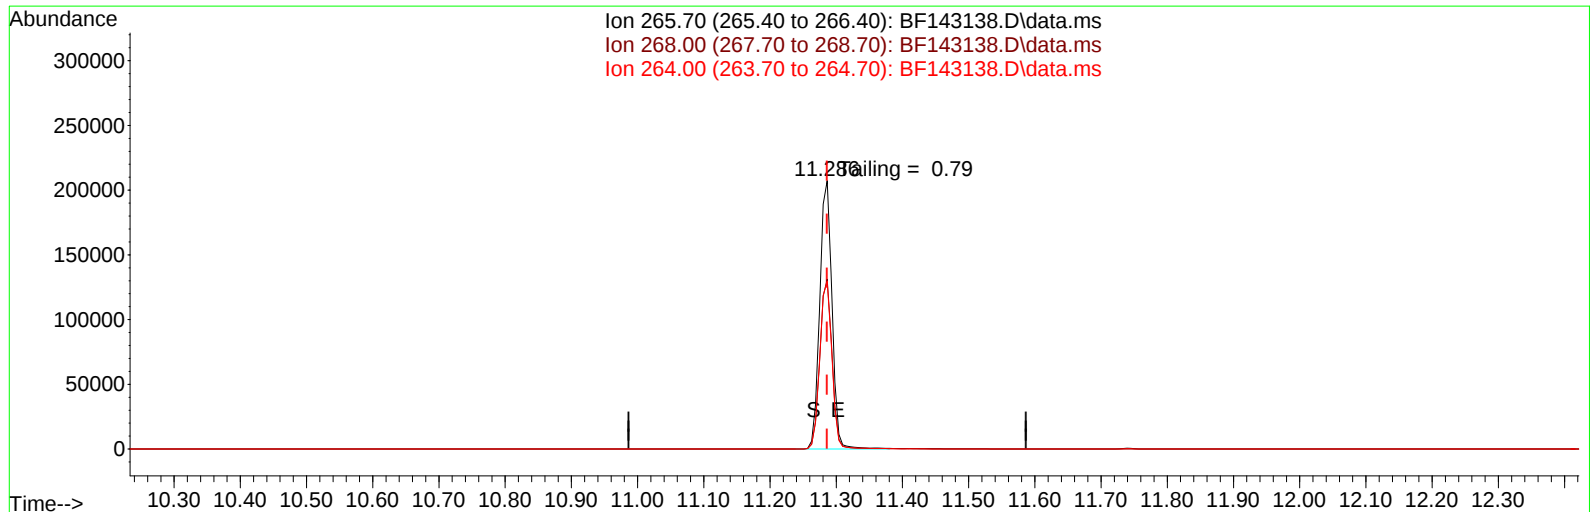

TIC: BF143138.D\data.ms

(70) Pentachlorophenol (C)




11.286min (+ 0.000) 29509.64 ng

response 268044

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.24
264.00	63.80	62.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071725\
Data File : BF143138.D
Acq On : 17 Jul 2025 09:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 17 16:32:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

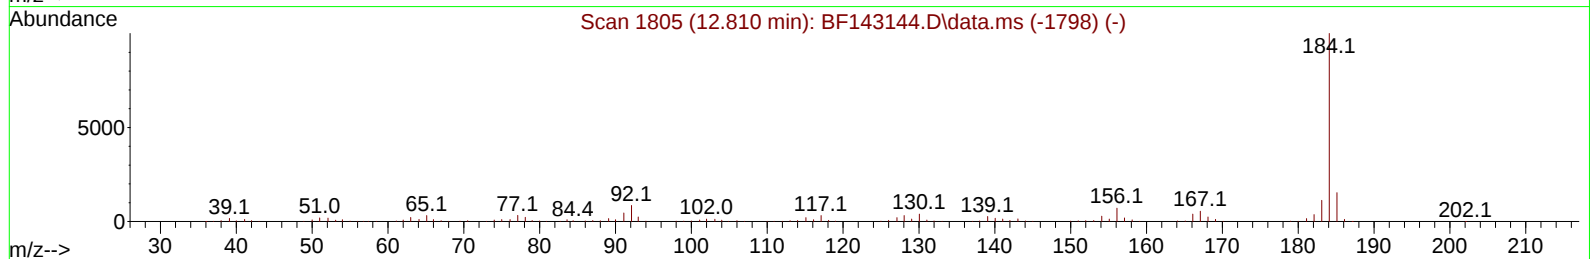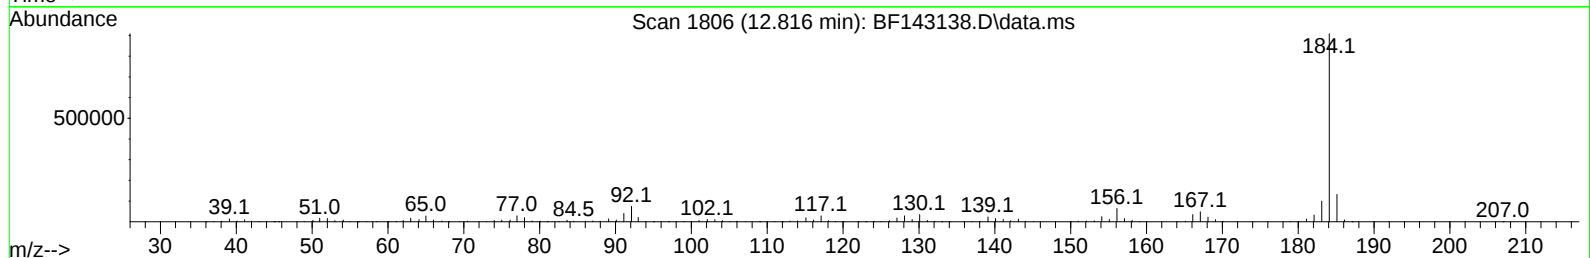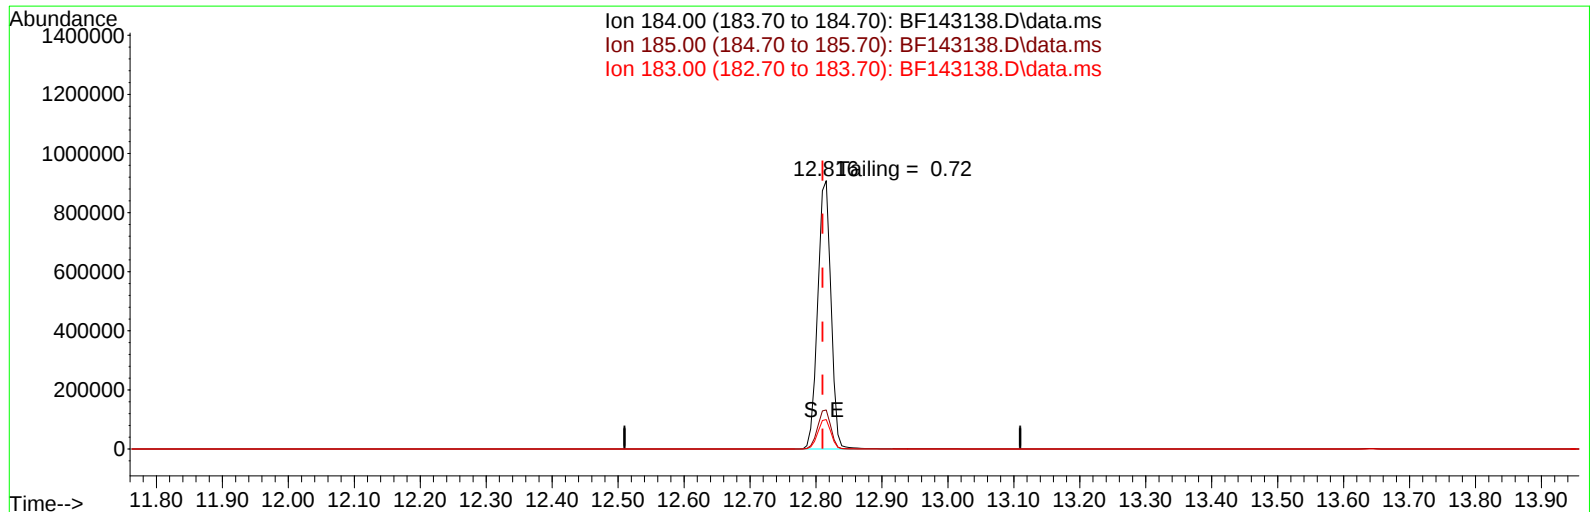

TIC: BF143138.D\data.ms

(77) Benzidine

12.816min (+ 0.006) 0.00 ng

response 1266864

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.57
183.00	11.20	10.98
0.00	0.00	0.00