

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071725\
 Data File : BF143154.D
 Acq On : 17 Jul 2025 18:07
 Operator : RC/JU
 Sample : PB168816BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB168816BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143154.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.216	506	514	522	rBV	271220	449758	9.46%	1.546%
2	5.598	572	579	584	rBV	2773351	3947484	83.01%	13.570%
3	6.581	738	746	751	rBV	2656881	4006781	84.25%	13.774%
4	6.963	805	811	816	rBV	697103	890629	18.73%	3.062%
5	7.516	898	905	910	rBV	1895297	2683198	56.42%	9.224%
6	8.239	1022	1028	1033	rBV	935730	1179882	24.81%	4.056%
7	9.316	1204	1211	1216	rBV	3572116	4755556	100.00%	16.348%
8	9.998	1321	1327	1332	rBV	1007521	1294069	27.21%	4.449%
9	10.781	1454	1460	1466	rBV	2113543	2793012	58.73%	9.601%
10	11.480	1574	1579	1584	rBV	1062161	1296767	27.27%	4.458%
11	13.069	1843	1849	1854	rBV	3137444	4141615	87.09%	14.237%
12	14.116	2022	2027	2036	rBV	619987	776261	16.32%	2.668%
13	14.363	2062	2069	2081	rVB3	22674	70032	1.47%	0.241%
14	15.621	2276	2283	2288	rBV	504588	804857	16.92%	2.767%




Sum of corrected areas: 29089901

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071725\
Data File : BF143154.D
Acq On : 17 Jul 2025 18:07
Operator : RC/JU
Sample : PB168816BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168816BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

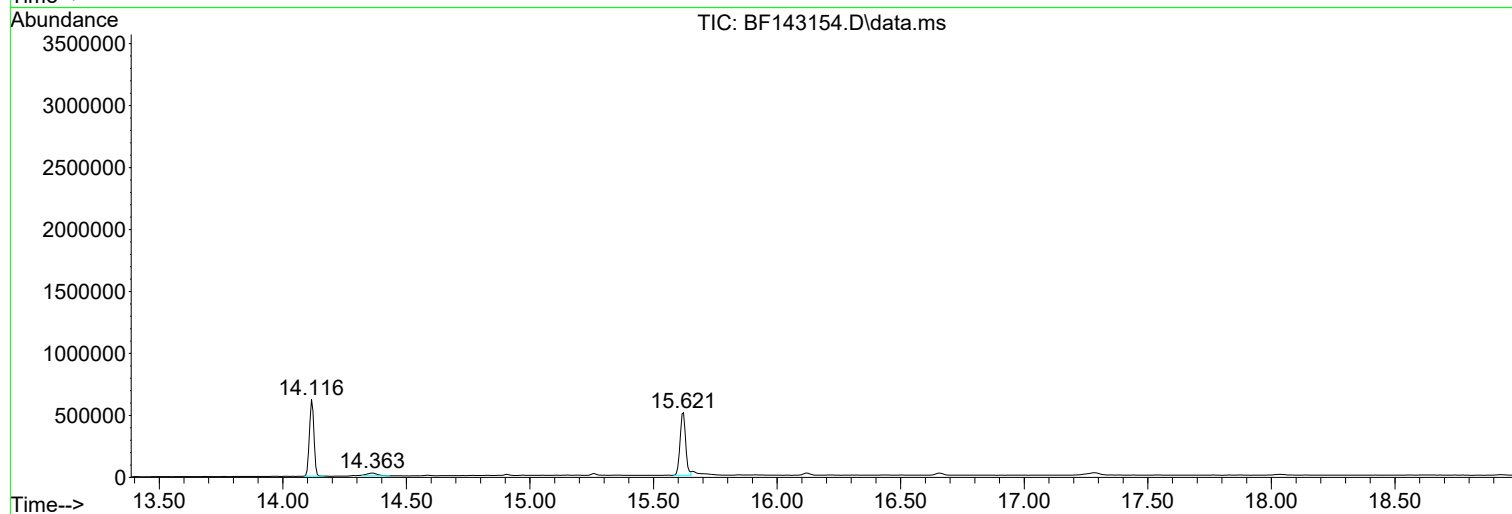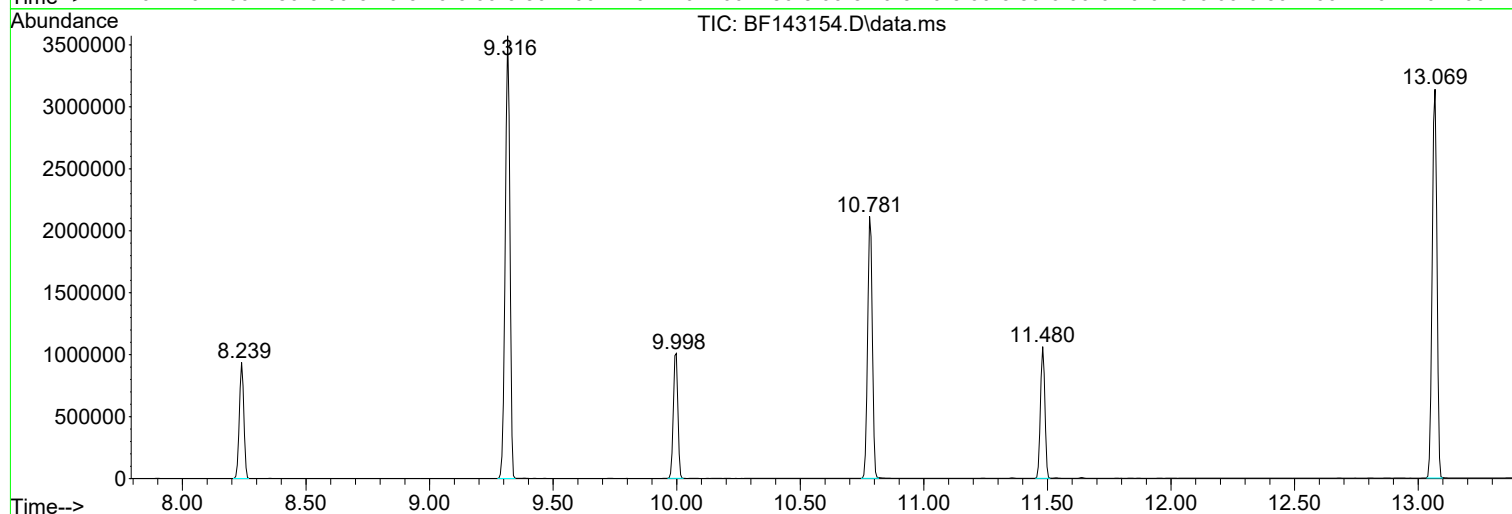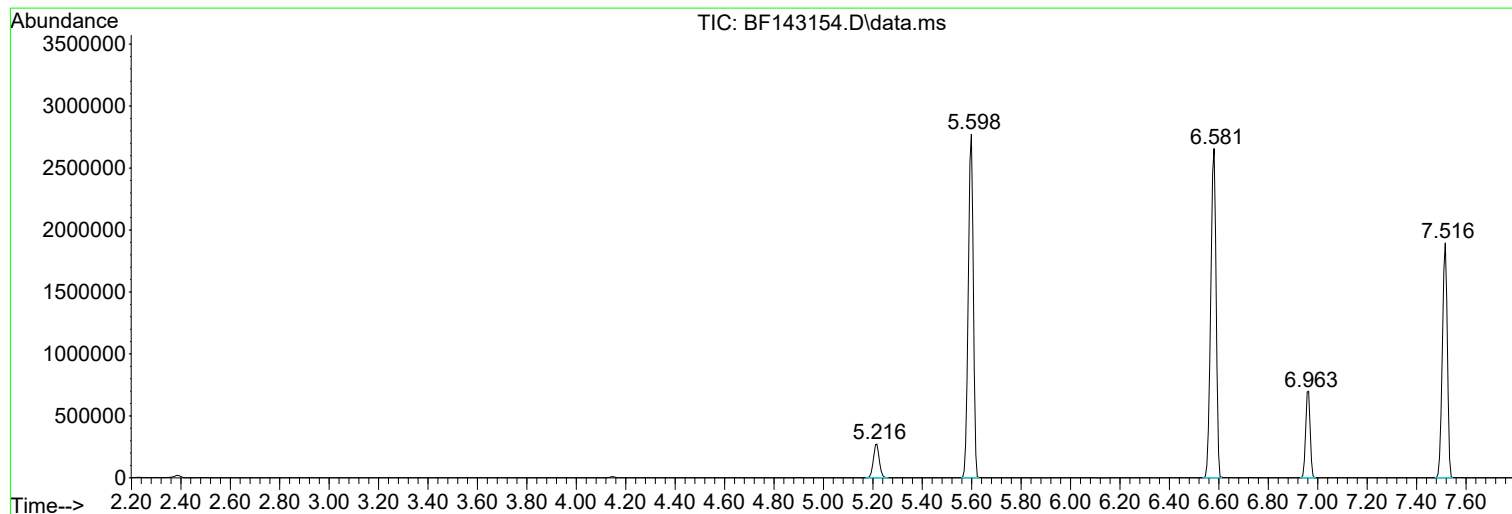

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071725\
Data File : BF143154.D
Acq On : 17 Jul 2025 18:07
Operator : RC/JU
Sample : PB168816BL
Misc :
ALS Vial : 17 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB168816BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
5.216	10.10 ng	449758	1,4-Dichlorobenzene-d4			6.963
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	59
2	2,3-Butanedione, monooxime		101	C4H7NO2	000057-71-6	27
3	1-Propen-2-ol, acetate		100	C5H8O2	000108-22-5	12
4	Acetone		58	C3H6O	000067-64-1	9
5	Butyl aldoxime, 3-methyl-, syn-		101	C5H11NO	005780-40-5	9

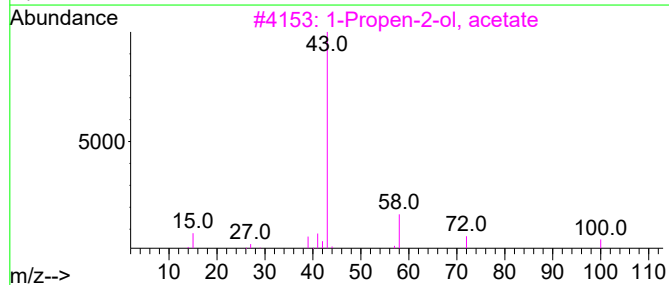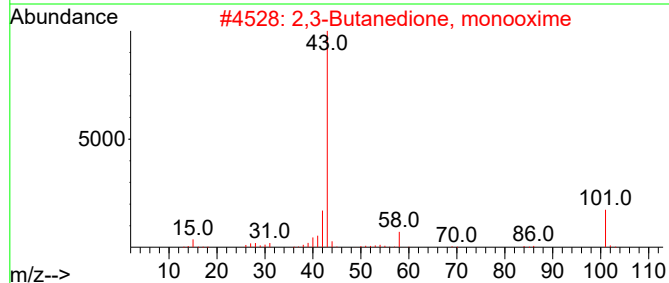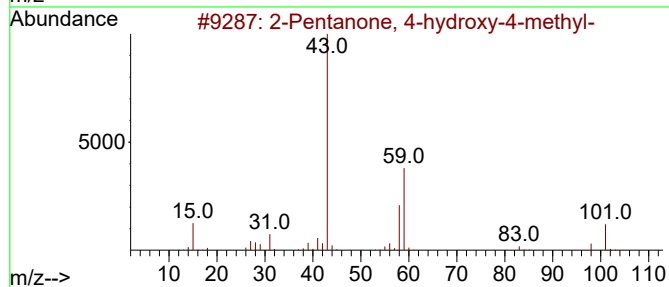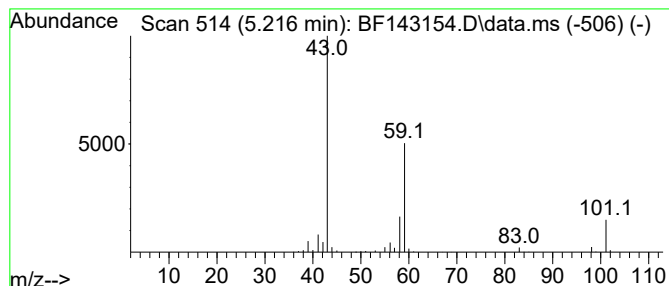

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071725\
Data File : BF143154.D
Acq On : 17 Jul 2025 18:07
Operator : RC/JU
Sample : PB168816BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168816BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.216	10.1	ng	449758	1	6.963	890629	20.0