
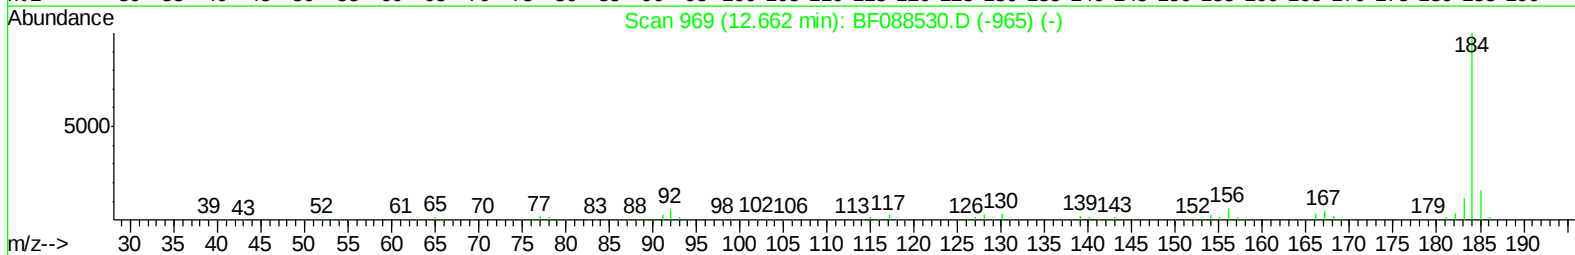
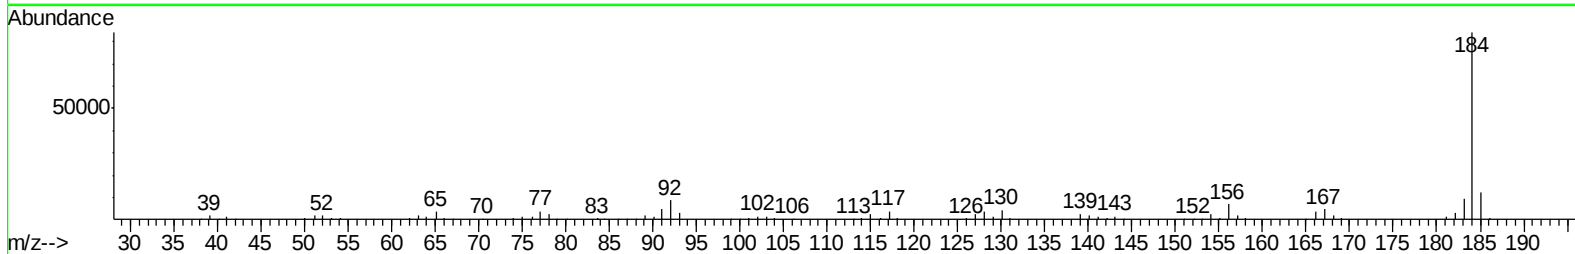


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071816\
Data File : BF089104.D
Acq On : 19 Jul 2016 3:08
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 06:52:22 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 19 03:29:12 2016
Response via : Initial Calibration

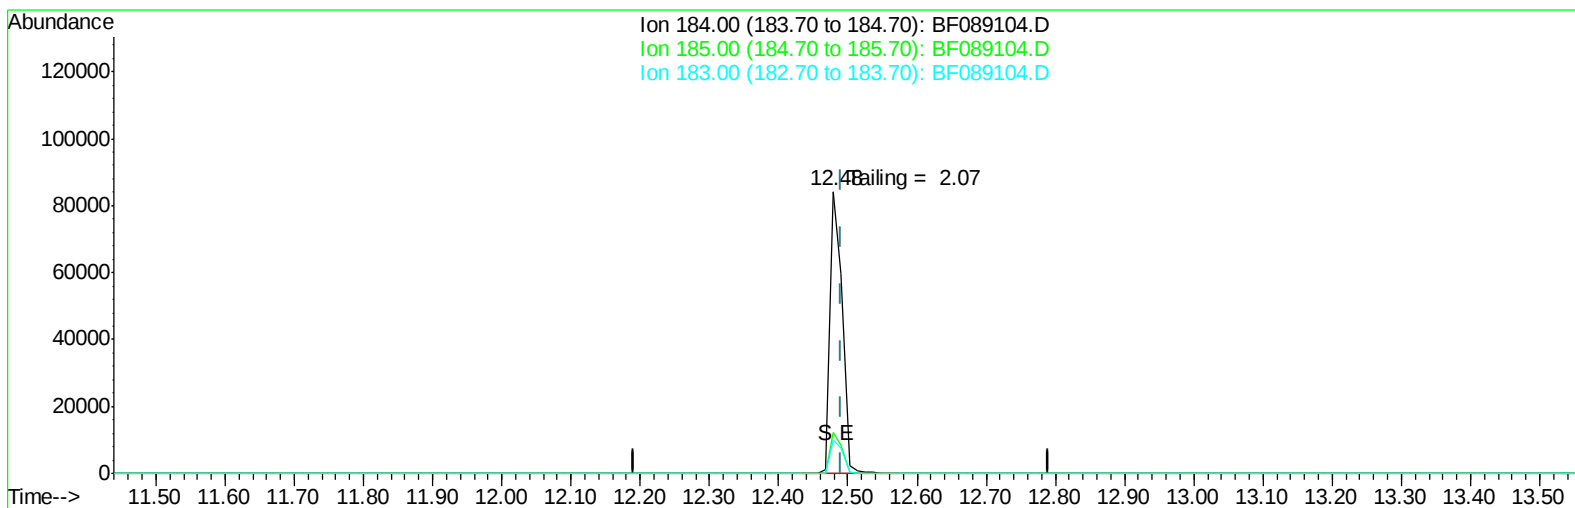

TIC: BF089104.D

(76) Benzidine




12.479min (-0.011) 0.00ng

response 102337

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.60
183.00	11.60	11.64
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071816\
Data File : BF089104.D
Acq On : 19 Jul 2016 3:08
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 06:52:22 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 19 03:29:12 2016
Response via : Initial Calibration

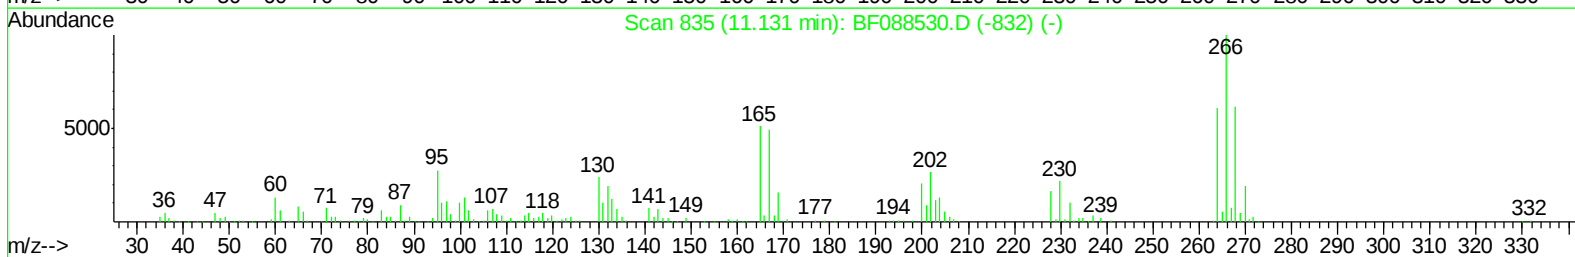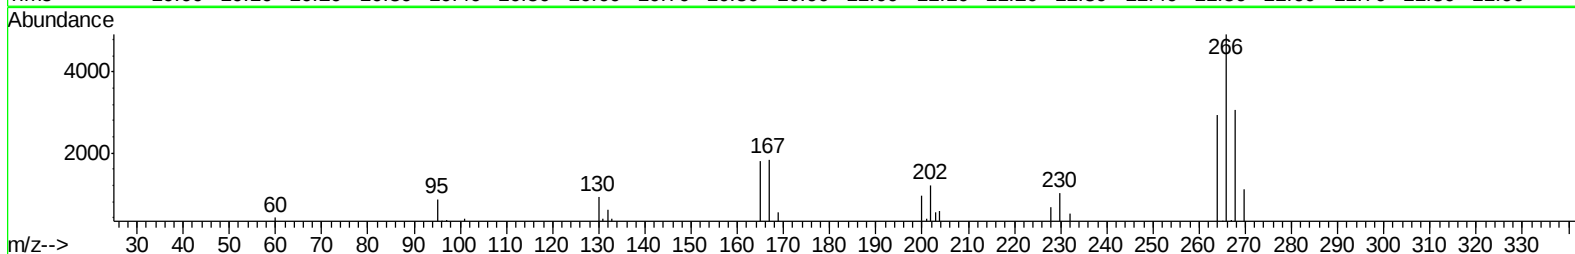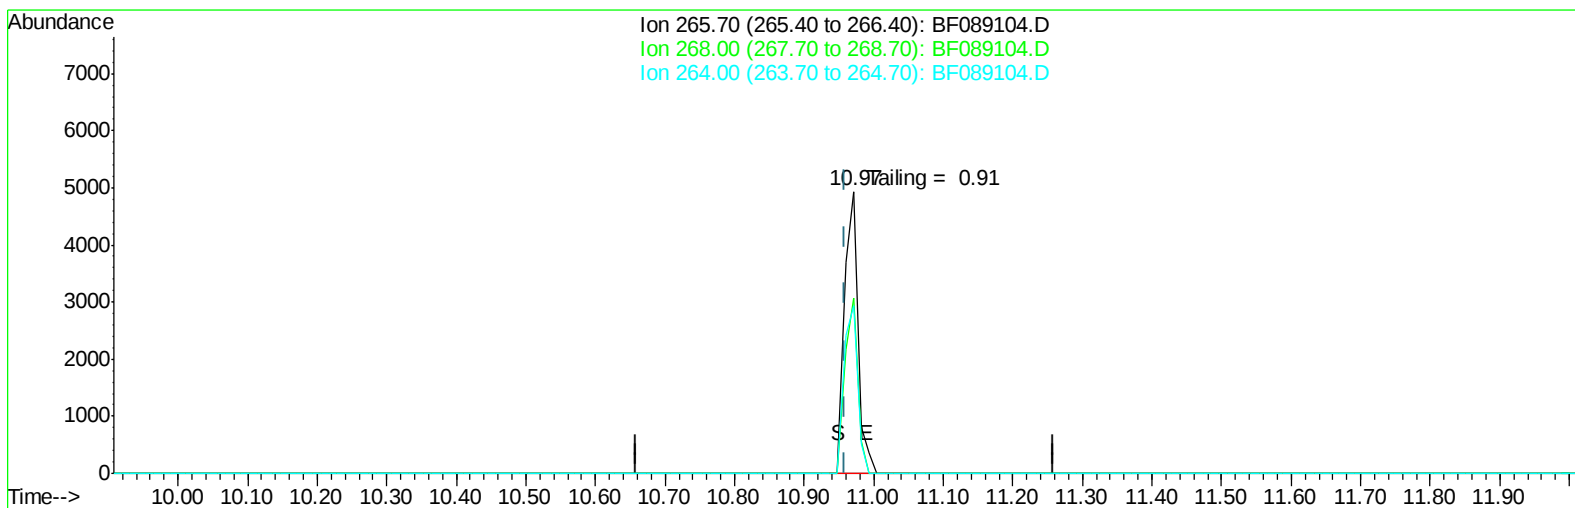

TIC: BF089104.D

(69) Pentachlorophenol (C)

10.971min (+0.011) 0.00ng

response 6717

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	62.08
264.00	62.00	59.44
0.00	0.00	0.00