


Data Path : Z:\HPCHEM1\BNA F\DATA\BF071816\
 Data File : BF089081.D
 Acq On : 18 Jul 2016 13:37
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 19 15:28:17 2016

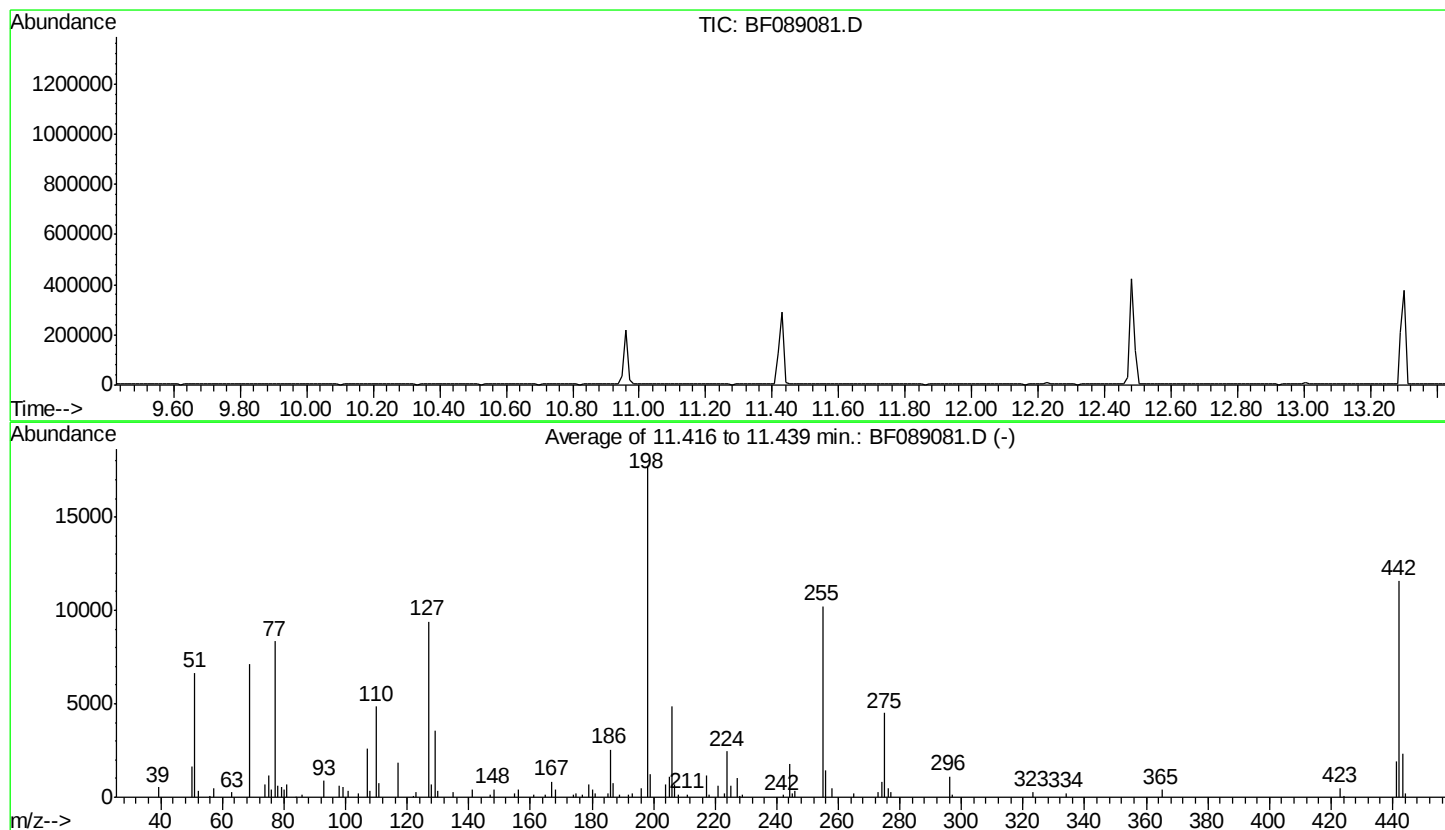

AutoFind: Scans 860, 861, 862; Background Corrected with Scan 856

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	6681	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.2	7133	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.9	9393	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17749	PASS
199	198	5	9	7.0	1247	PASS
275	198	10	60	25.3	4495	PASS
365	198	1	100	2.2	390	PASS
441	442	0.01	24	16.8	1942	PASS
442	198	50	100	65.3	11589	PASS
443	442	15	24	20.1	2327	PASS