


Data Path : Z:\HPCHEM1\BNA F\DATA\BF071816\
 Data File : BF089104.D
 Acq On : 19 Jul 2016 3:08
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 19 15:28:17 2016

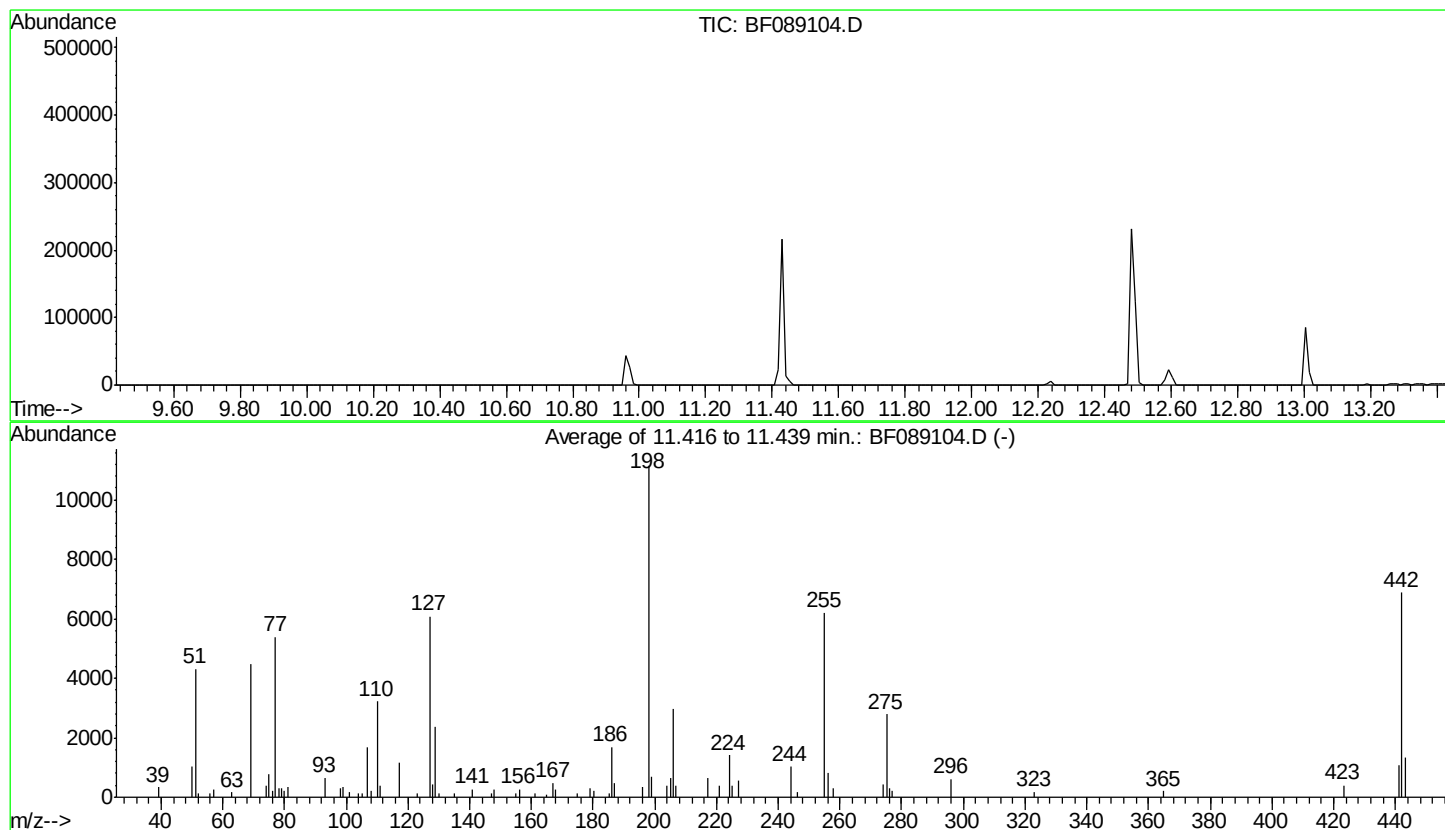

AutoFind: Scans 860, 861, 862; Background Corrected with Scan 857

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	4312	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.2	4478	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.6	6091	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	11151	PASS
199	198	5	9	6.2	693	PASS
275	198	10	60	24.9	2779	PASS
365	198	1	100	1.9	214	PASS
441	442	0.01	24	15.9	1097	PASS
442	198	50	100	61.7	6884	PASS
443	442	15	24	19.3	1330	PASS