
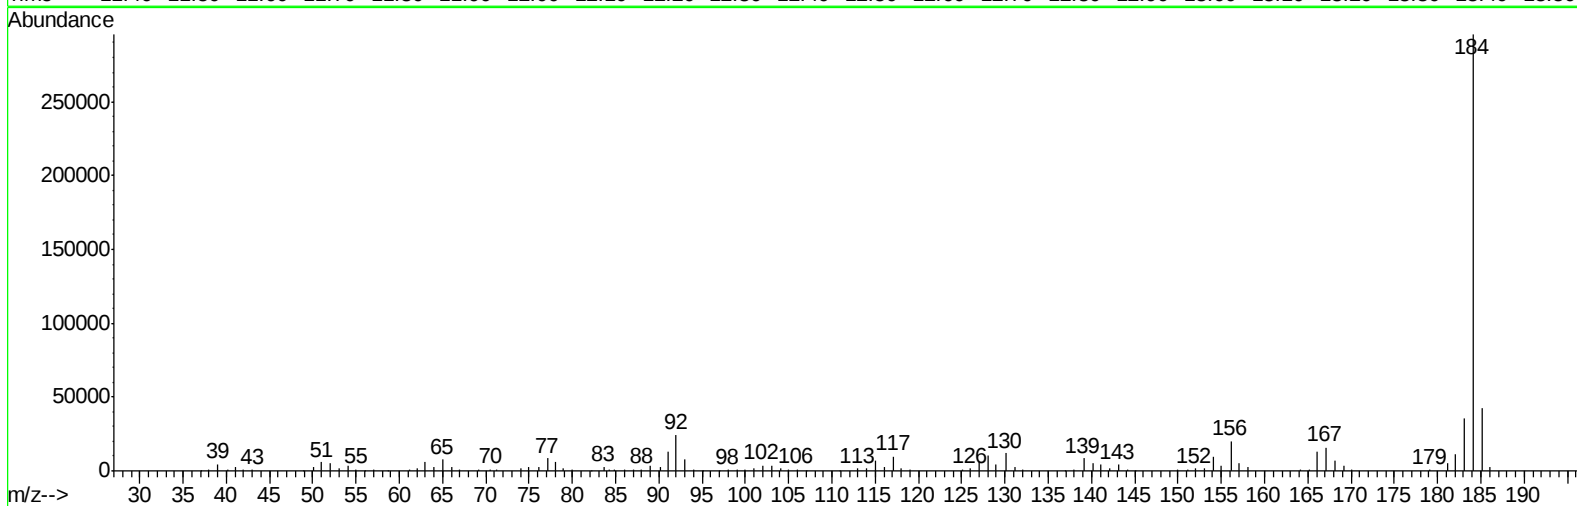


Data Path : Z:\HPCHEM1\BNA F\DATA\BF071817\
 Data File : BF096858.D
 Acq On : 18 Jul 2017 21:57
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 04:44:11 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 18 13:33:22 2017
 Response via : Initial Calibration

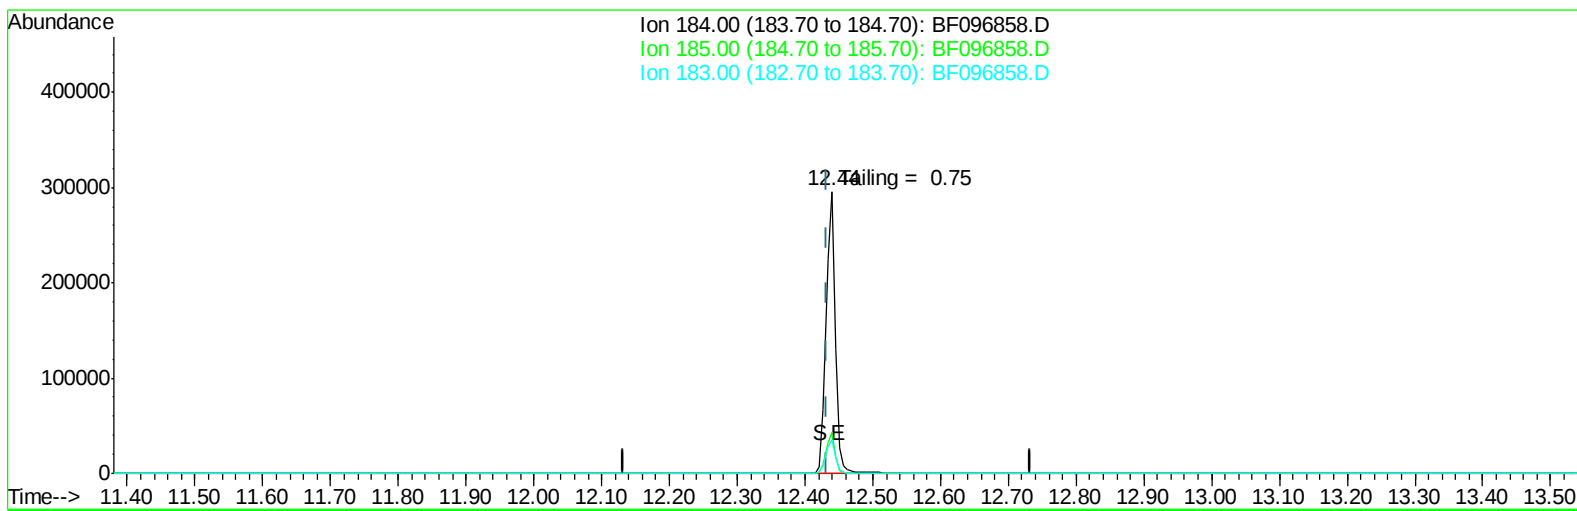

TIC: BF096858.D

(76) Benzidine



12.439min (+0.006) 52078.43ng

response 274684

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.40#
183.00	12.20	11.96
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF071817\
Data File : BF096858.D
Acq On : 18 Jul 2017 21:57
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 04:44:11 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 18 13:33:22 2017
Response via : Initial Calibration

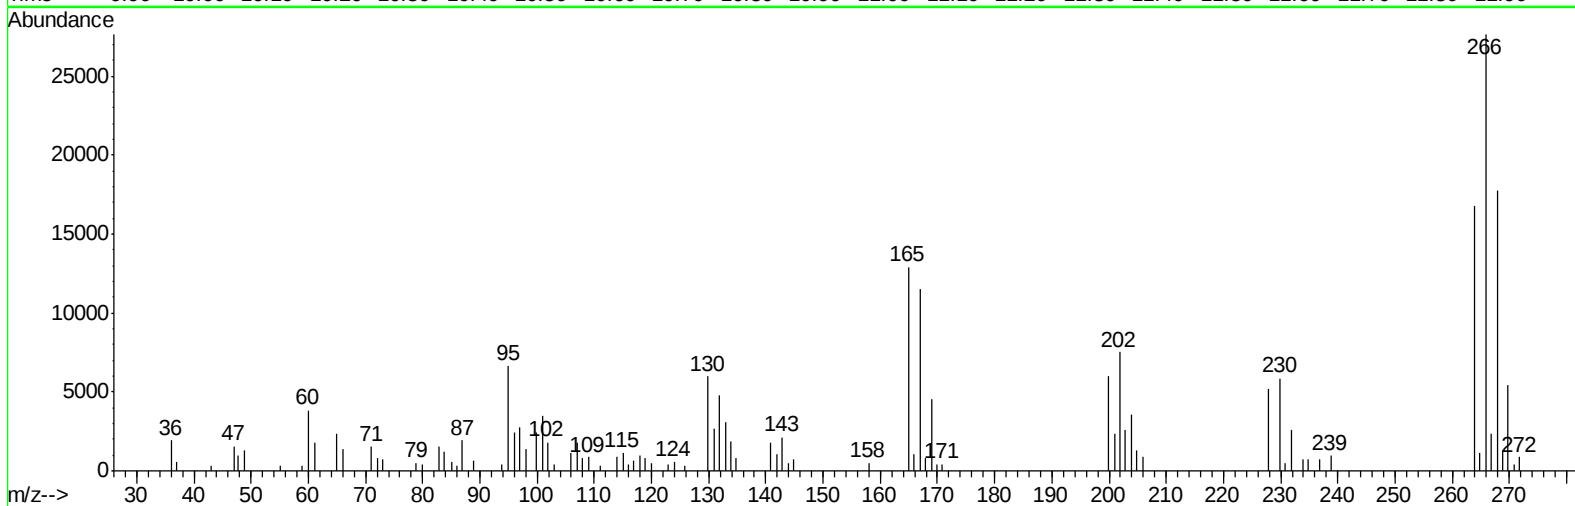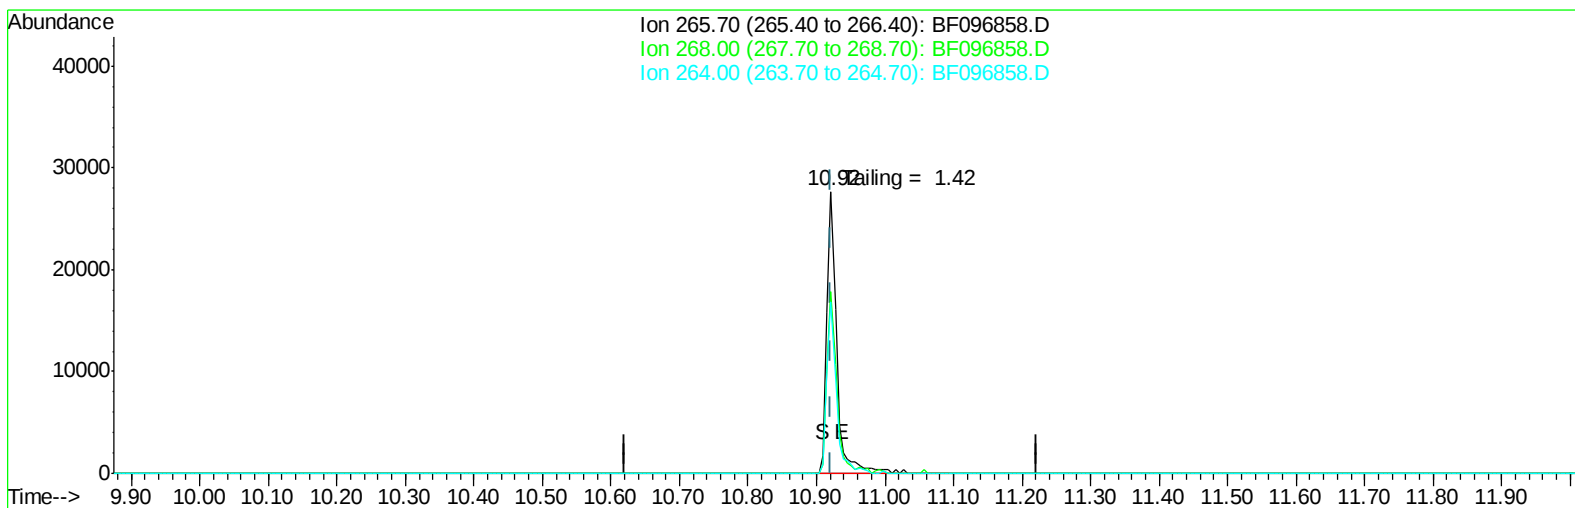

TIC: BF096858.D

(69) Pentachlorophenol (C)

10.921min (-0.000) 0.00ng

response 26650

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.33
264.00	64.60	60.78
0.00	0.00	0.00