


Data Path : Z:\HPCHEM1\BNA F\Data\BF071817\
 Data File : BF096835.D
 Acq On : 18 Jul 2017 9:15
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 18 13:33:22 2017

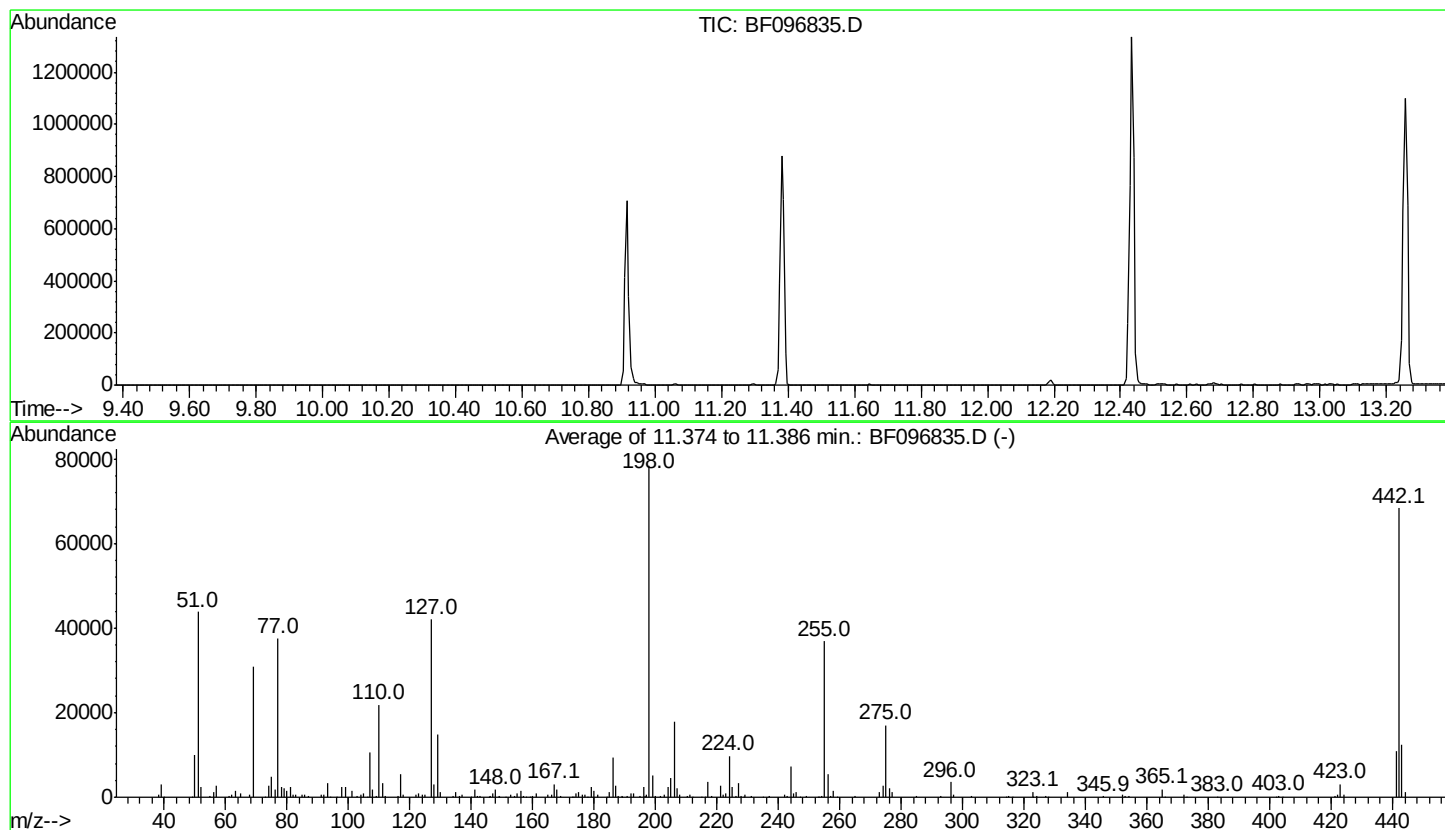

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.9	43800	PASS
68	69	0.00	2	1.8	545	PASS
69	198	0.00	100	39.4	30901	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.6	41986	PASS
197	198	0.00	2	0.9	742	PASS
198	198	100	100	100.0	78378	PASS
199	198	5	9	6.6	5193	PASS
275	198	10	60	21.8	17065	PASS
365	198	1	100	2.3	1837	PASS
441	442	0.01	24	16.1	10978	PASS
442	198	50	100	87.2	68346	PASS
443	442	15	24	18.0	12330	PASS