

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071822\
 Data File : BF129263.D
 Acq On : 18 Jul 2022 10:26
 Operator : CG\JU
 Sample : PB146238BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146238BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129263.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.046	294	299	305	rVB	133395	167216	1.75%	0.268%
2	5.181	488	492	501	rVB	65573	96930	1.01%	0.155%
3	5.540	547	553	556	rBV	7439314	8109875	84.68%	12.989%
4	6.534	715	722	725	rBV	6897000	8346416	87.15%	13.368%
5	6.898	780	784	787	rBV	2170580	1784603	18.63%	2.858%
6	7.463	874	880	883	rBV	4687676	5661040	59.11%	9.067%
7	8.181	997	1002	1006	rBV	2608750	2472032	25.81%	3.959%
8	9.263	1179	1186	1189	rBV	8559630	9519212	99.39%	15.246%
9	9.939	1295	1301	1305	rBV	3064148	2800525	29.24%	4.485%
10	10.733	1429	1436	1439	rBV	5998811	6285090	65.62%	10.066%
11	11.433	1548	1555	1558	rBV	3052204	2803019	29.27%	4.489%
12	13.022	1818	1825	1828	rBV	8843666	9577519	100.00%	15.340%
13	14.074	2000	2004	2008	rBV	2525312	2423017	25.30%	3.881%
14	14.163	2014	2019	2026	rBV	145765	206234	2.15%	0.330%
15	15.574	2253	2259	2272	rBV	1599975	2183762	22.80%	3.498%




Sum of corrected areas: 62436490

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071822\
Data File : BF129263.D
Acq On : 18 Jul 2022 10:26
Operator : CG\JU
Sample : PB146238BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146238BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

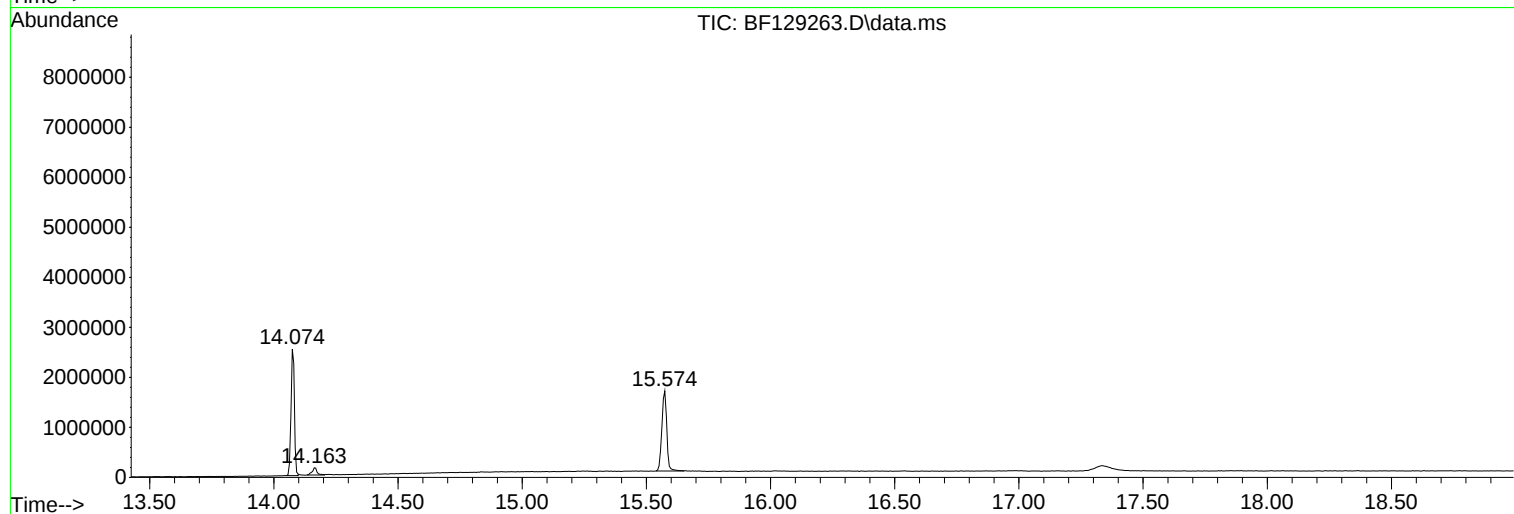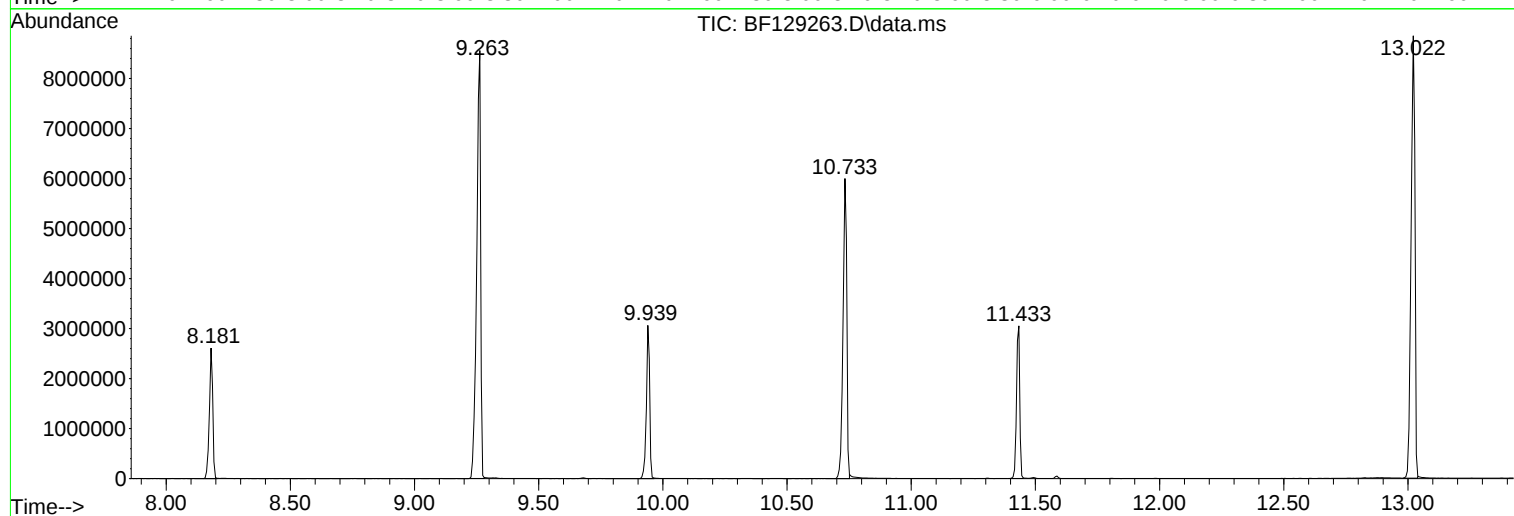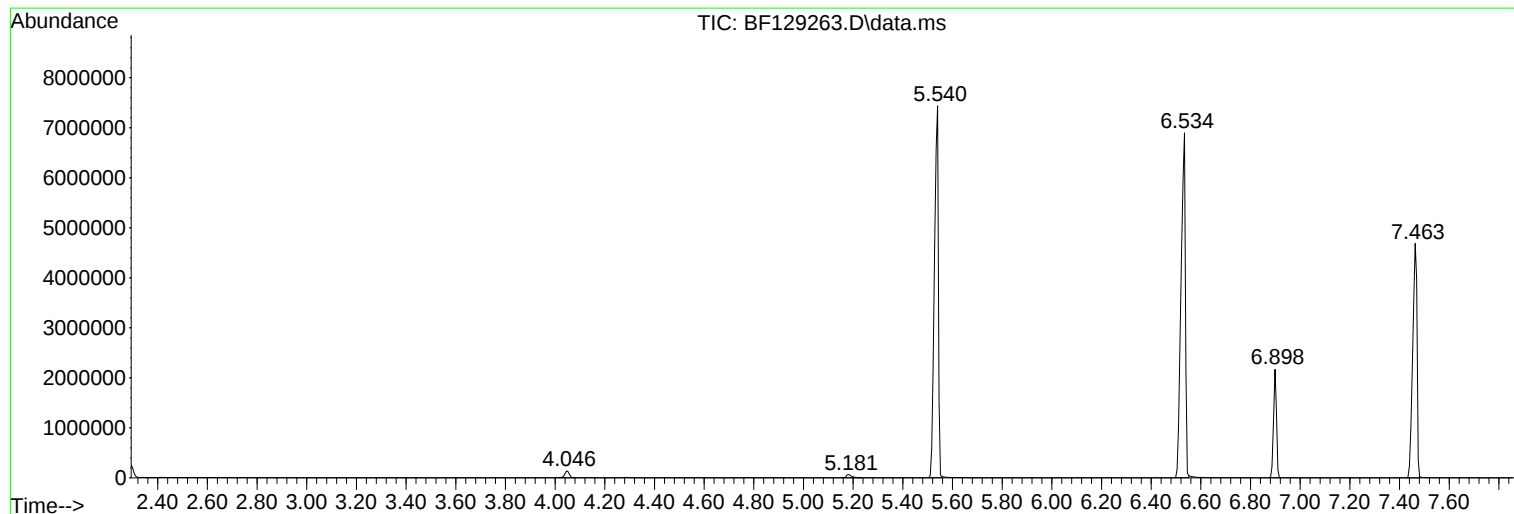

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071822\
Data File : BF129263.D
Acq On : 18 Jul 2022 10:26
Operator : CG\JU
Sample : PB146238BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146238BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071822\
Data File : BF129263.D
Acq On : 18 Jul 2022 10:26
Operator : CG\JU
Sample : PB146238BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146238BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------