

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071822\
 Data File : BF129269.D
 Acq On : 18 Jul 2022 15:54
 Operator : CG\JU
 Sample : PB146273BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146273BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129269.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.052	295	300	307	rVB	144440	179395	1.73%	0.270%
2	5.540	547	553	556	rBV	7809474	8607849	82.89%	12.968%
3	6.534	715	722	725	rBV	7028085	8878851	85.50%	13.377%
4	6.898	780	784	788	rBV	2385141	1917408	18.46%	2.889%
5	7.463	874	880	883	rBV	4727880	6071162	58.46%	9.147%
6	8.181	997	1002	1006	rBV	2696444	2674884	25.76%	4.030%
7	9.263	1178	1186	1189	rBV	9215600	10385081	100.00%	15.646%
8	9.939	1295	1301	1305	rBV	3280029	3077777	29.64%	4.637%
9	10.739	1429	1437	1440	rBV	5955169	6751395	65.01%	10.172%
10	11.433	1548	1555	1558	rBV	3510875	3039335	29.27%	4.579%
11	13.022	1816	1825	1828	rBV	8769255	9993320	96.23%	15.056%
12	14.074	2000	2004	2008	rBV	2579995	2425009	23.35%	3.653%
13	14.163	2013	2019	2027	rBV	289014	380282	3.66%	0.573%
14	15.574	2253	2259	2268	rBV	1481854	1993324	19.19%	3.003%




Sum of corrected areas: 66375072

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071822\
Data File : BF129269.D
Acq On : 18 Jul 2022 15:54
Operator : CG\JU
Sample : PB146273BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146273BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

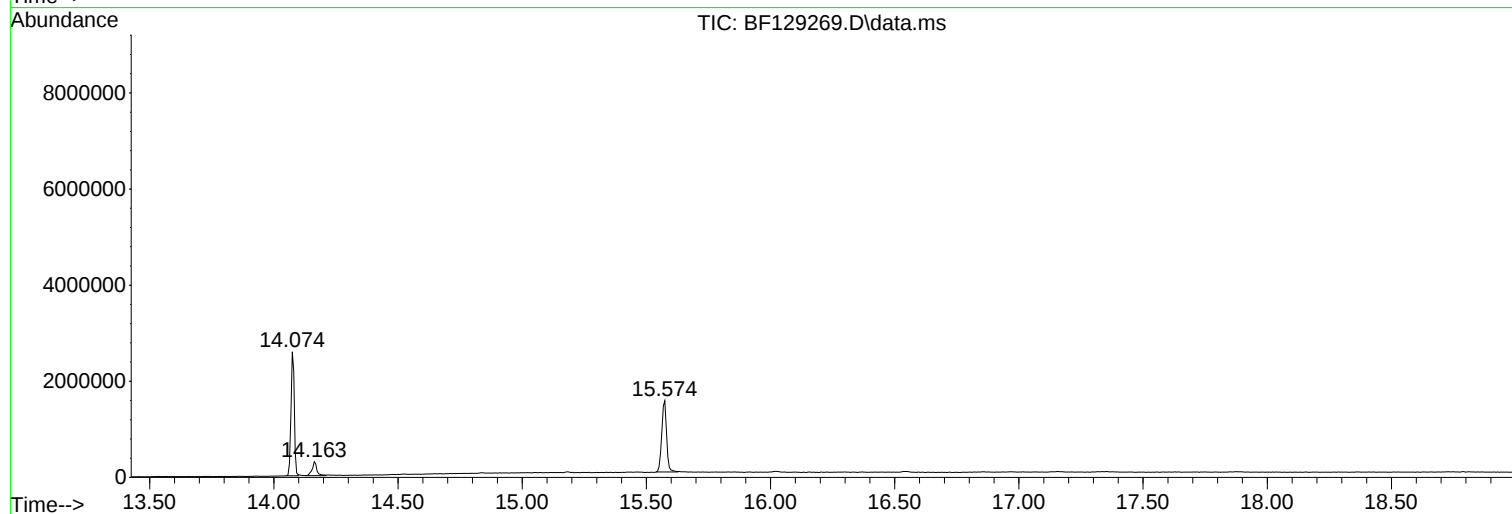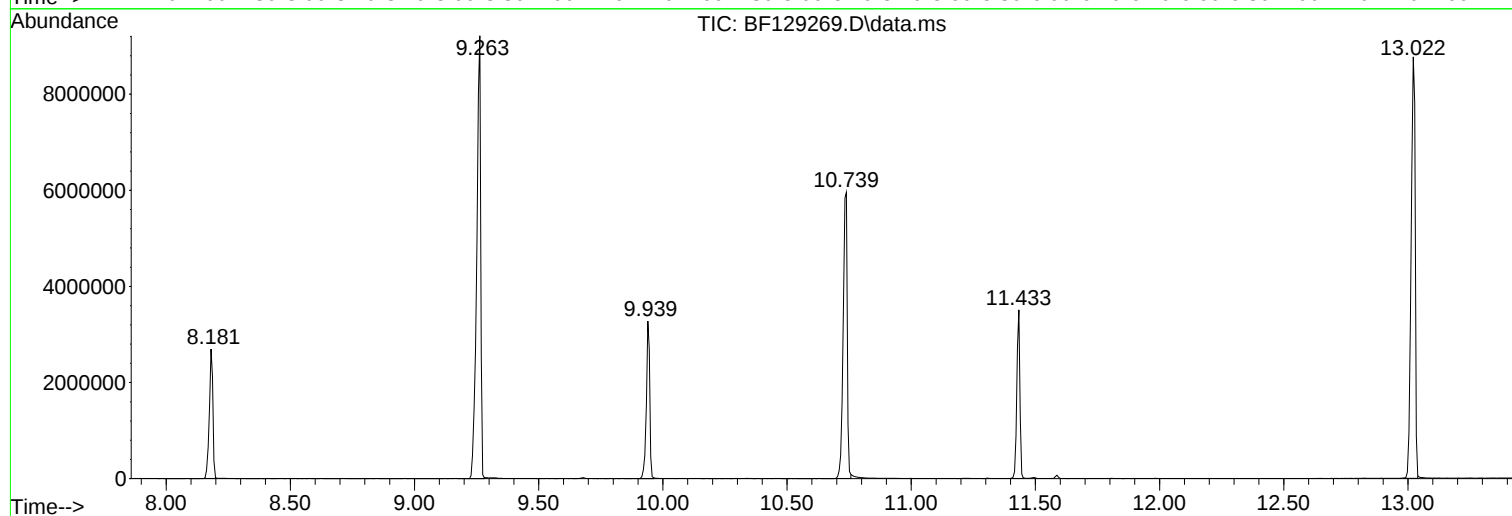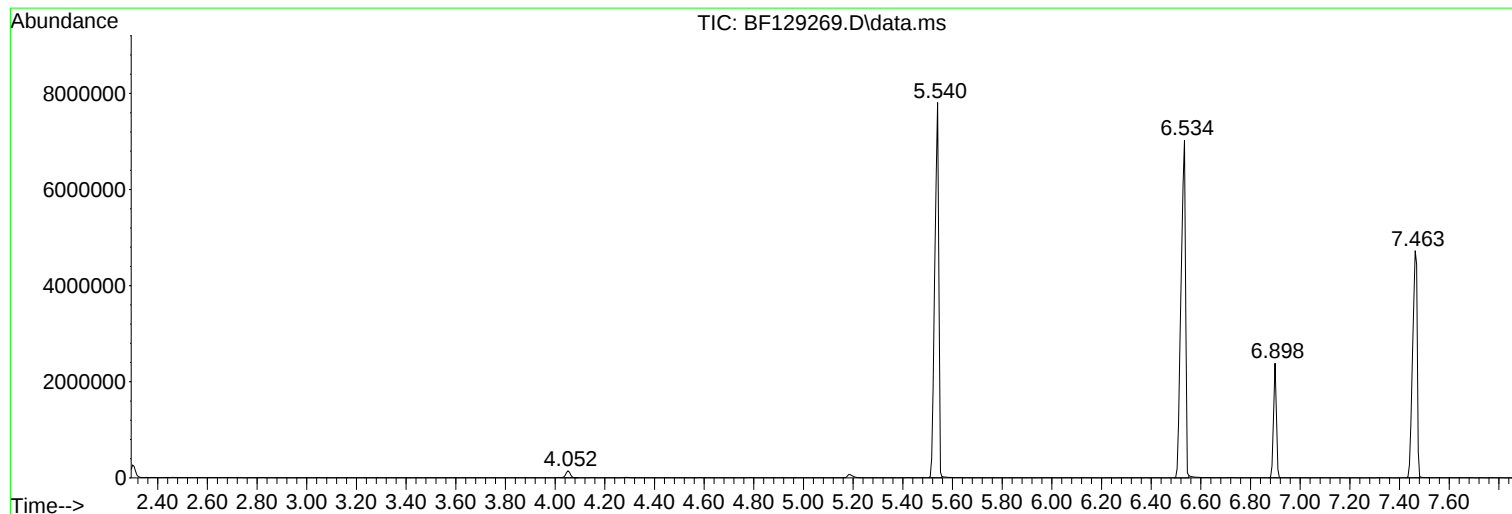

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071822\
Data File : BF129269.D
Acq On : 18 Jul 2022 15:54
Operator : CG\JU
Sample : PB146273BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146273BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.163	3.14 ng	380282	Chrysene-d12	14.074

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	95
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	94
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	64
4			(Carbethoxymethyl)-triphenylphos...	428	C22H22BrO2P	001530-45-6	38
5			Dimethoxymethyl-hydroxy-tripheny...	354	C21H23O3P	1000132-00-1	28

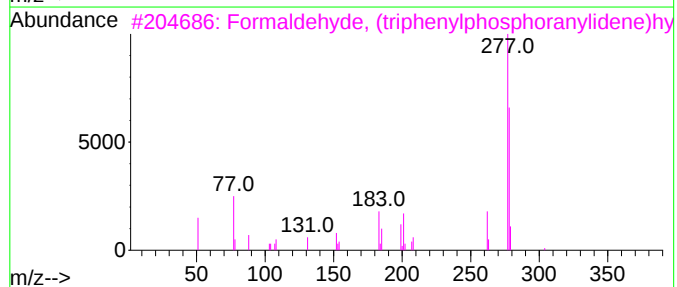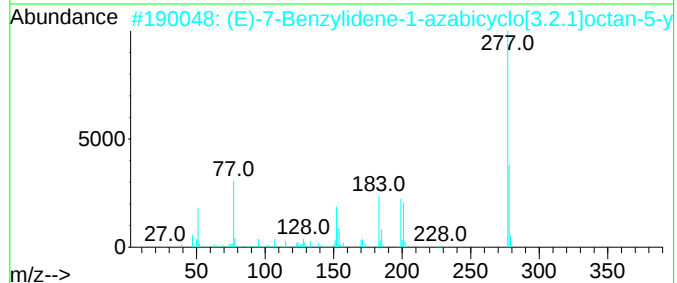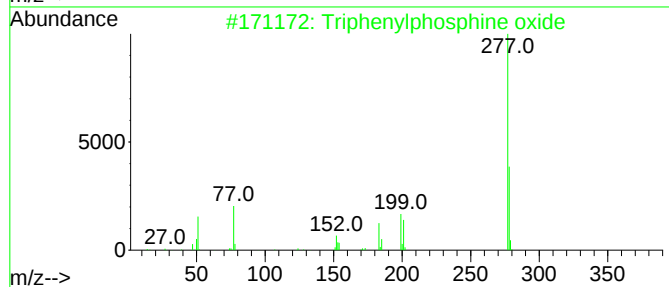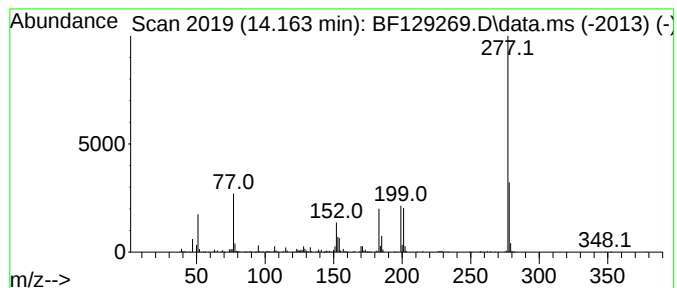

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071822\
Data File : BF129269.D
Acq On : 18 Jul 2022 15:54
Operator : CG\JU
Sample : PB146273BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146273BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.163	3.1	ng	380282	5	14.074	2425010	20.0