

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071822\
 Data File : BF129270.D
 Acq On : 18 Jul 2022 16:26
 Operator : CG\JU
 Sample : PB146277BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146277BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129270.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.057	296	301	306	rVB	141525	180824	1.72%	0.269%
2	5.187	489	493	504	rVB	71574	107282	1.02%	0.160%
3	5.540	547	553	556	rBV	7956759	8750693	83.42%	13.027%
4	6.534	715	722	725	rBV	7002772	9148480	87.22%	13.619%
5	6.898	780	784	788	rBV	2371817	1955335	18.64%	2.911%
6	7.469	874	881	884	rBV	5010050	6139024	58.53%	9.139%
7	8.181	996	1002	1006	rBV	2753193	2747083	26.19%	4.090%
8	9.263	1178	1186	1189	rBV	9688569	10489474	100.00%	15.616%
9	9.939	1295	1301	1305	rBV	3310466	3130035	29.84%	4.660%
10	10.739	1429	1437	1440	rBV	6164631	6773100	64.57%	10.083%
11	11.433	1548	1555	1558	rBV	3500316	3069098	29.26%	4.569%
12	13.022	1820	1825	1828	rBV	8875157	9893205	94.32%	14.728%
13	14.074	2000	2004	2008	rBV	2605491	2418022	23.05%	3.600%
14	14.163	2013	2019	2026	rBV	257028	336397	3.21%	0.501%
15	15.574	2253	2259	2271	rBV	1526979	2035283	19.40%	3.030%




Sum of corrected areas: 67173335

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071822\
Data File : BF129270.D
Acq On : 18 Jul 2022 16:26
Operator : CG\JU
Sample : PB146277BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146277BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

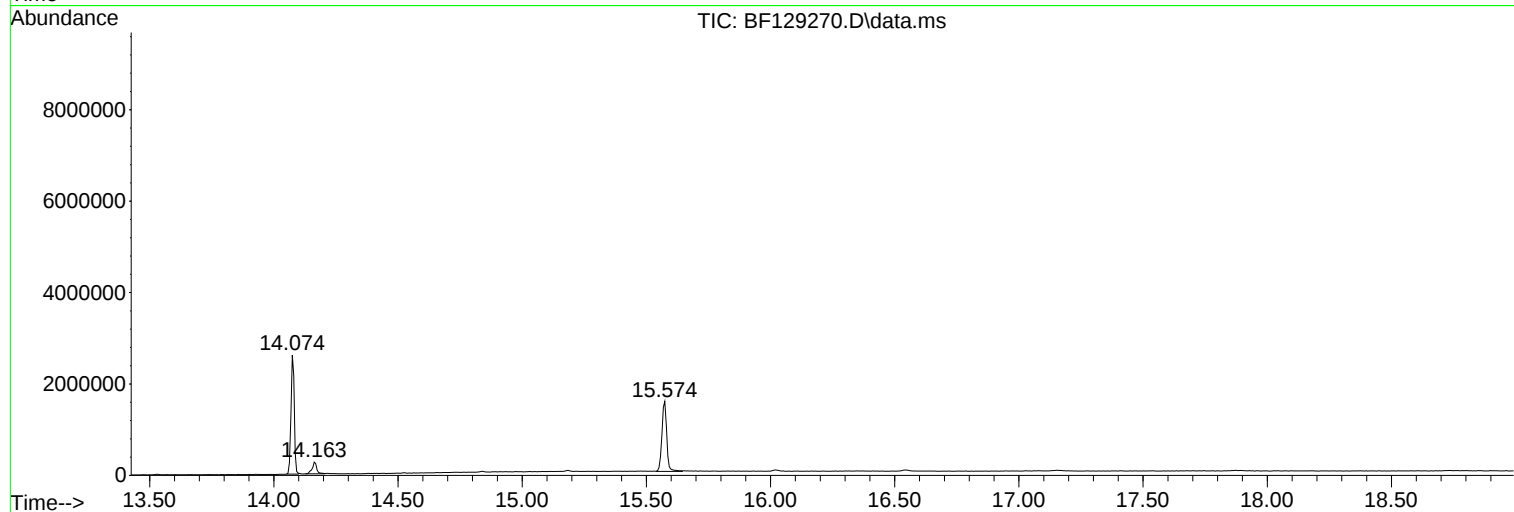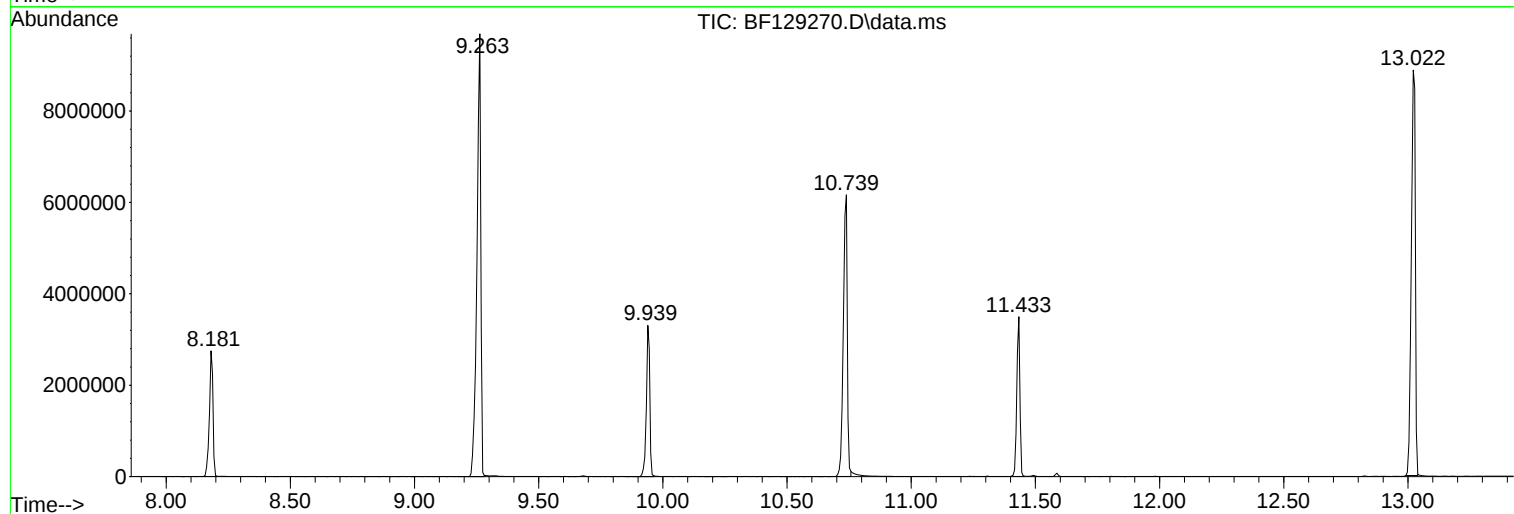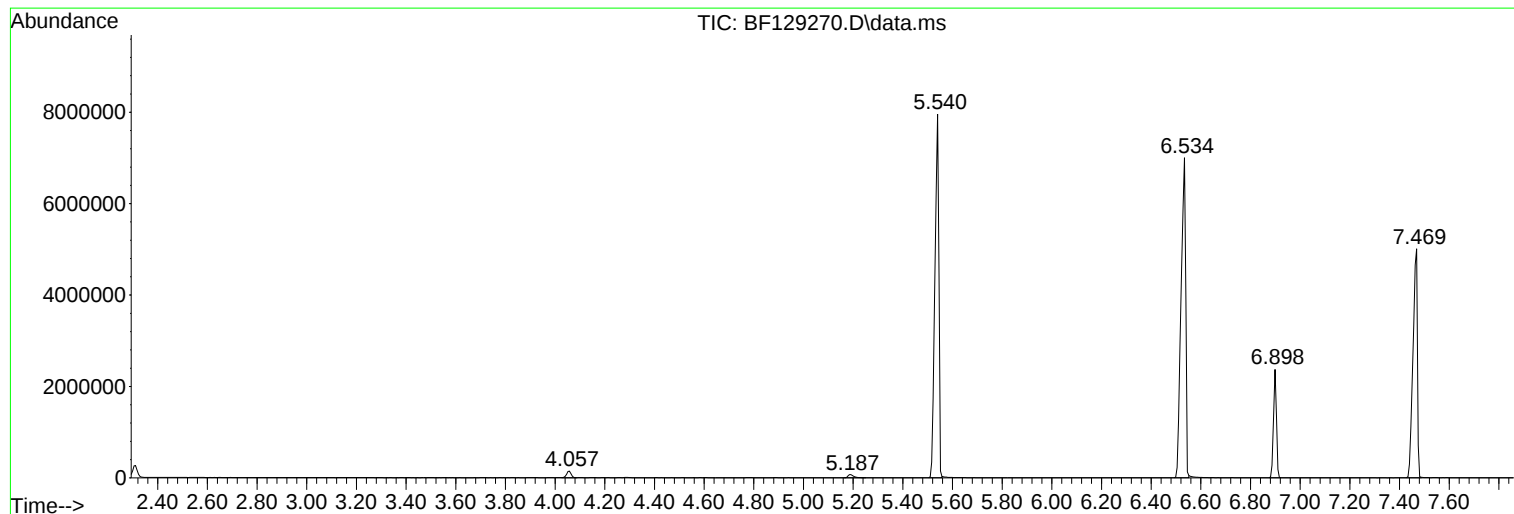

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071822\
Data File : BF129270.D
Acq On : 18 Jul 2022 16:26
Operator : CG\JU
Sample : PB146277BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146277BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.163	2.78 ng	336397	Chrysene-d12	14.074

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	96
2			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19N03S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	64
4			4-Nitro-4'-methyldiphenylsulfone	277	C13H11N04S	004094-37-5	43
5			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	37

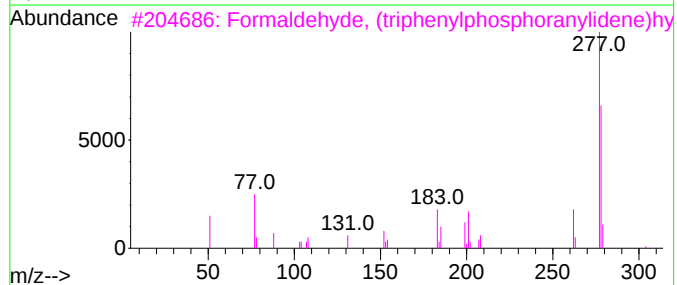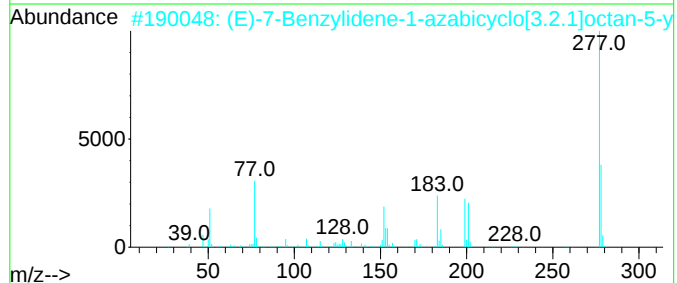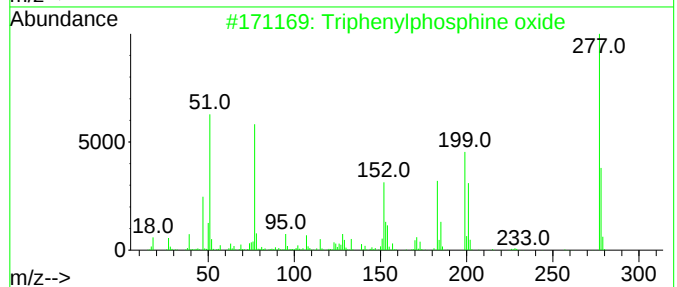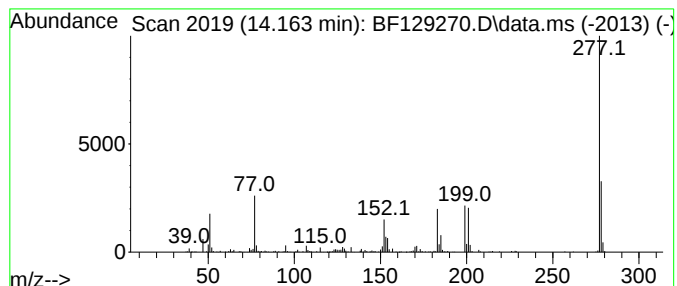

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071822\
Data File : BF129270.D
Acq On : 18 Jul 2022 16:26
Operator : CG\JU
Sample : PB146277BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146277BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.163	2.8	ng	336397	5	14.074	2418020	20.0