
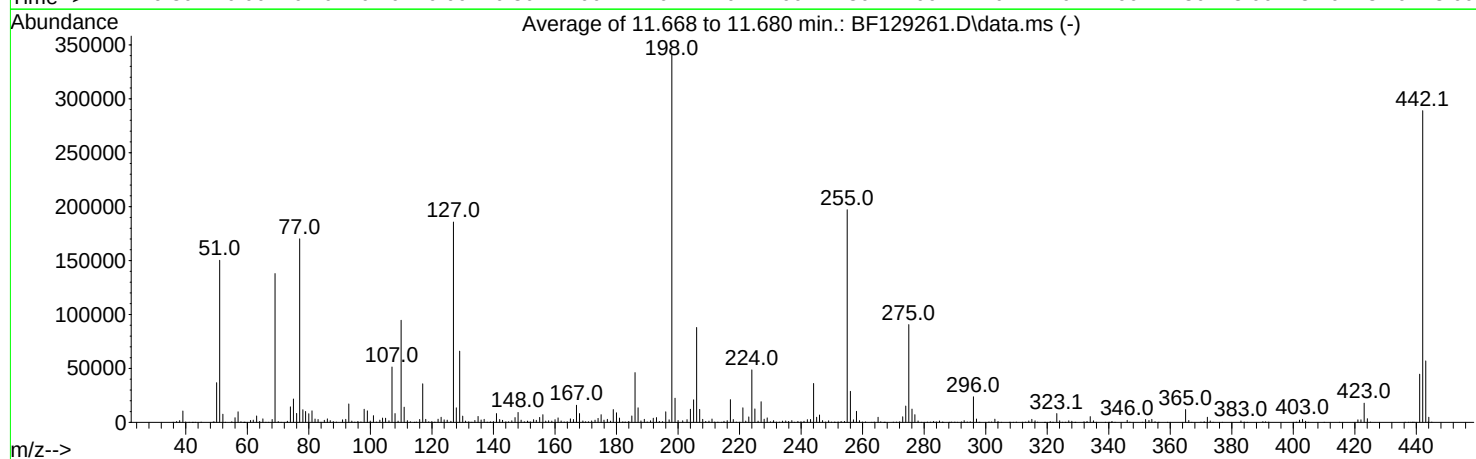


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071822\
 Data File : BF129261.D
 Acq On : 18 Jul 2022 09:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 15 12:55:49 2022

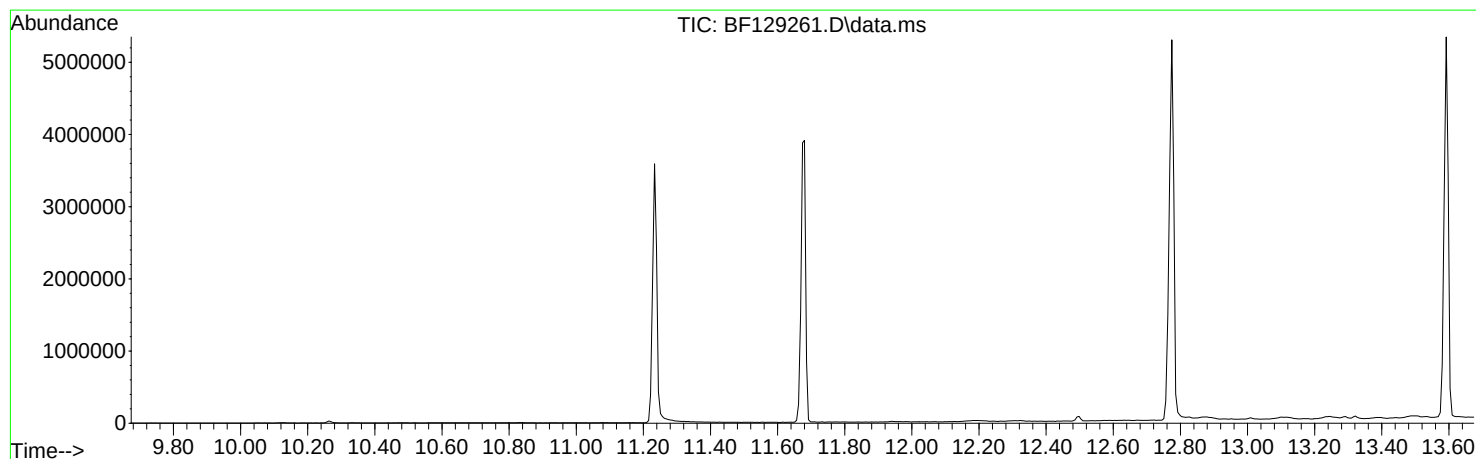




AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.1	150283	PASS
68	69	0.00	2	1.9	2630	PASS
69	198	0.00	100	40.5	137992	PASS
70	69	0.00	2	0.5	731	PASS
127	198	10	80	54.5	185707	PASS
197	198	0.00	2	0.7	2374	PASS
198	198	100	100	100.0	341035	PASS
199	198	5	9	6.6	22403	PASS
275	198	10	60	26.6	90640	PASS
365	198	1	100	3.5	11941	PASS
441	198	0.01	100	13.1	44605	PASS
442	442	50	100	100.0	289019	PASS
443	442	15	24	19.7	56976	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071822\
Data File : BF129261.D
Acq On : 18 Jul 2022 09:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 19 05:42:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 12:55:49 2022
Response via : Initial Calibration

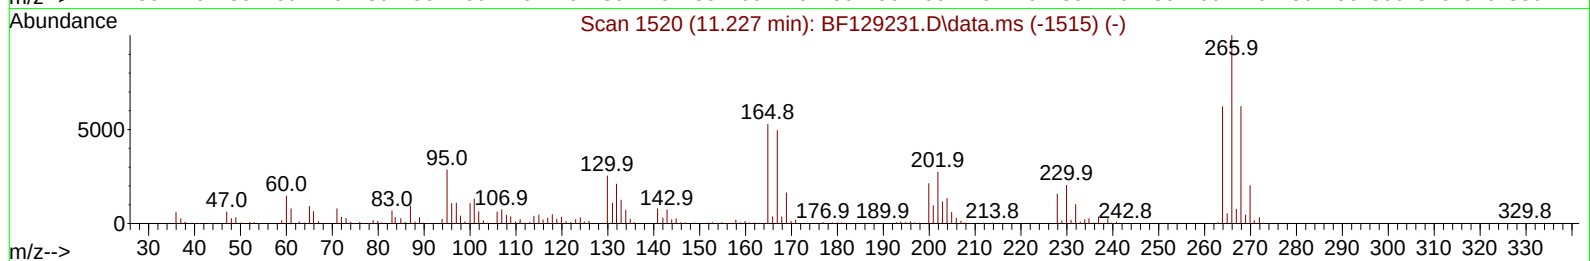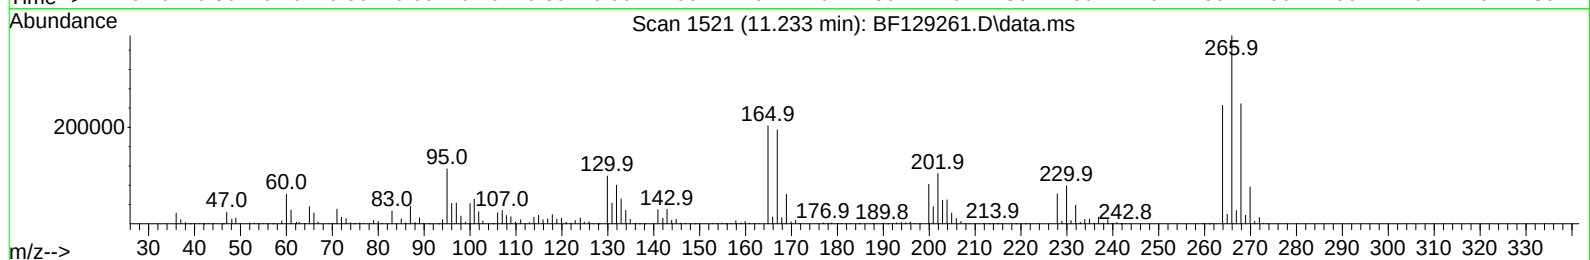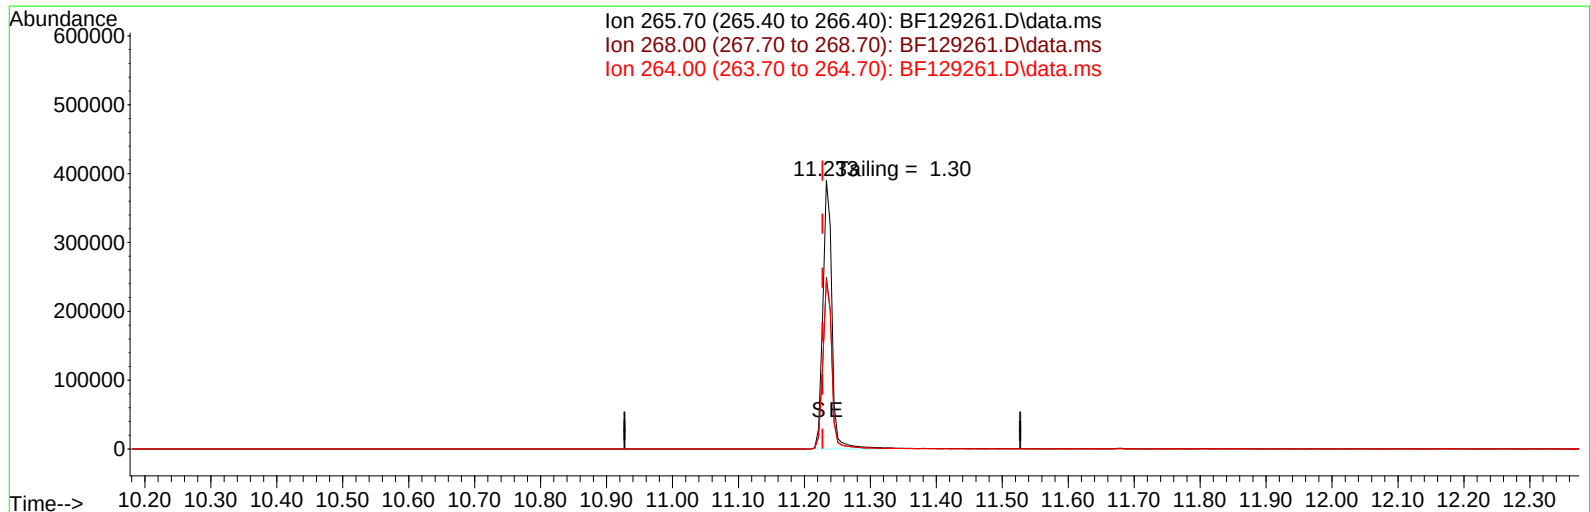

TIC: BF129261.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.006) 178710.46 ng




response 375758

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.86
264.00	61.80	62.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071822\
 Data File : BF129261.D
 Acq On : 18 Jul 2022 09:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 19 05:42:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 15 12:55:49 2022
 Response via : Initial Calibration

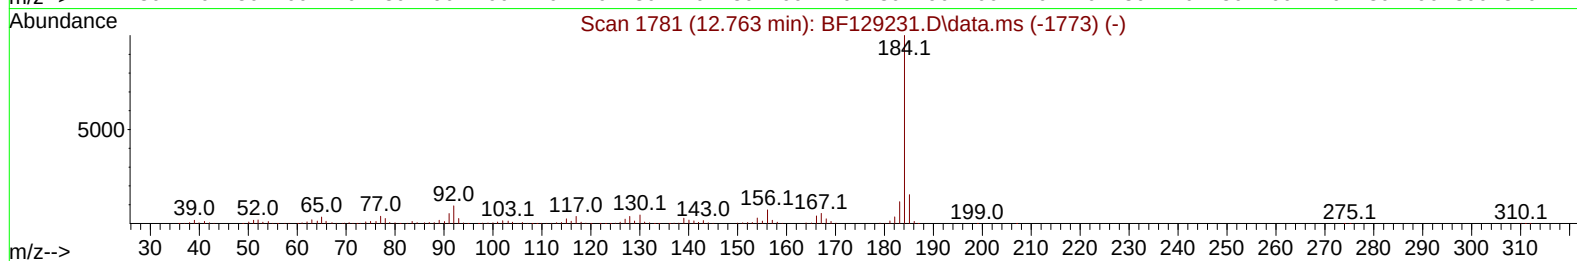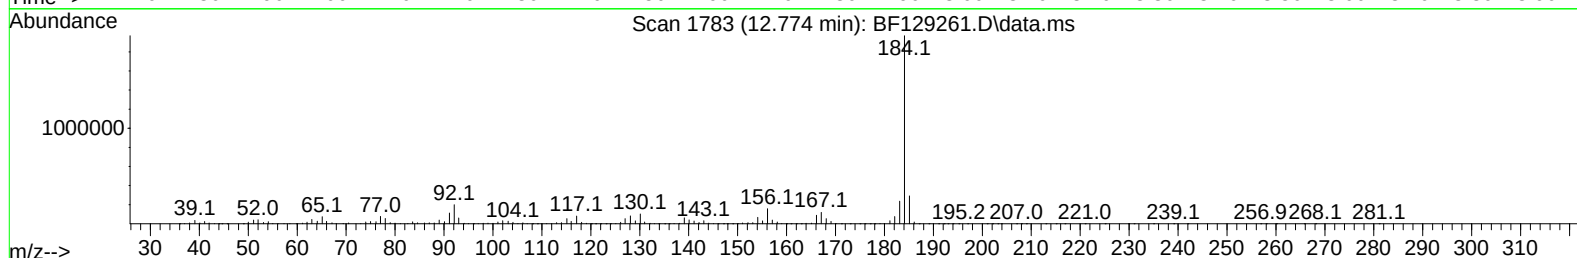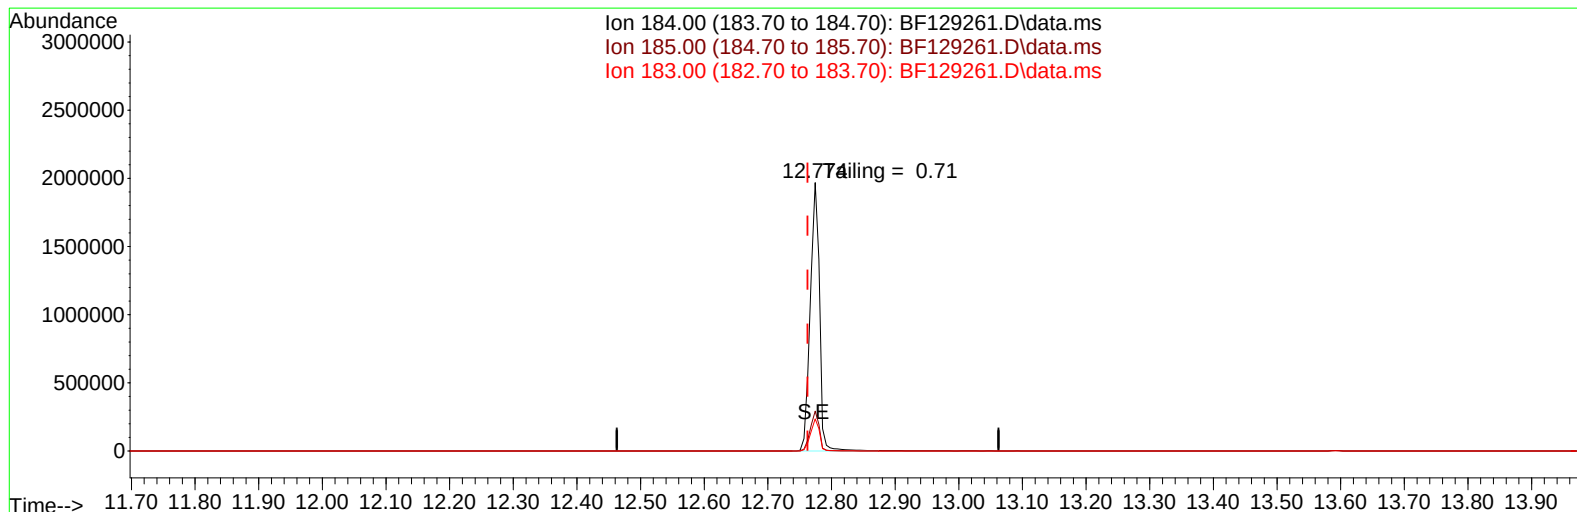

TIC: BF129261.D\data.ms

(77) Benzidine

12.774min (+ 0.012) 78602.07 ng

response 2010994

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.84
183.00	11.60	12.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/18/2022	BNA_F	<u>BF129261.D</u>
Compound Name	Response	Retention Time
DDT	845683	13.592
DDD	10021	13.321
DDE	1070	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11091	856774	1.29

Instrument :
BNA_F
ClientSampleId :
DFTPP