
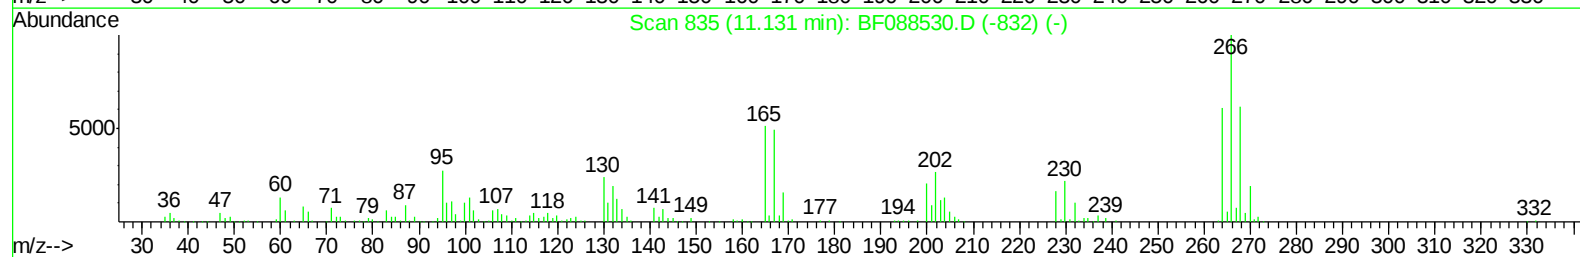
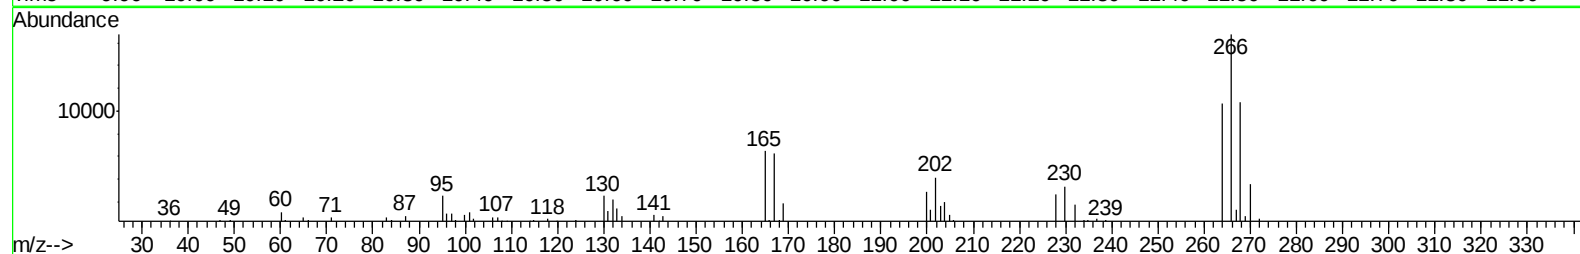


Data Path : Z:\HPCHEM1\BNA F\Data\BF071916\
Data File : BF089109.D
Acq On : 19 Jul 2016 10:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 18:05:55 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 19 15:28:17 2016
Response via : Initial Calibration

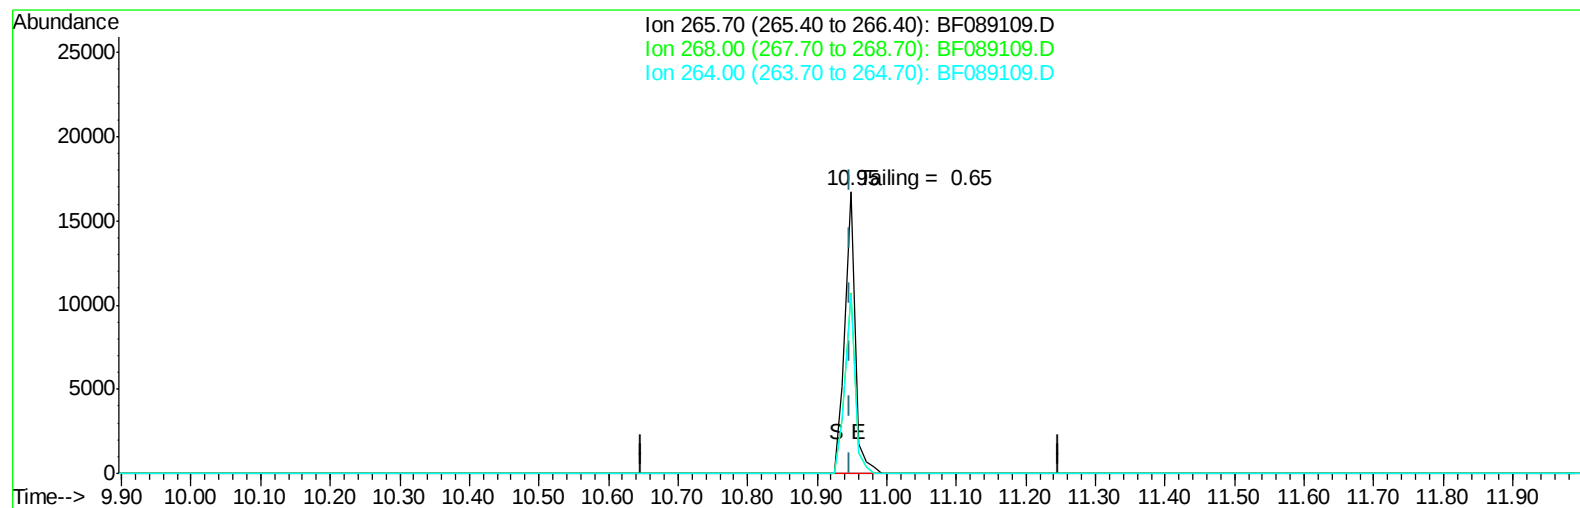

TIC: BF089109.D

(69) Pentachlorophenol (C)




10.948min (-0.000) 0.00ng

response 16952

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	64.31
264.00	62.00	63.43
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF071916\
Data File : BF089109.D
Acq On : 19 Jul 2016 10:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 18:05:55 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 19 15:28:17 2016
Response via : Initial Calibration

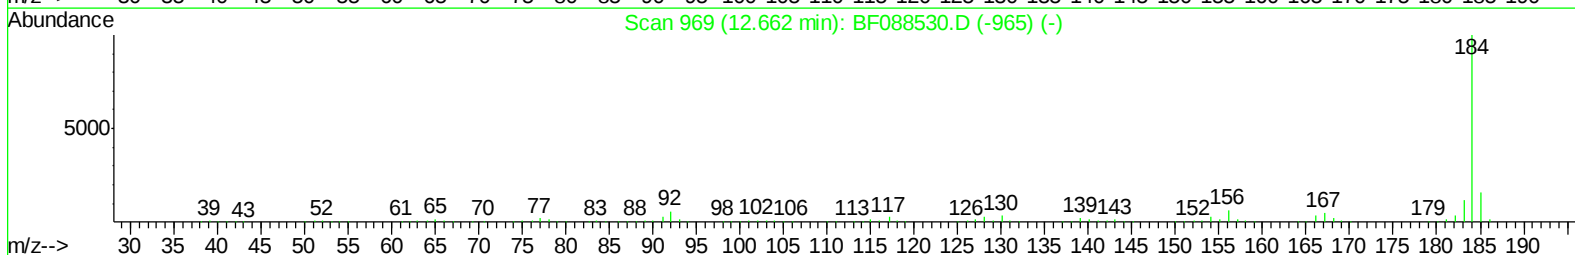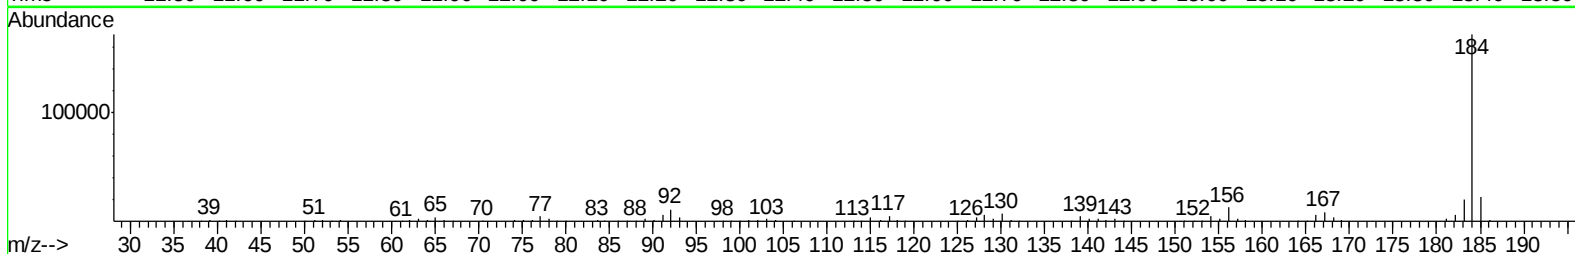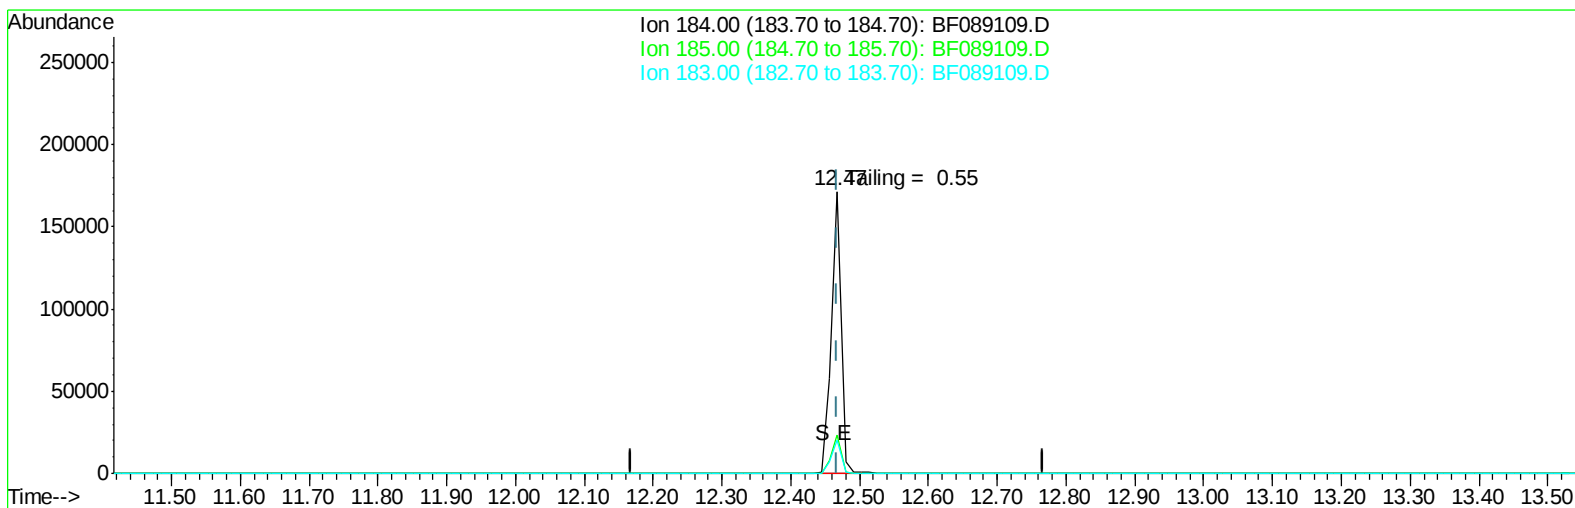

TIC: BF089109.D

(76) Benzidine

12.468min (-0.000) 0.00ng

response 164348

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	13.54
183.00	11.60	11.86
0.00	0.00	0.00