


Data Path : Z:\HPCHEM1\BNA F\Data\BF071916\
 Data File : BF089109.D
 Acq On : 19 Jul 2016 10:47
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 19 15:28:17 2016

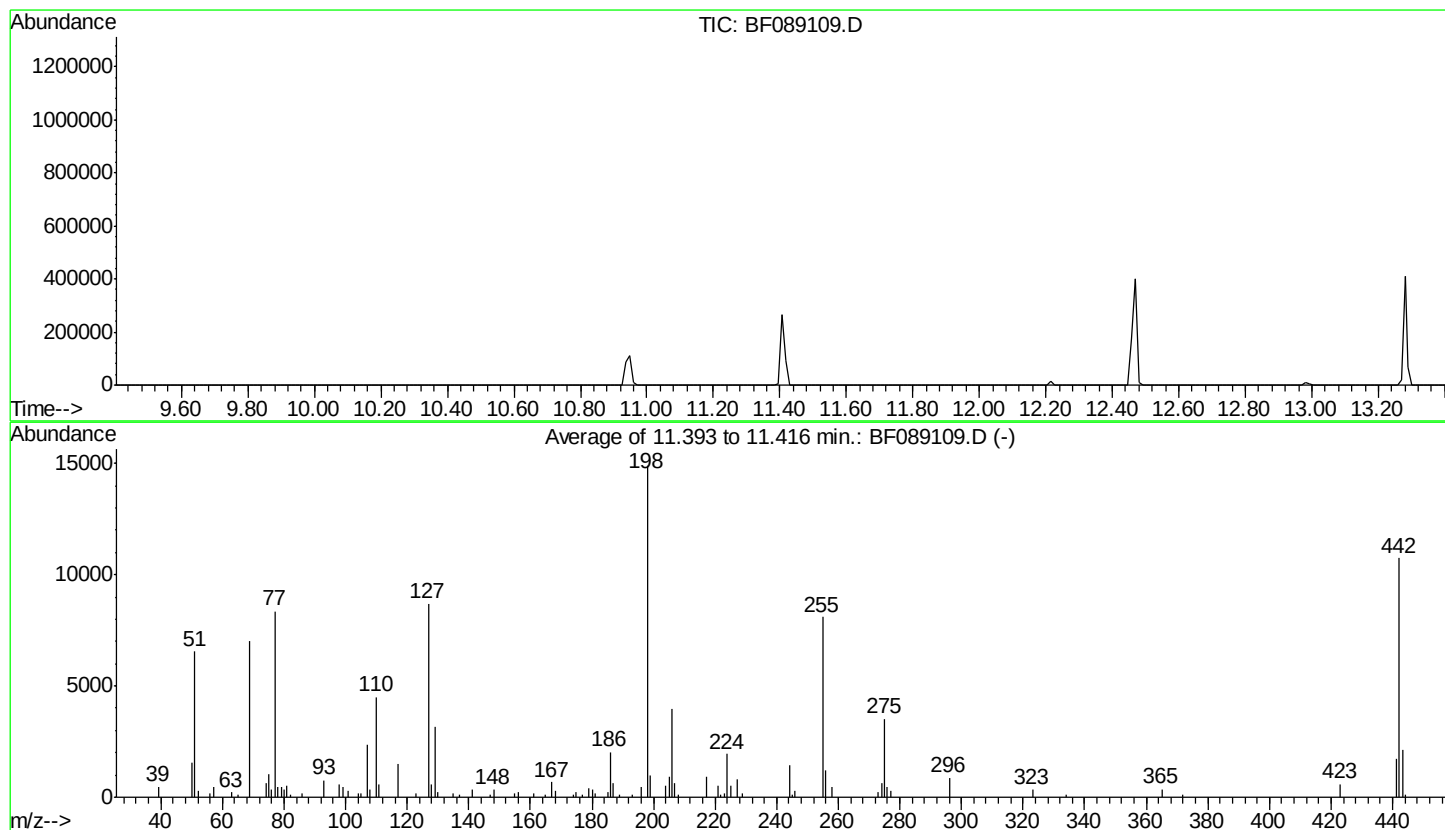

AutoFind: Scans 858, 859, 860; Background Corrected with Scan 855

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.0	6557	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.9	6993	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	58.4	8708	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14901	PASS
199	198	5	9	6.5	976	PASS
275	198	10	60	23.7	3525	PASS
365	198	1	100	2.4	362	PASS
441	442	0.01	24	16.1	1727	PASS
442	198	50	100	72.0	10732	PASS
443	442	15	24	19.9	2139	PASS