
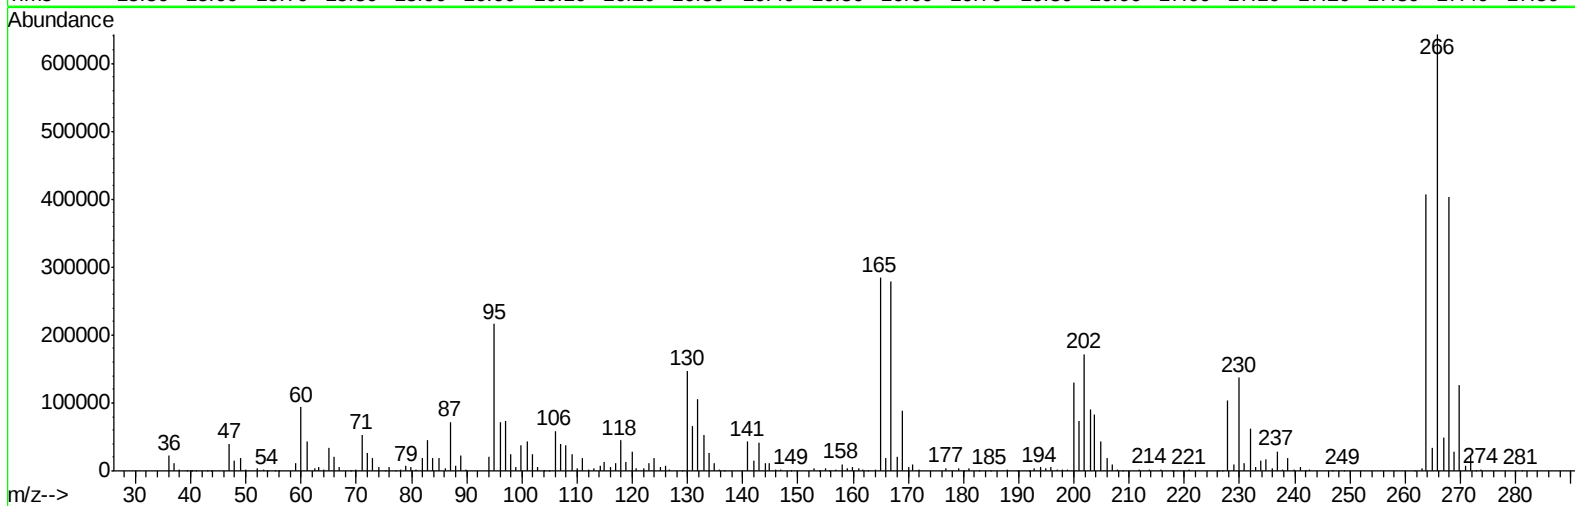


Data Path : Z:\HPCHEM1\BNA M\DATA\BM071917\
Data File : BM010888.D
Acq On : 19 Jul 2017 11:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jul 20 02:00:07 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

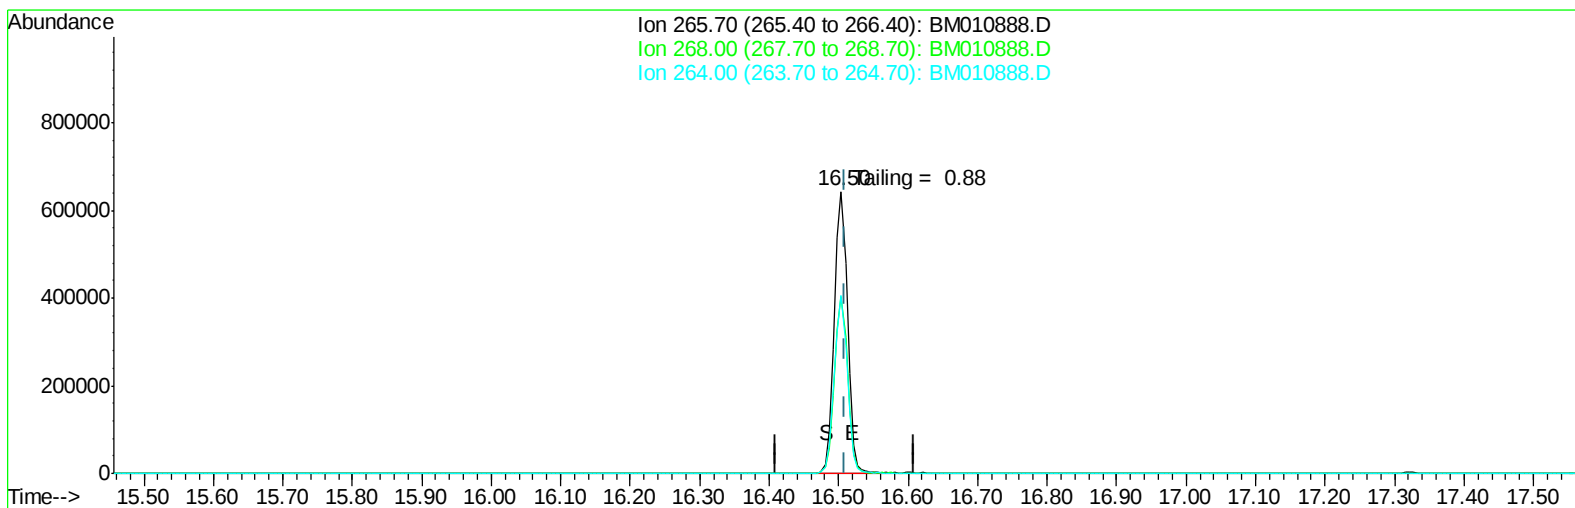

TIC: BM010888.D

(69) Pentachlorophenol (C)

16.504min (-0.006) 45040.41ng



response 848565

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.78
264.00	61.20	63.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071917\
Data File : BM010888.D
Acq On : 19 Jul 2017 11:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jul 20 02:00:07 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

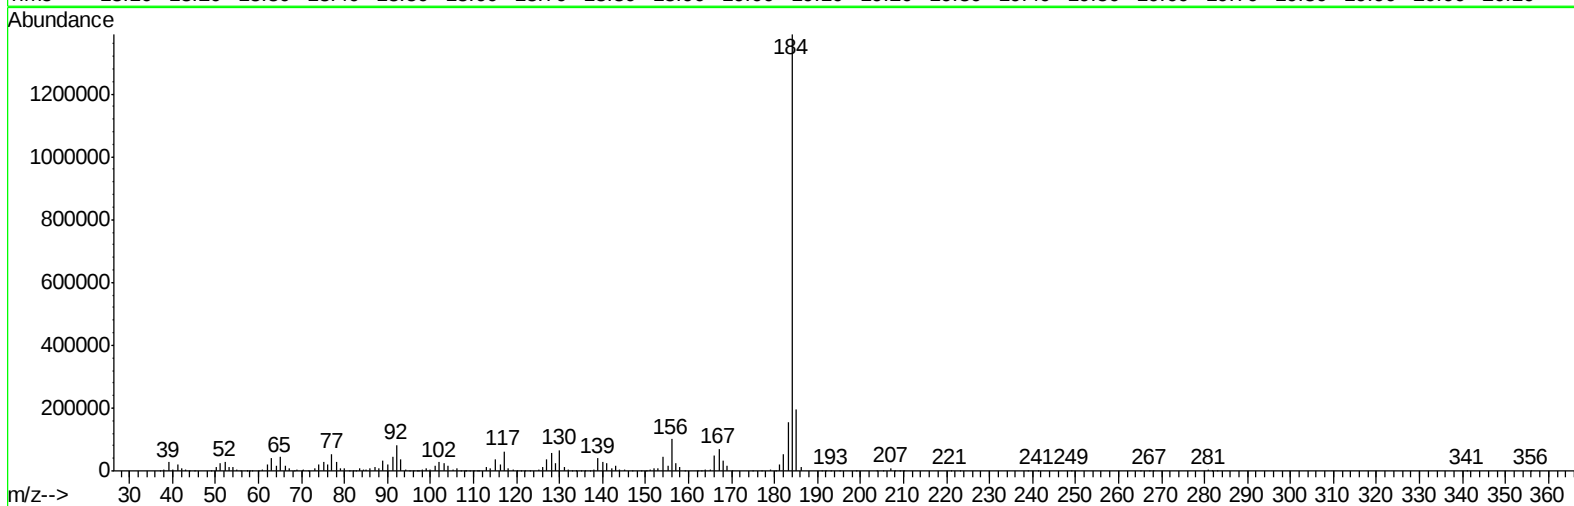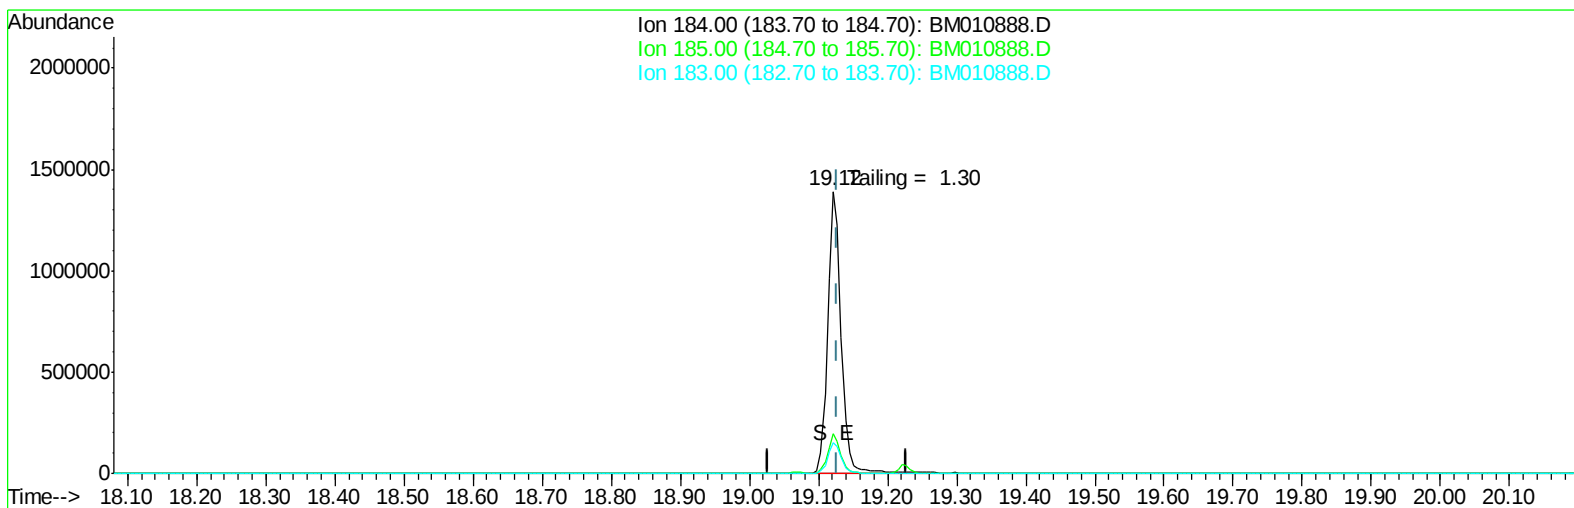

TIC: BM010888.D

(76) Benzidine

19.121min (-0.006) 2482.93ng



response 1862752

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.96
183.00	11.10	11.13
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071917\
Data File : BM010888.D
Acq On : 19 Jul 2017 11:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jul 20 02:00:07 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

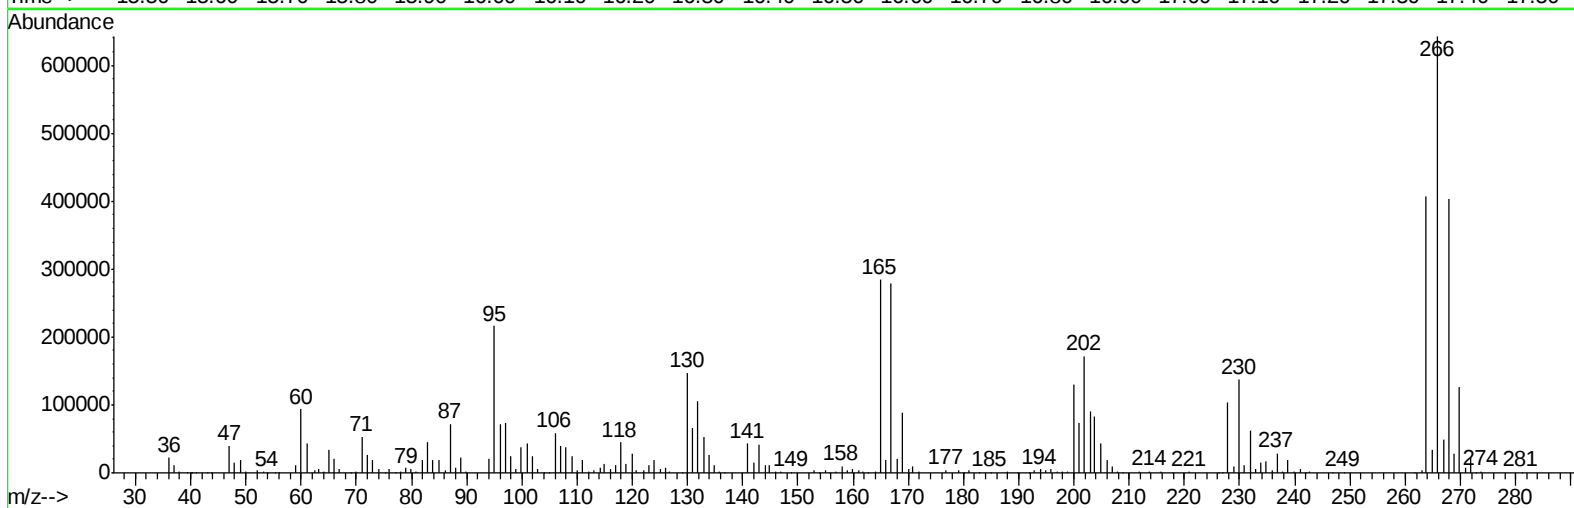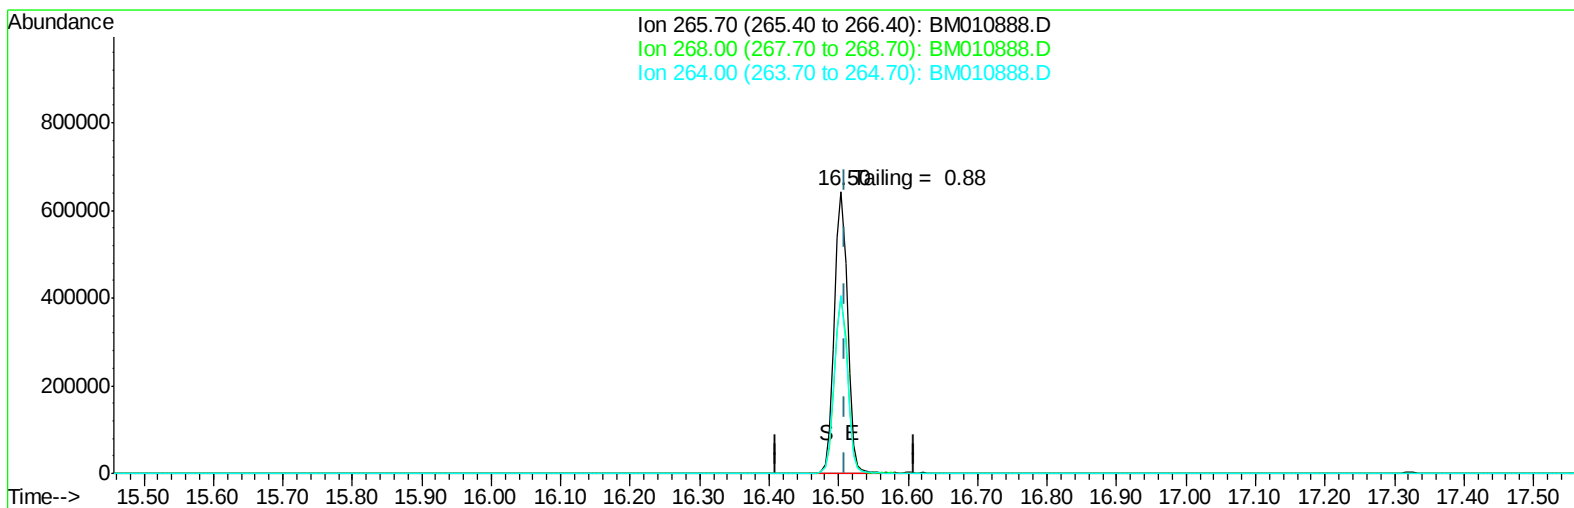

TIC: BM010888.D

(69) Pentachlorophenol (C)

16.504min (-0.006) 45040.41ng



response 848565

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.78
264.00	61.20	63.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071917\
Data File : BM010888.D
Acq On : 19 Jul 2017 11:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jul 20 03:35:06 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

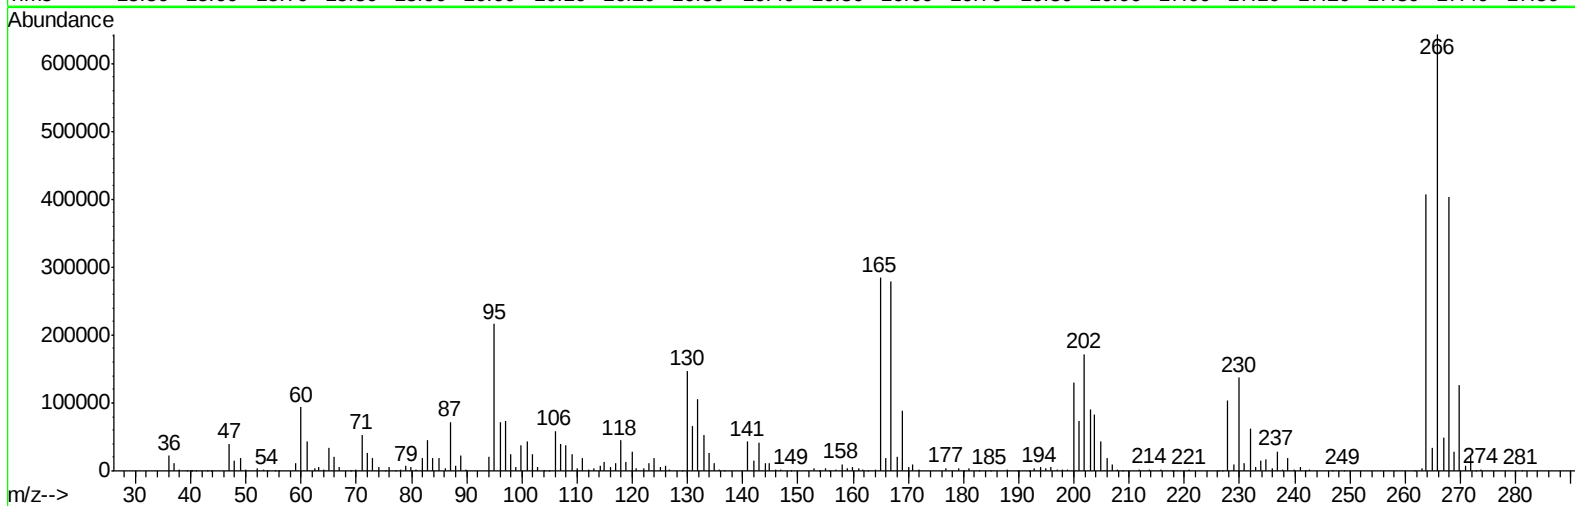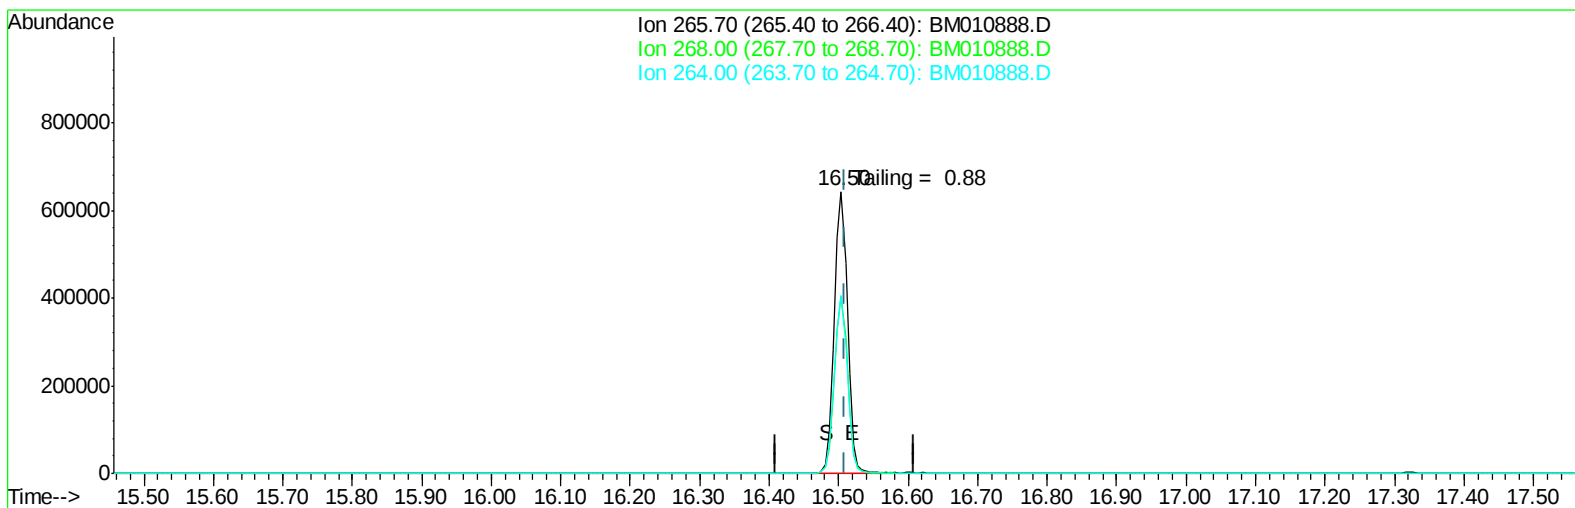

TIC: BM010888.D

(69) Pentachlorophenol (C)

16.504min (-0.006) 45040.41ng



response 848565

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.78
264.00	61.20	63.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071917\
Data File : BM010888.D
Acq On : 19 Jul 2017 11:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jul 20 03:35:06 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

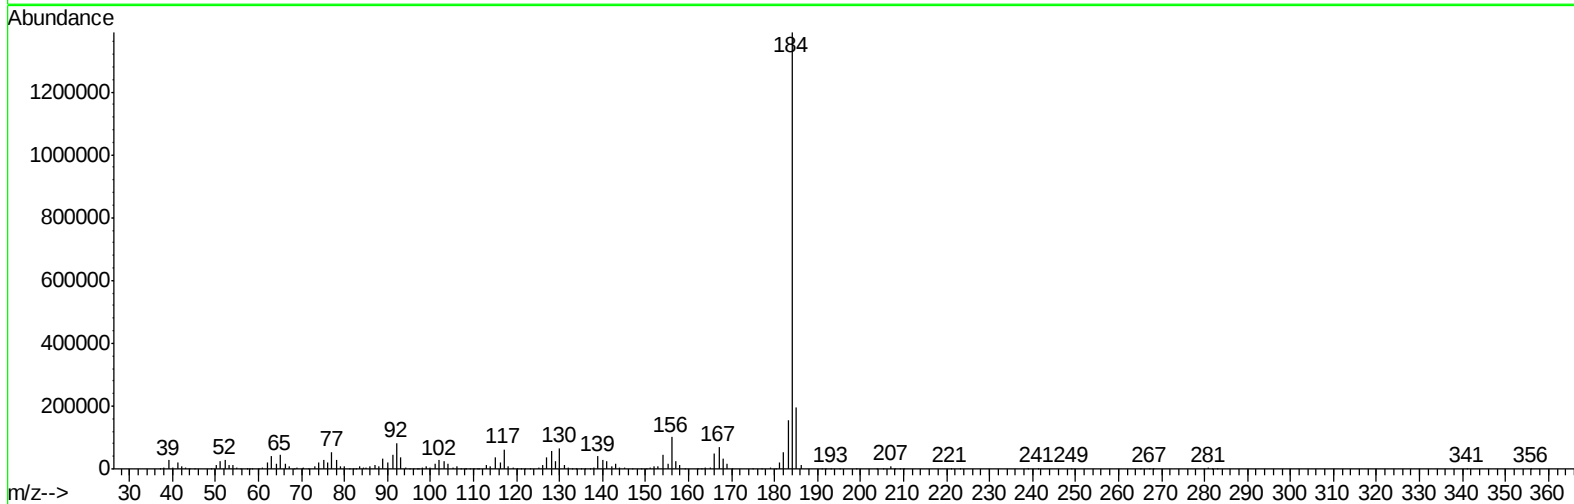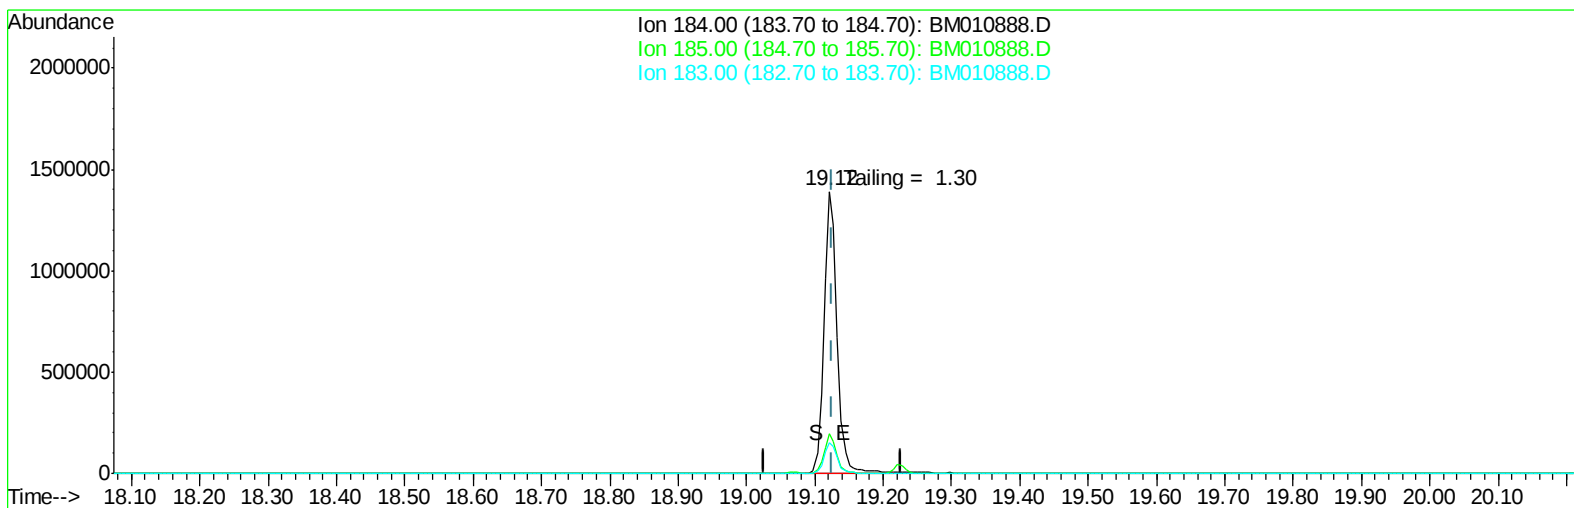

TIC: BM010888.D

(76) Benzidine

19.121min (-0.006) 2495.22ng m



response 1871973

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.96
183.00	11.10	11.13
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM071917\
Data File : BM010888.D
Acq On : 19 Jul 2017 11:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jul 20 03:45:58 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM071217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 14:21:16 2017
Response via : Initial Calibration

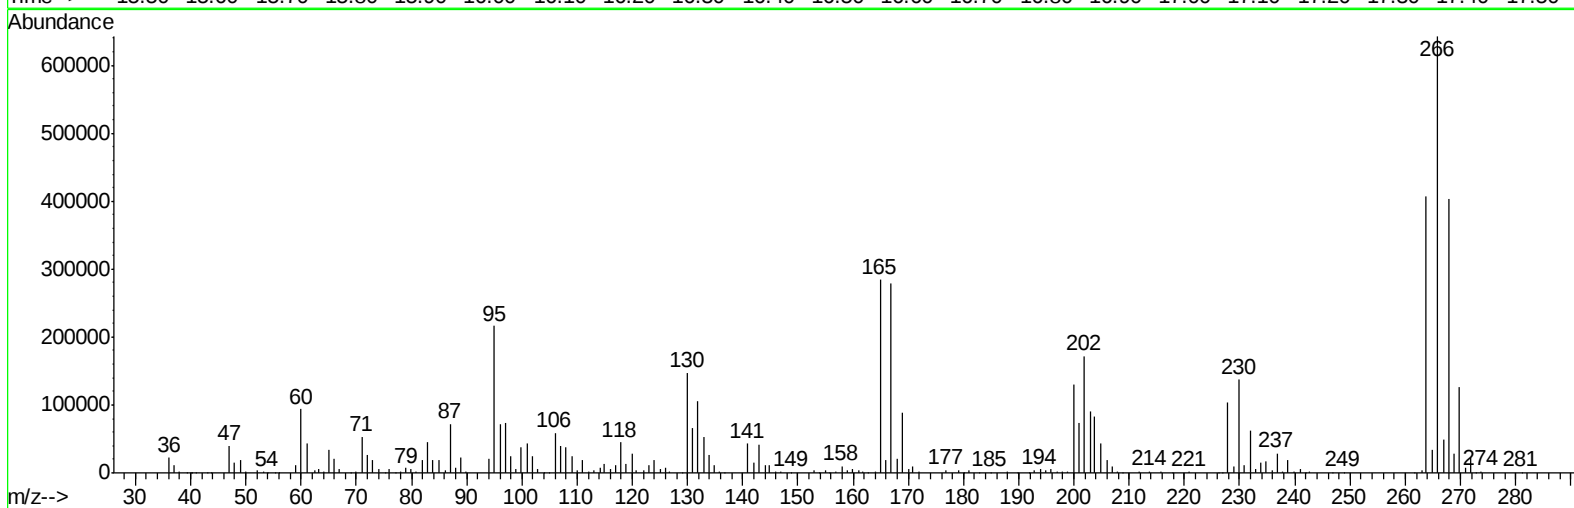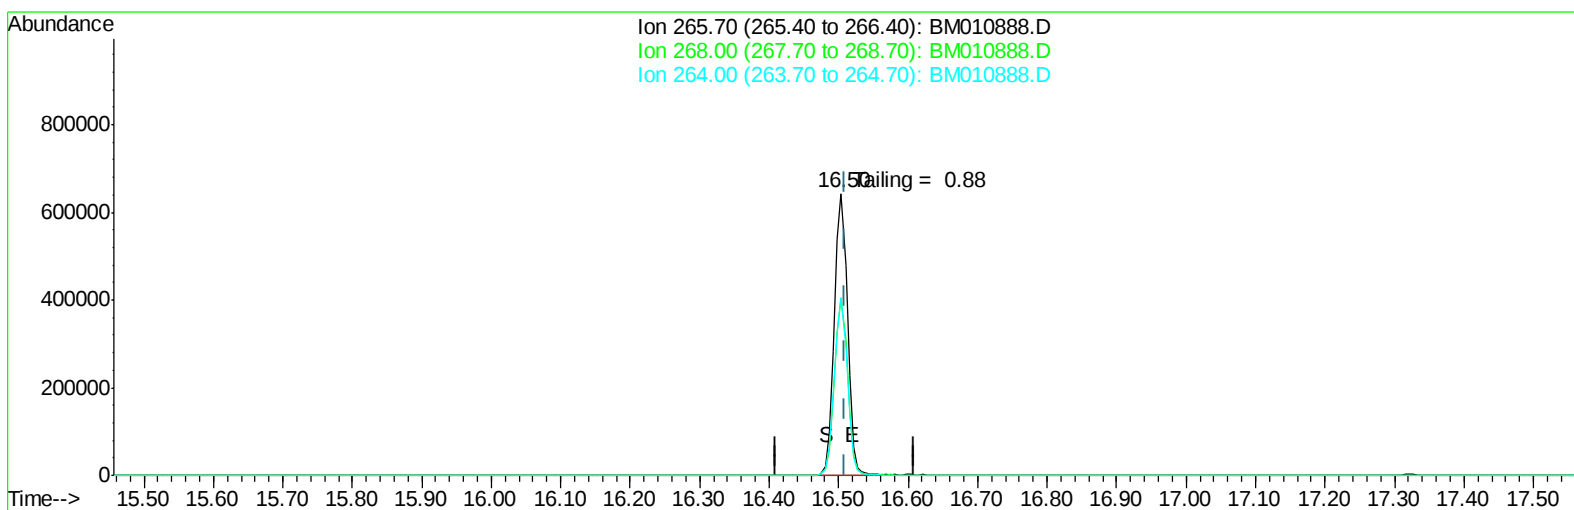

TIC: BM010888.D

(69) Pentachlorophenol (C)

16.504min (-0.006) 45040.41ng

response 848565

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.78
264.00	61.20	63.25
0.00	0.00	0.00