
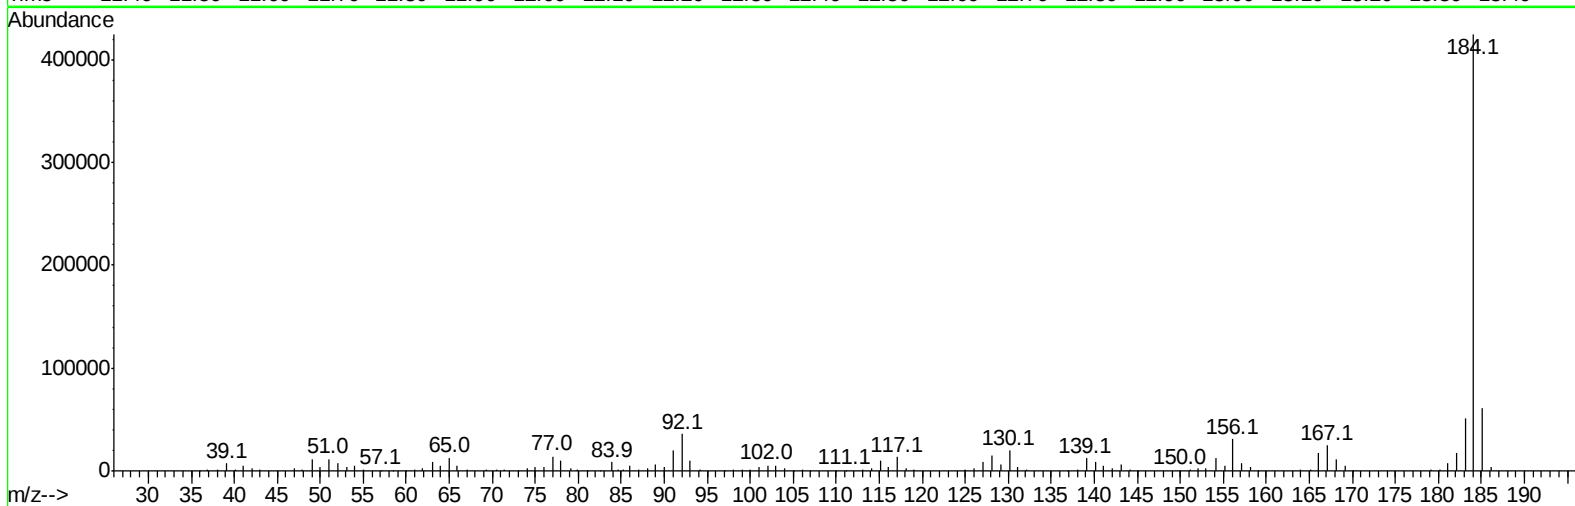


Data Path : Z:\HPCHEM1\BNA F\Data\BF071917\
Data File : BF096867.D
Acq On : 19 Jul 2017 13:52
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 08:15:39 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 18 13:33:22 2017
Response via : Initial Calibration

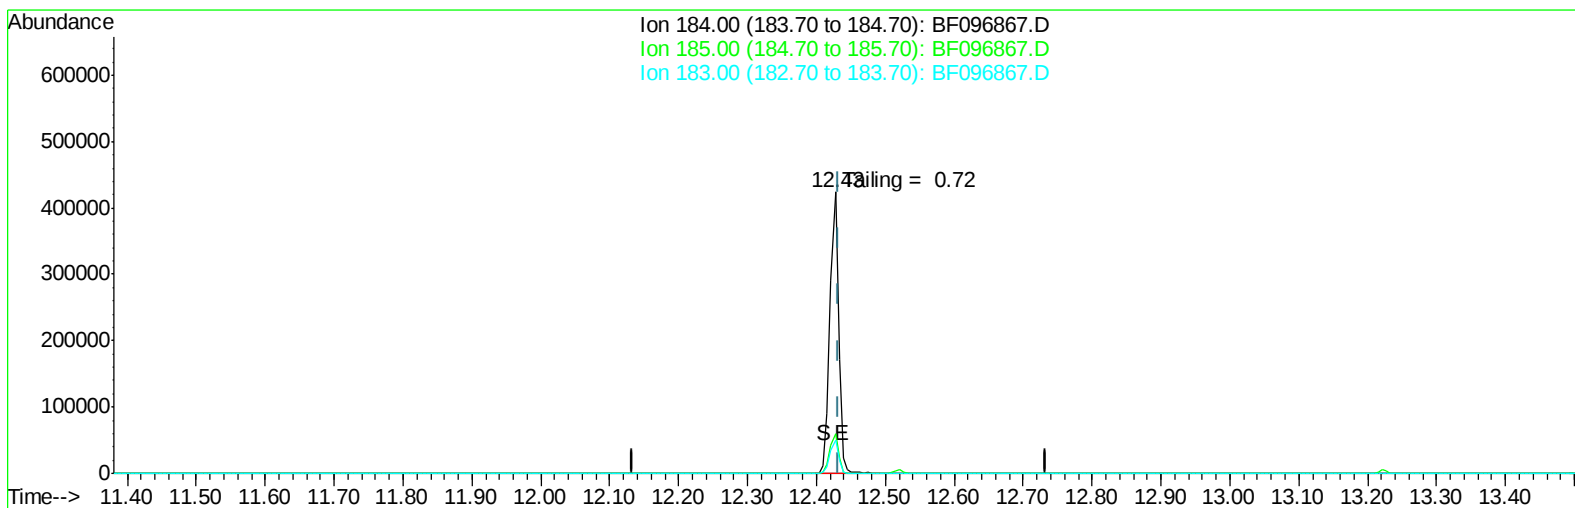

TIC: BF096867.D

(76) Benzidine



12.427min (-0.006) 17070.72ng

response 364068

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.24#
183.00	12.20	11.91
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF071917\
Data File : BF096867.D
Acq On : 19 Jul 2017 13:52
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 08:15:39 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 18 13:33:22 2017
Response via : Initial Calibration

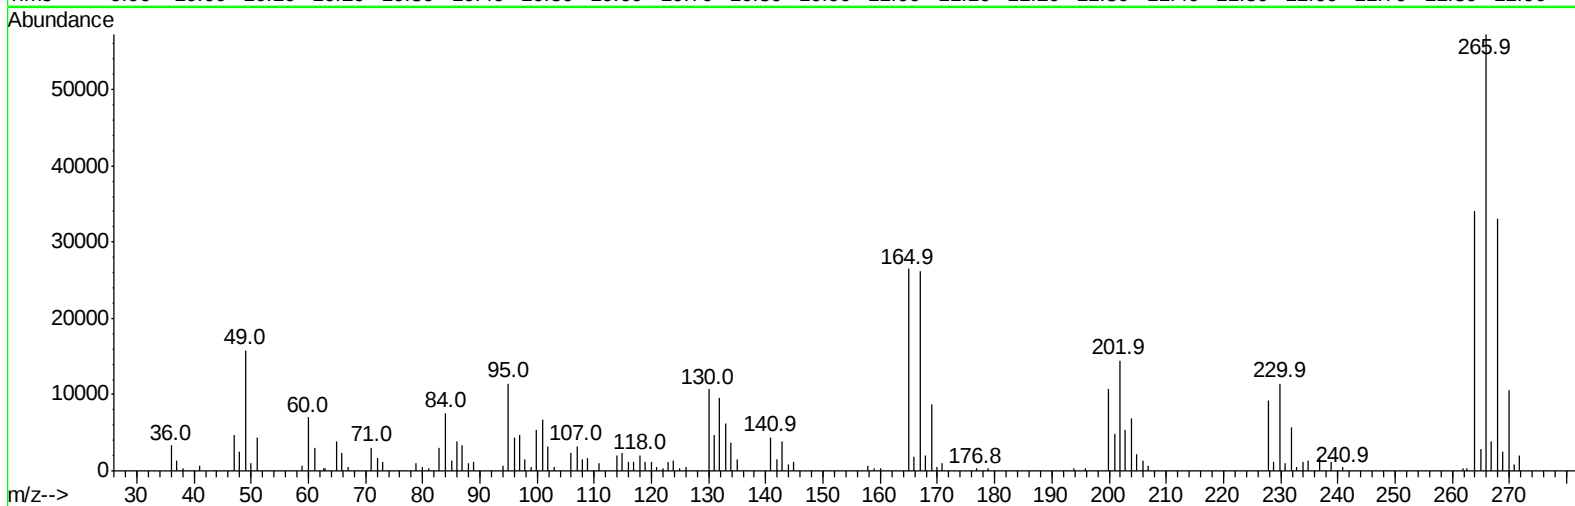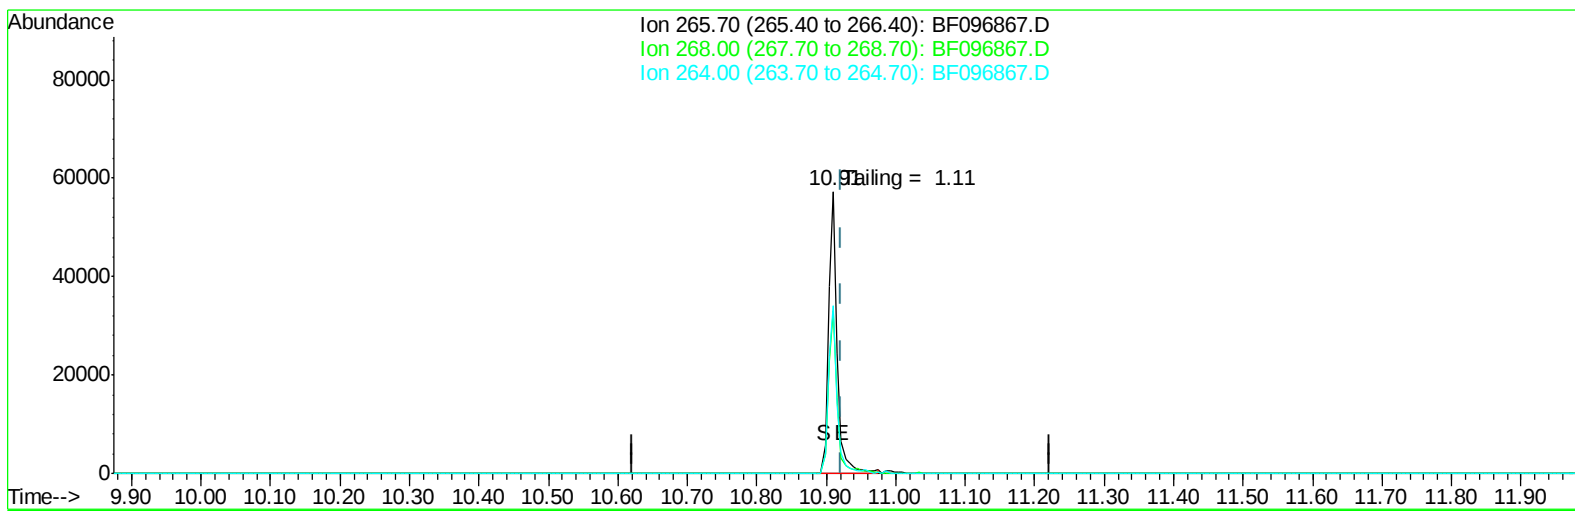

TIC: BF096867.D

(69) Pentachlorophenol (C)

10.910min (-0.012) 82929.10ng

response 50111

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	57.72
264.00	64.60	59.45
0.00	0.00	0.00