
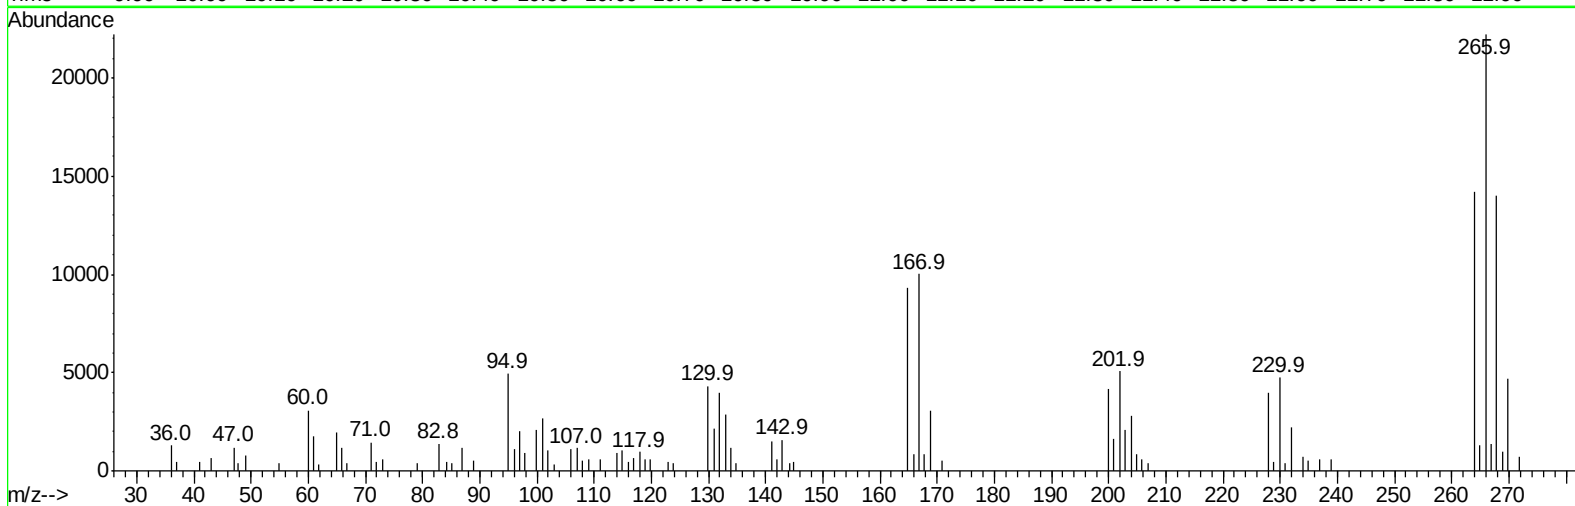


Data Path : Z:\HPCHEM1\BNA F\Data\BF071917\
Data File : BF096892.D
Acq On : 20 Jul 2017 2:31
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 08:17:45 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 18 13:33:22 2017
Response via : Initial Calibration

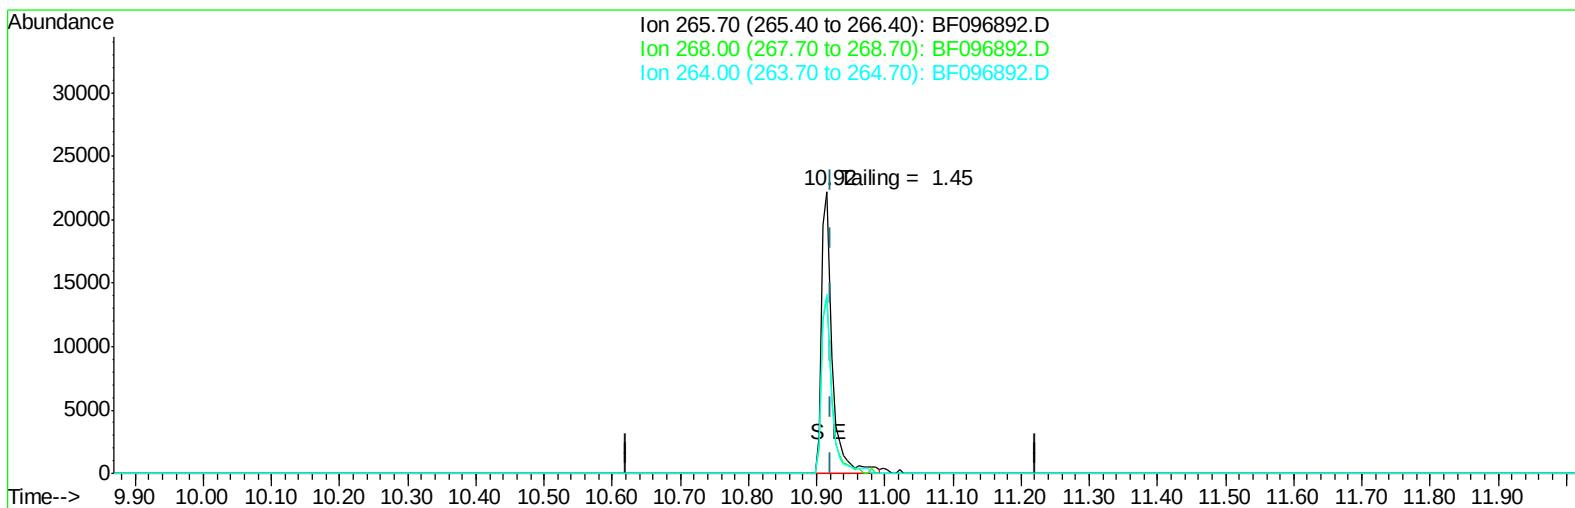

TIC: BF096892.D

(69) Pentachlorophenol (C)



10.916min (-0.006) 30827.16ng

response 23708

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.95
264.00	64.60	63.83
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF071917\
 Data File : BF096892.D
 Acq On : 20 Jul 2017 2:31
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 08:17:45 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 18 13:33:22 2017
 Response via : Initial Calibration

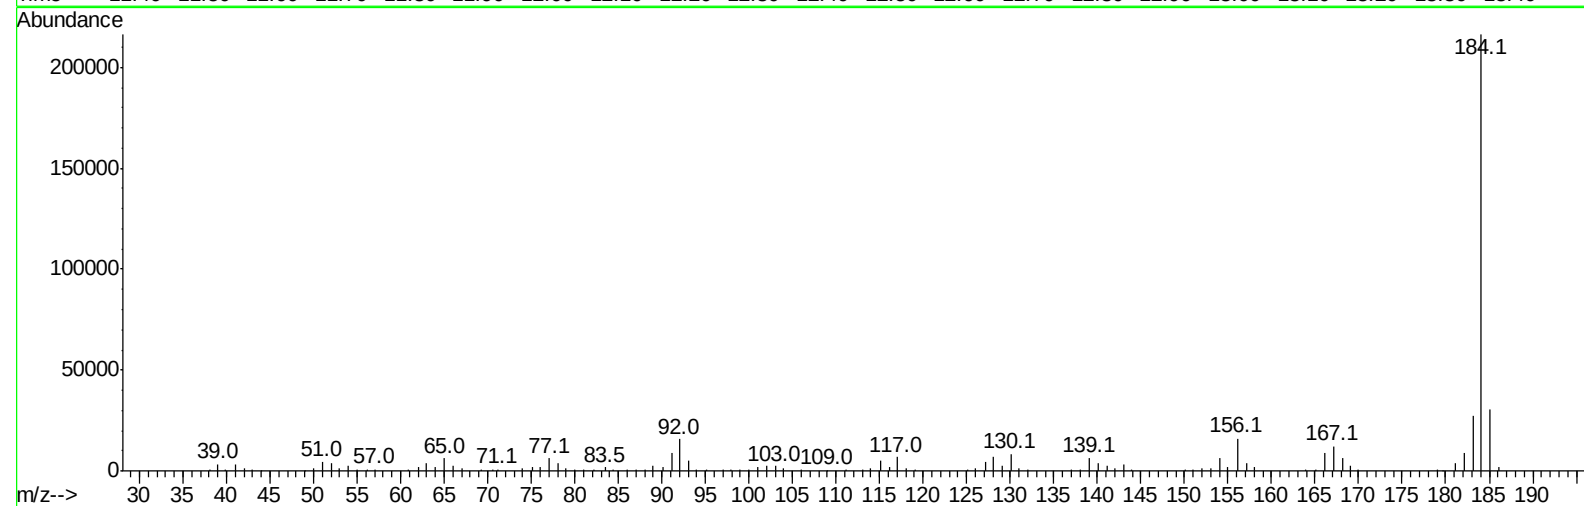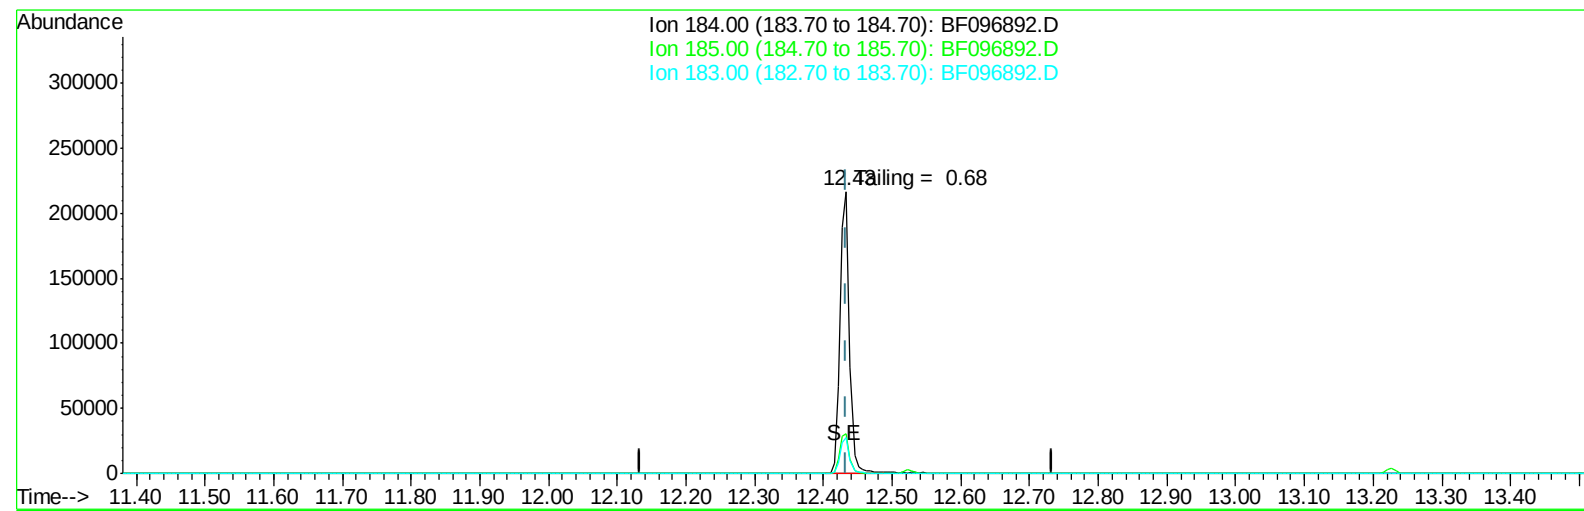

TIC: BF096892.D

(76) Benzidine

12.433min (-0.000) 0.00ng

response 209843

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.95#
183.00	12.20	12.67
0.00	0.00	0.00