
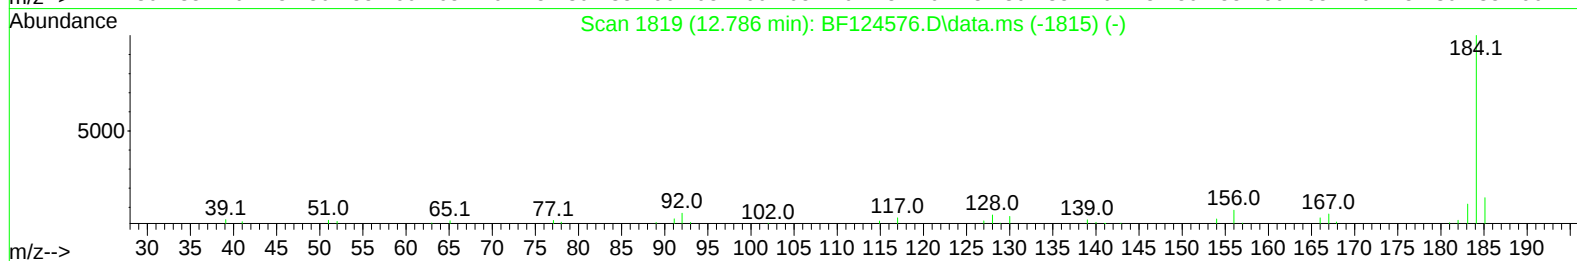
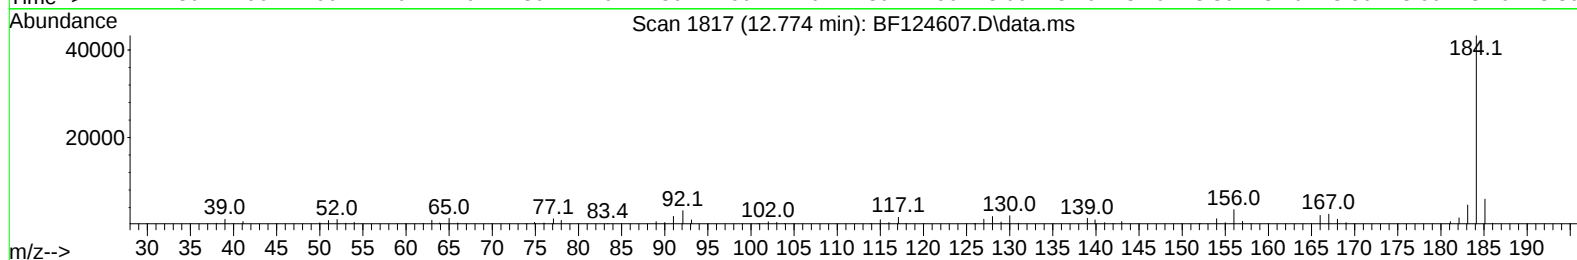


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071921\
Data File : BF124607.D
Acq On : 19 Jul 2021 10:24
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 11:14:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 08 07:53:19 2021
Response via : Initial Calibration

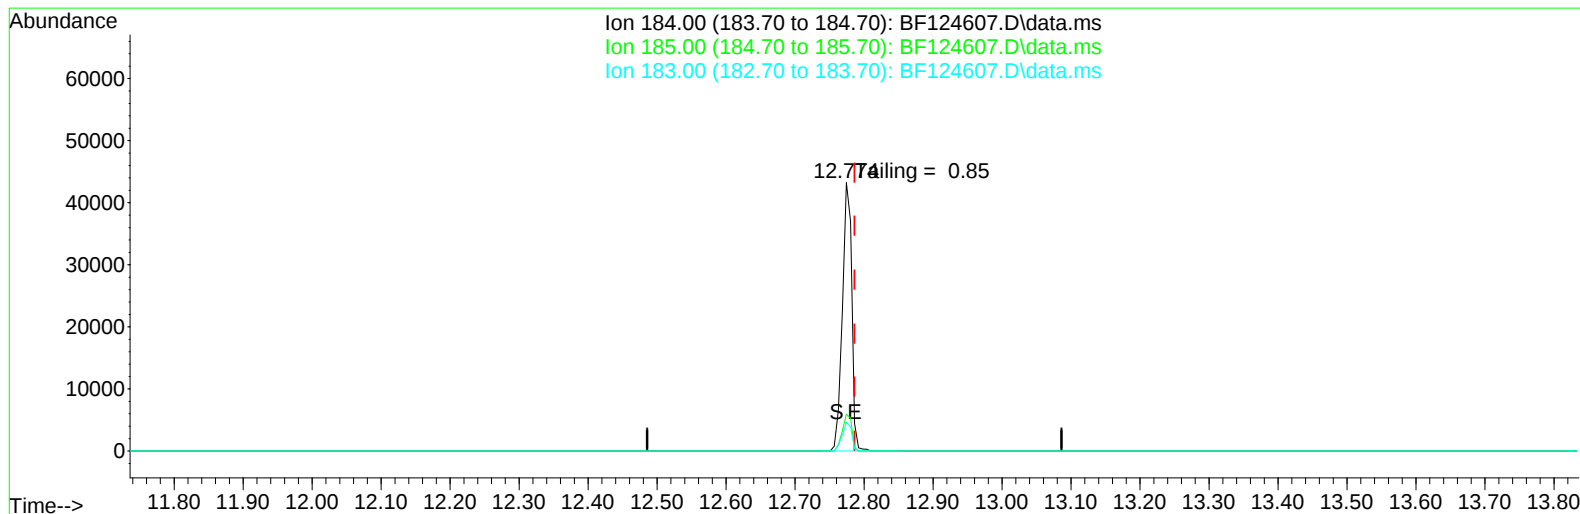

TIC: BF124607.D\data.ms

(77) Benzidine




12.774min (-0.012) 0.00 ng

response 40876

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.73
183.00	10.10	10.60
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071921\  
Data File : BF124607.D  
Acq On    : 19 Jul 2021  10:24  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jul 19 11:14:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 08 07:53:19 2021
Response via : Initial Calibration

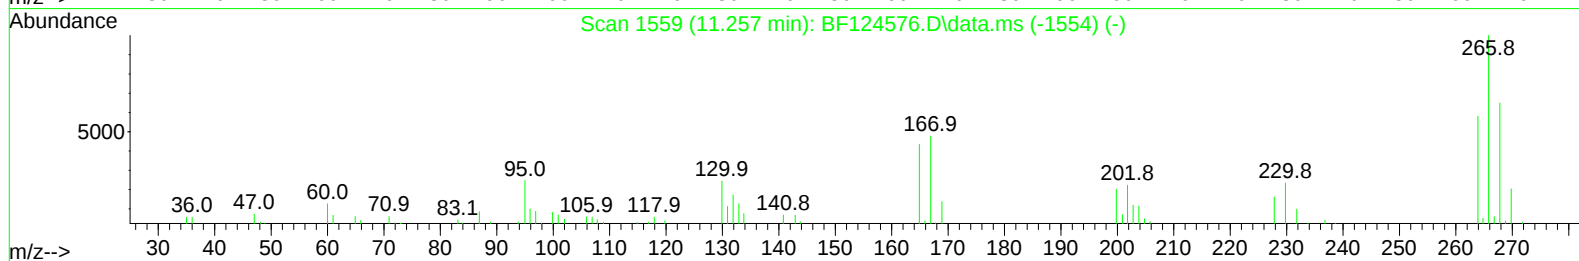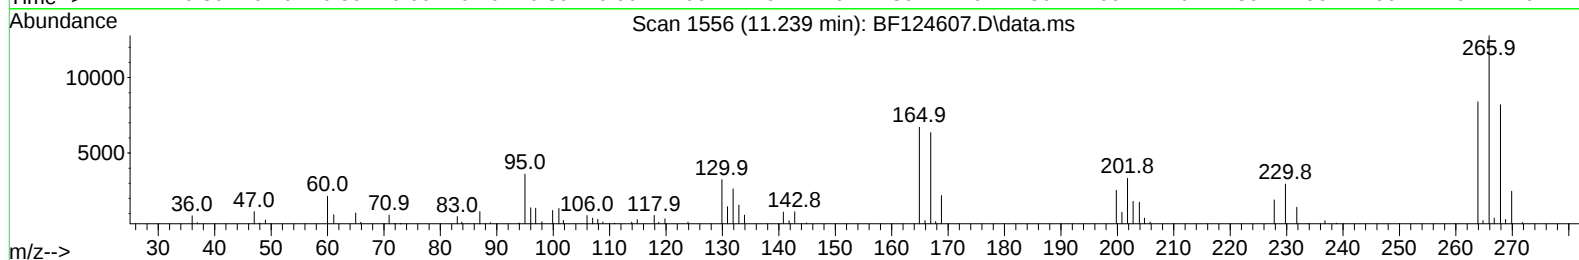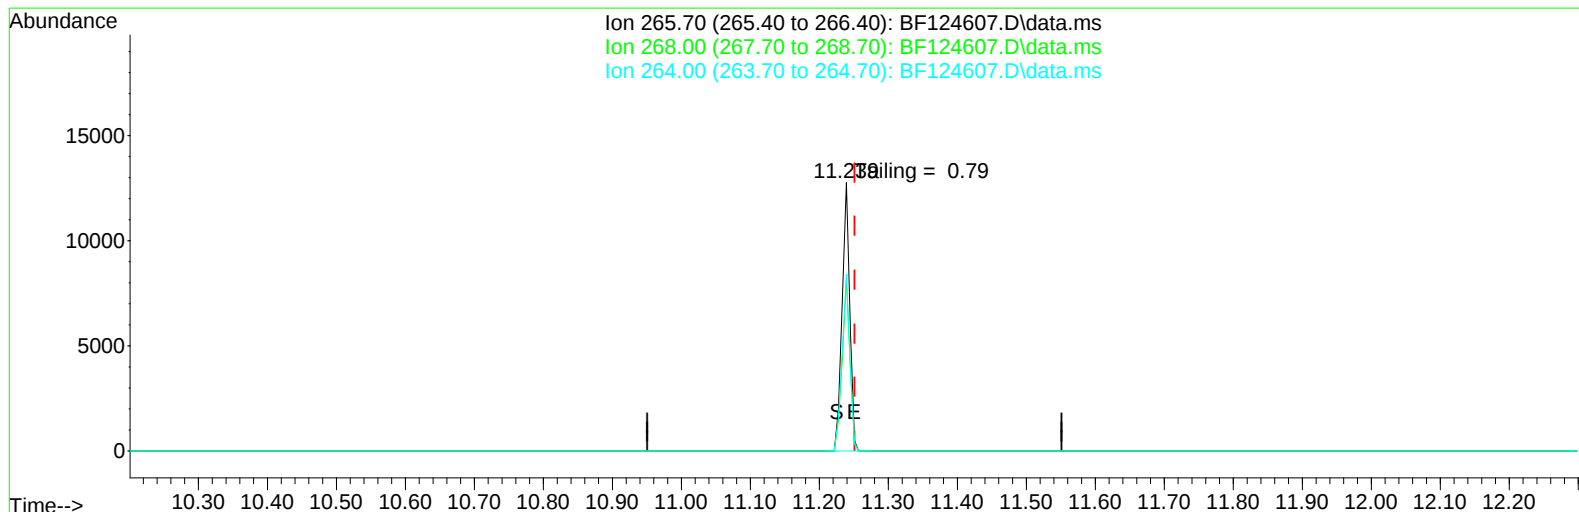

TIC: BF124607.D\data.ms

(70) Pentachlorophenol (C)

11.239min (-0.012) 0.00 ng

response	9879
----------	------

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.21
264.00	69.90	65.76
0.00	0.00	0.00