

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071921\
 Data File : BF124612.D
 Acq On : 19 Jul 2021 14:11
 Operator : JU/CG
 Sample : PB137725BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137725BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124612.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.204	527	530	534	rBB	3513	4283	1.19%	0.211%
2	5.557	584	590	592	rBB	231197	263992	73.46%	12.985%
3	6.539	750	757	759	rBB	219854	261585	72.79%	12.866%
4	6.910	817	820	823	rBB	63257	53490	14.88%	2.631%
5	7.475	910	916	919	rBB	137372	176046	48.98%	8.659%
6	8.198	1033	1039	1042	rBB	67066	73117	20.34%	3.596%
7	9.275	1215	1222	1225	rBB	332164	358547	99.77%	17.636%
8	9.951	1332	1337	1340	rBB	92908	85341	23.75%	4.198%
9	10.745	1466	1472	1475	rBB	227798	211301	58.79%	10.393%
10	11.439	1586	1590	1594	rBB	95969	85934	23.91%	4.227%
11	13.033	1856	1861	1864	rBV	322322	359391	100.00%	17.677%
12	14.080	2035	2039	2042	rBV	71931	58323	16.23%	2.869%
13	15.568	2288	2292	2297	rBB	35124	41726	11.61%	2.052%




Sum of corrected areas: 2033076

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071921\
Data File : BF124612.D
Acq On : 19 Jul 2021 14:11
Operator : JU/CG
Sample : PB137725BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137725BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

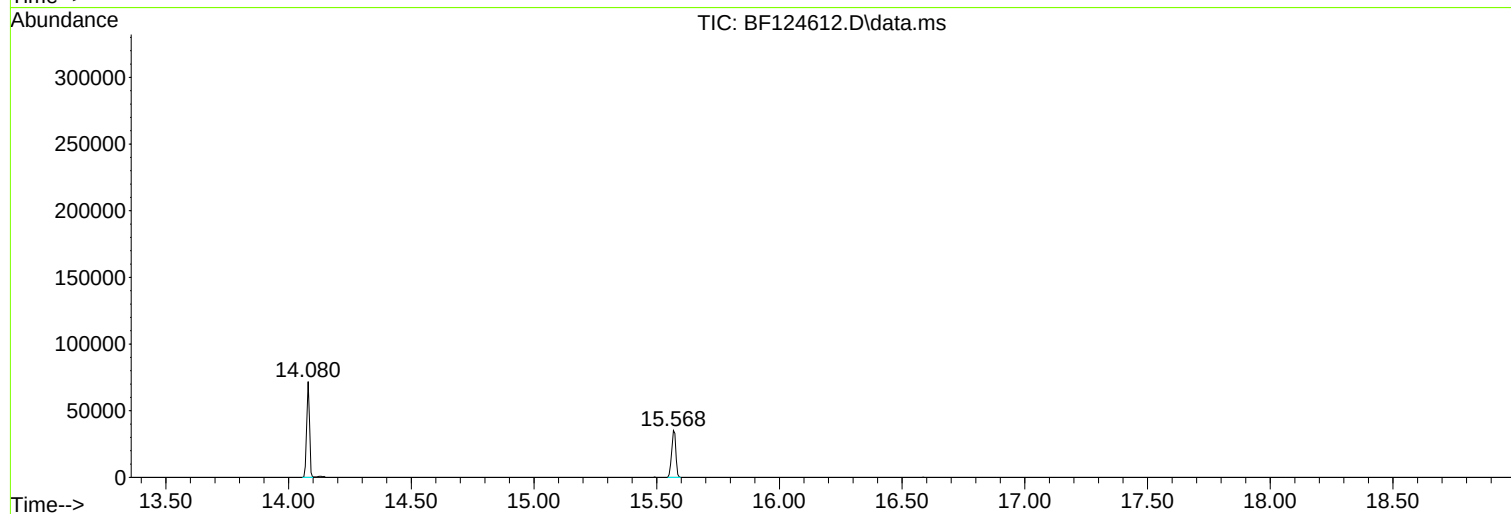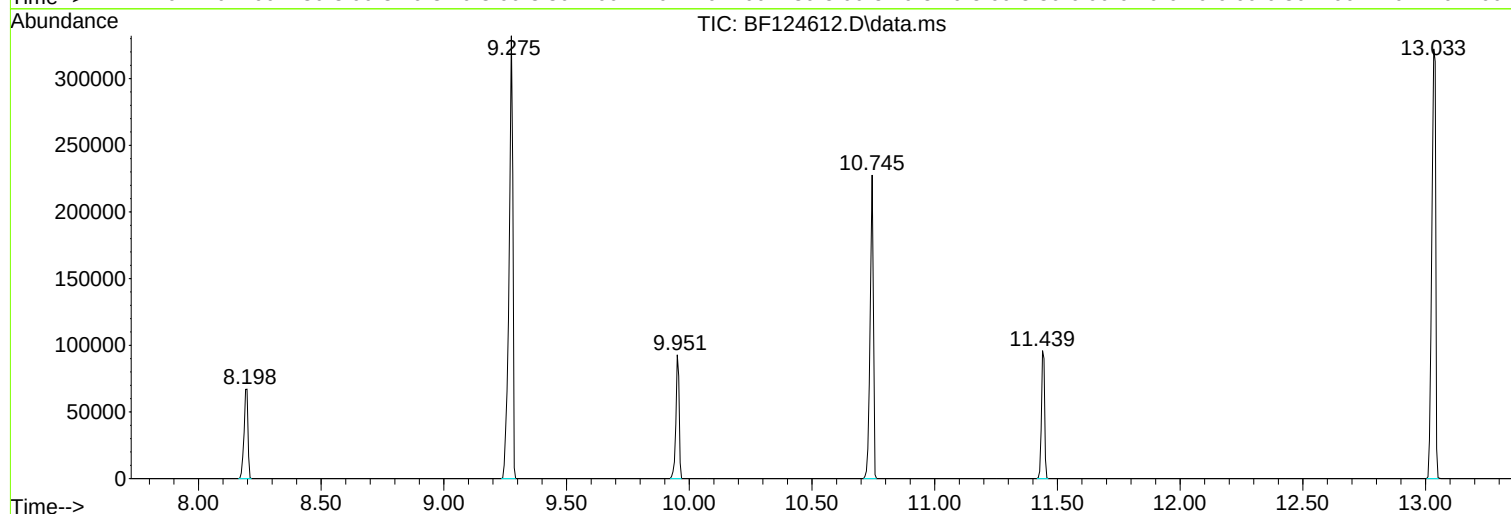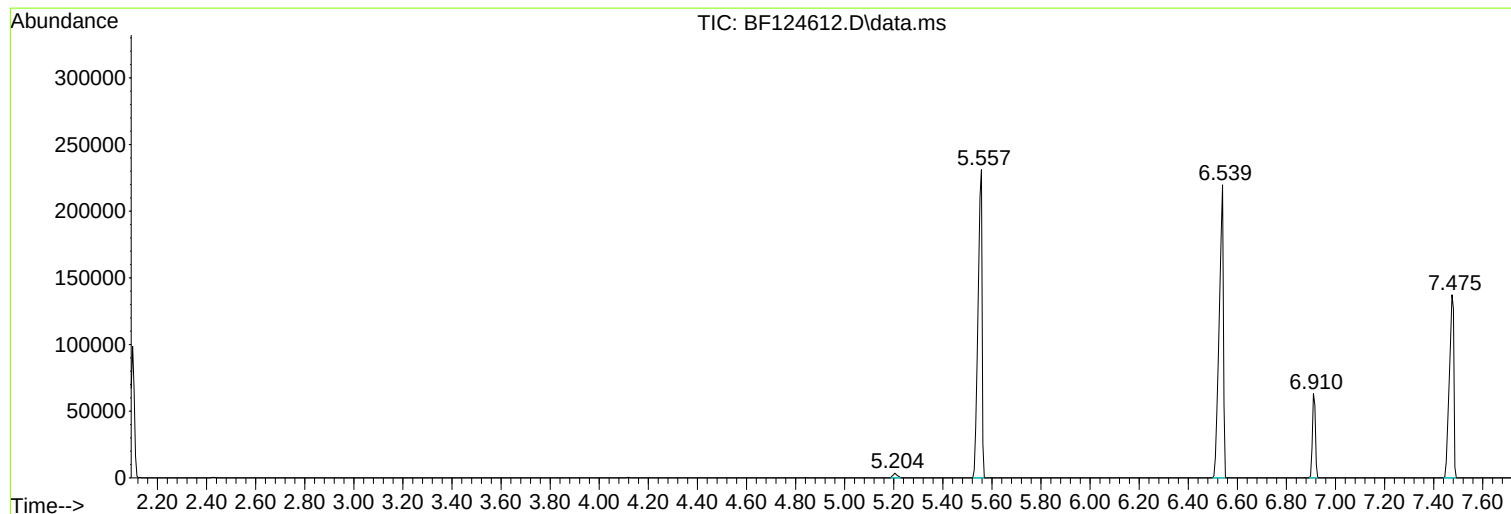

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071921\
Data File : BF124612.D
Acq On : 19 Jul 2021 14:11
Operator : JU/CG
Sample : PB137725BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137725BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071921\
Data File : BF124612.D
Acq On : 19 Jul 2021 14:11
Operator : JU/CG
Sample : PB137725BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137725BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------