

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071921\
 Data File : BF124615.D
 Acq On : 19 Jul 2021 15:51
 Operator : JU/CG
 Sample : PB137770BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137770BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.210	527	531	535	rBB2	3006	4286	1.16%	0.207%
2	5.557	584	590	592	rBB	240836	273921	74.14%	13.202%
3	6.540	750	757	760	rBB	227286	274864	74.40%	13.248%
4	6.910	817	820	823	rBB	60916	54291	14.70%	2.617%
5	7.475	910	916	919	rBB	144511	183249	49.60%	8.832%
6	8.192	1033	1038	1042	rBB	73489	75260	20.37%	3.627%
7	9.275	1215	1222	1225	rBB	352444	369451	100.00%	17.807%
8	9.951	1332	1337	1340	rBB	98147	88683	24.00%	4.274%
9	10.745	1466	1472	1475	rBB	222344	214441	58.04%	10.336%
10	11.439	1587	1590	1594	rVB	95782	84959	23.00%	4.095%
11	13.039	1856	1862	1865	rBV	357042	355295	96.17%	17.125%
12	14.080	2036	2039	2043	rBV	65065	55865	15.12%	2.693%
13	15.574	2288	2293	2297	rBV	34873	40206	10.88%	1.938%




Sum of corrected areas: 2074771

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071921\
Data File : BF124615.D
Acq On : 19 Jul 2021 15:51
Operator : JU/CG
Sample : PB137770BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137770BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

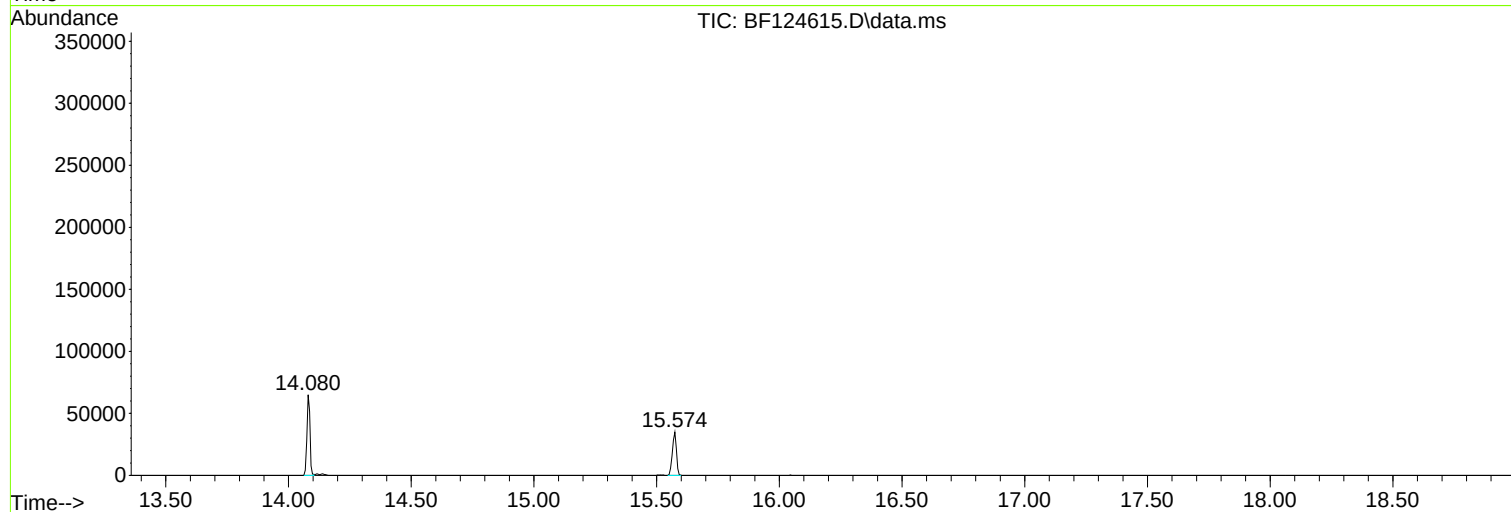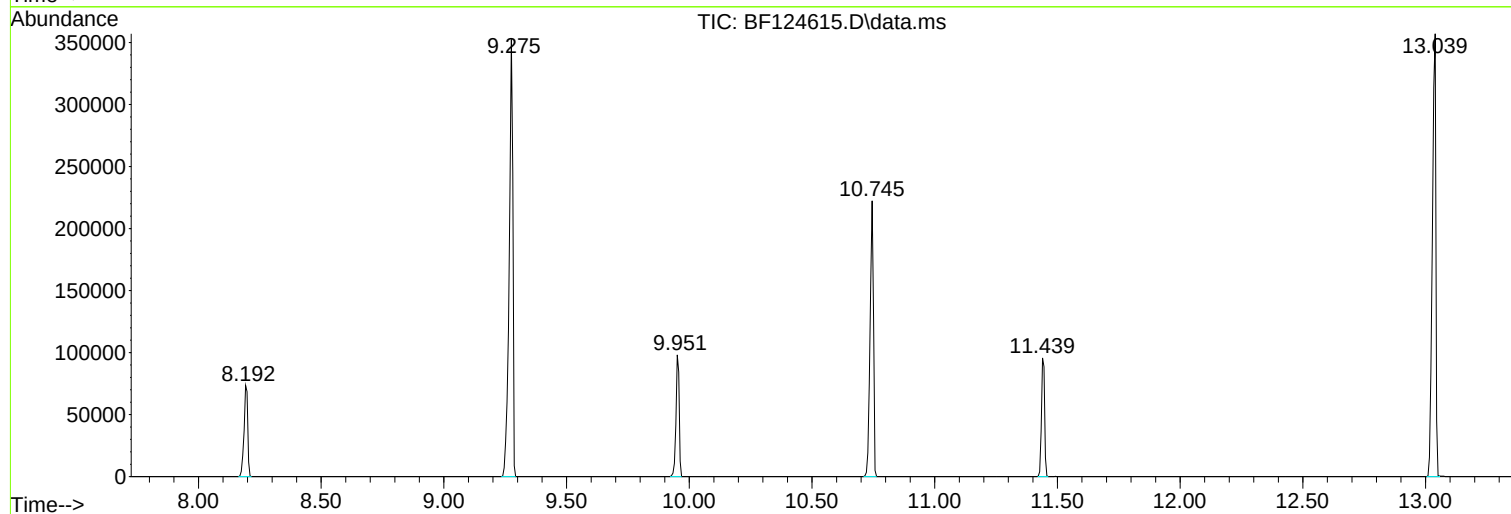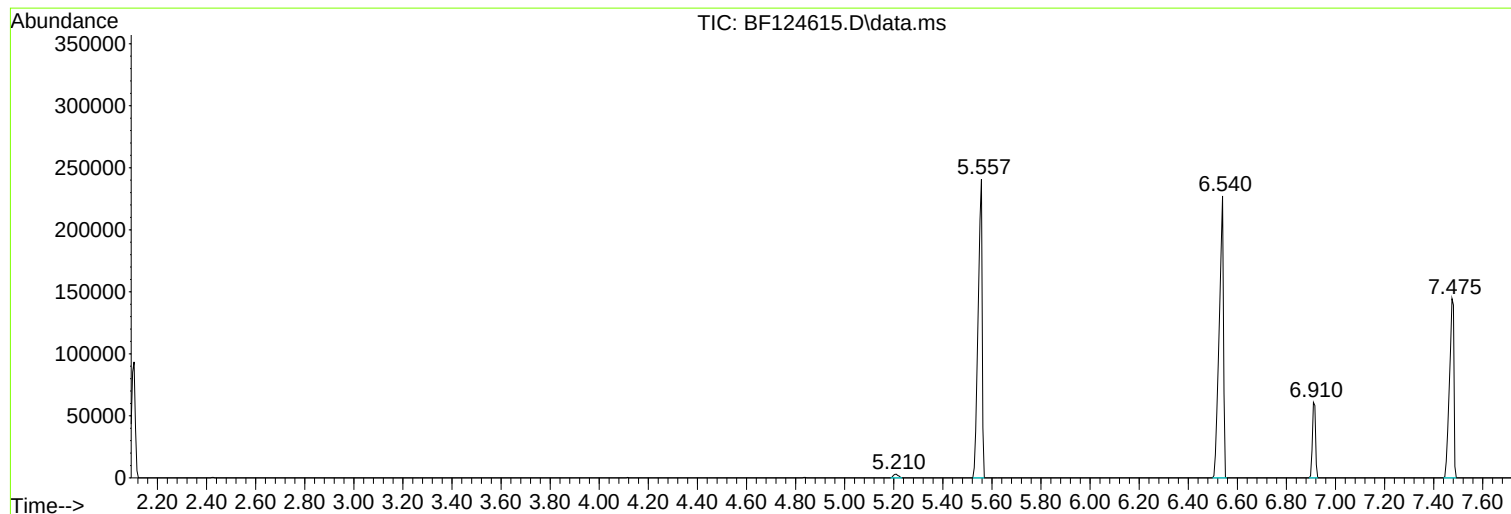

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071921\
Data File : BF124615.D
Acq On : 19 Jul 2021 15:51
Operator : JU/CG
Sample : PB137770BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137770BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071921\
Data File : BF124615.D
Acq On : 19 Jul 2021 15:51
Operator : JU/CG
Sample : PB137770BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137770BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------