
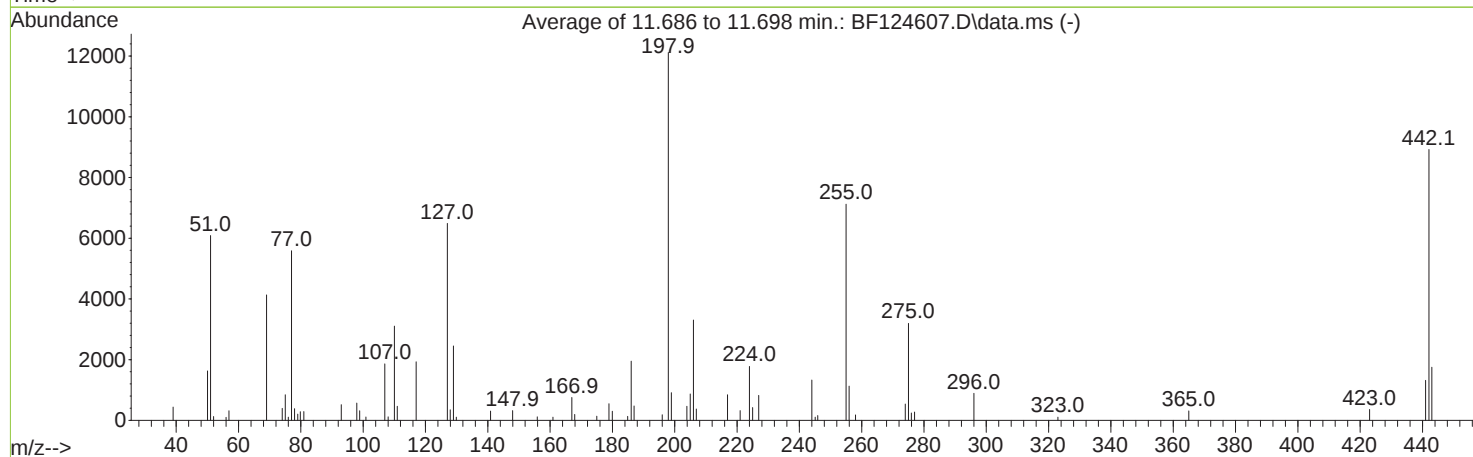


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071921\
 Data File : BF124607.D
 Acq On : 19 Jul 2021 10:24
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 19 11:33:09 2021

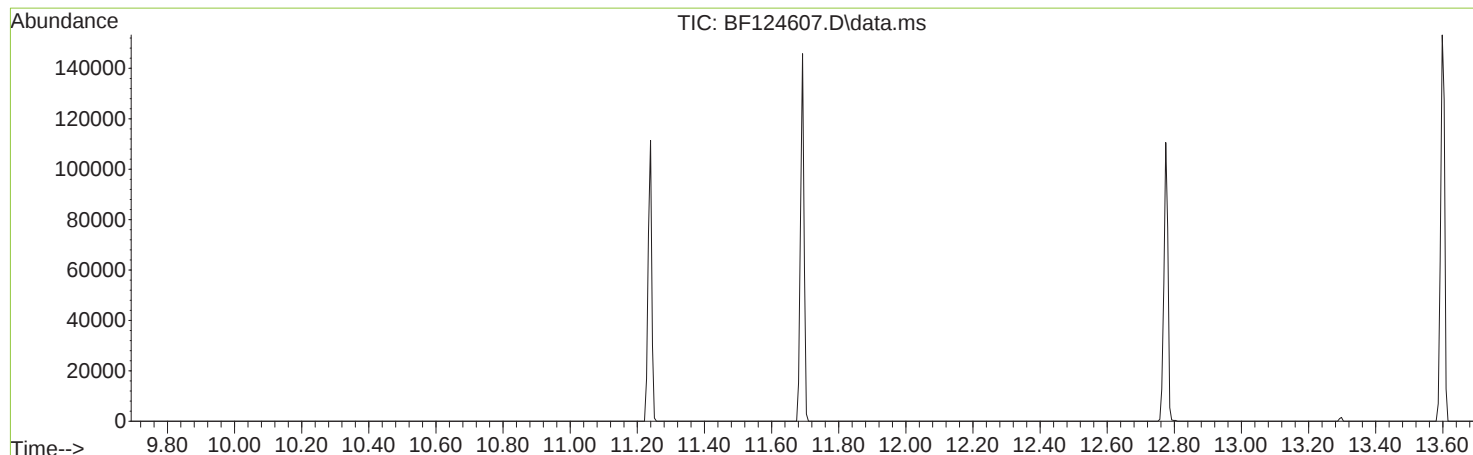




AutoFind: Scans 1632, 1633, 1634; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.2	6085	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.1	4133	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.5	6487	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12116	PASS
199	198	5	9	7.5	910	PASS
275	198	10	60	26.4	3195	PASS
365	198	1	100	2.6	309	PASS
441	198	0.01	100	10.9	1319	PASS
442	442	50	100	100.0	8920	PASS
443	442	15	24	19.6	1752	PASS


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071921\  
Data File : BF124607.D  
Acq On    : 19 Jul 2021  10:24  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 19 11:14:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 08 07:53:19 2021
Response via : Initial Calibration

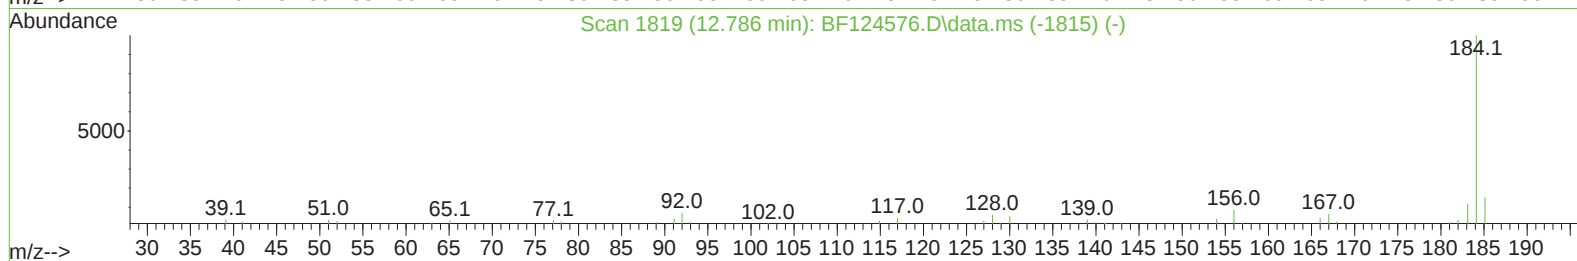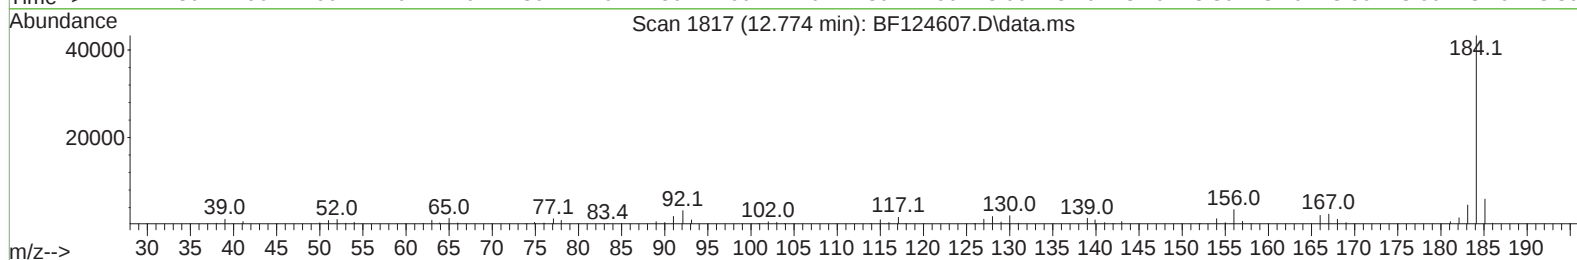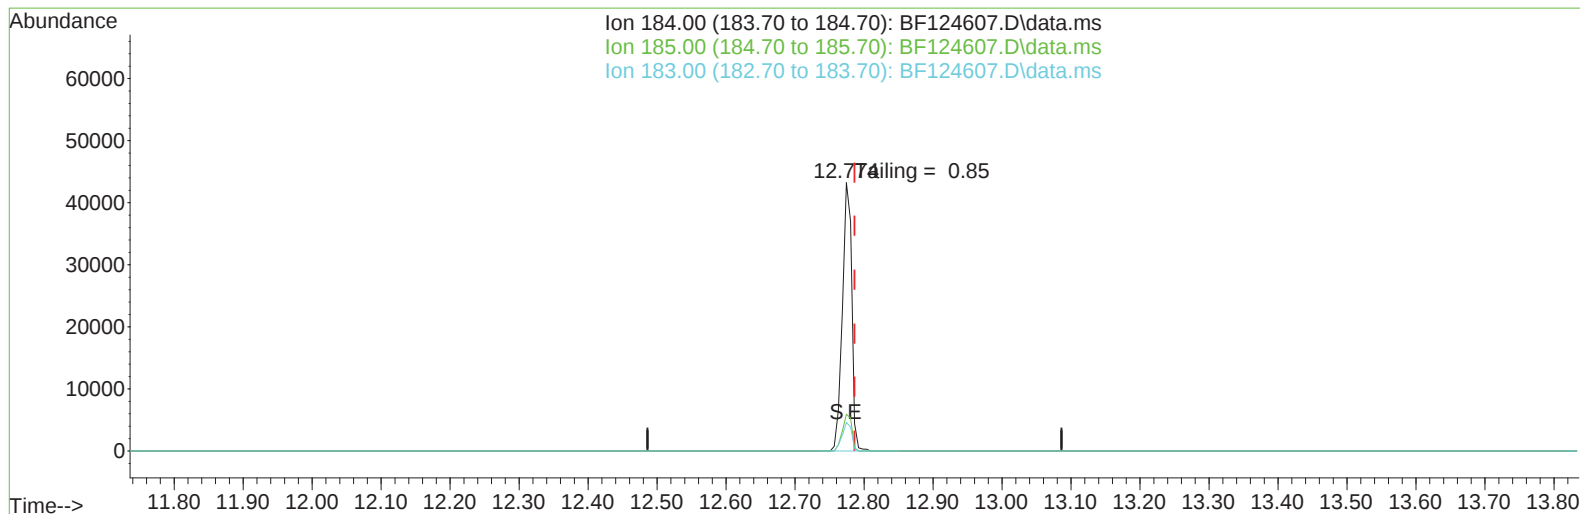

TIC: BF124607.D\data.ms

(77) Benzidine

12.774min (-0.012) 0.00 ng

response 40876

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.73
183.00	10.10	10.60
0.00	0.00	0.00

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/19/2021	BNA_F	<u>BF124607.D</u>
Compound Name	Response	Retention Time
DDT	25460	13.6
DDD	448	13.29
DDE	0	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
448	25908	1.73