
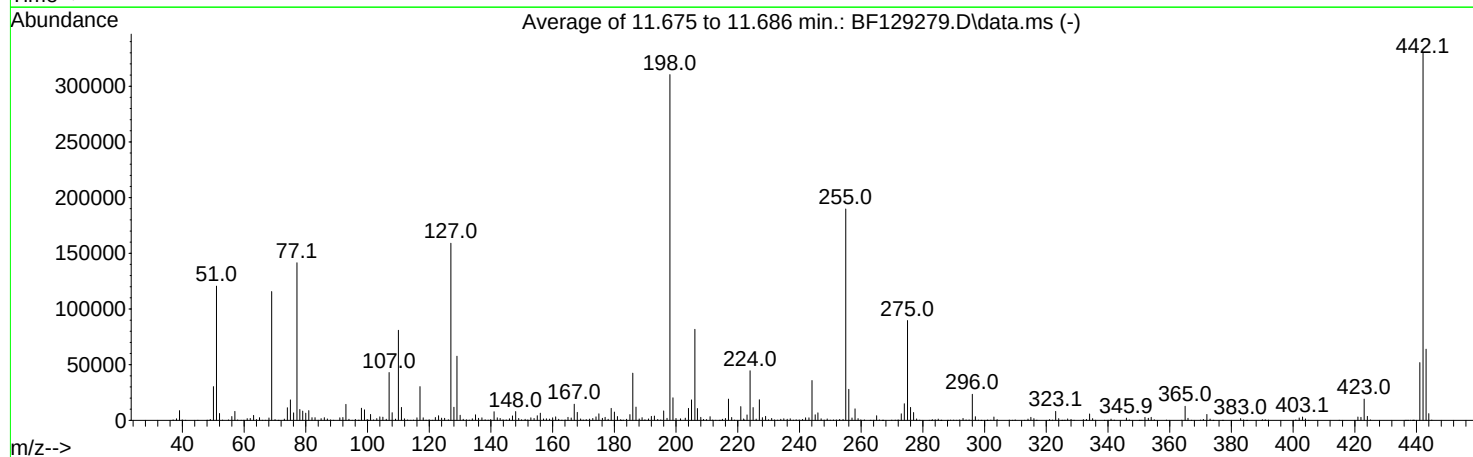


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071922\
 Data File : BF129279.D
 Acq On : 19 Jul 2022 08:56
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 15 12:55:49 2022

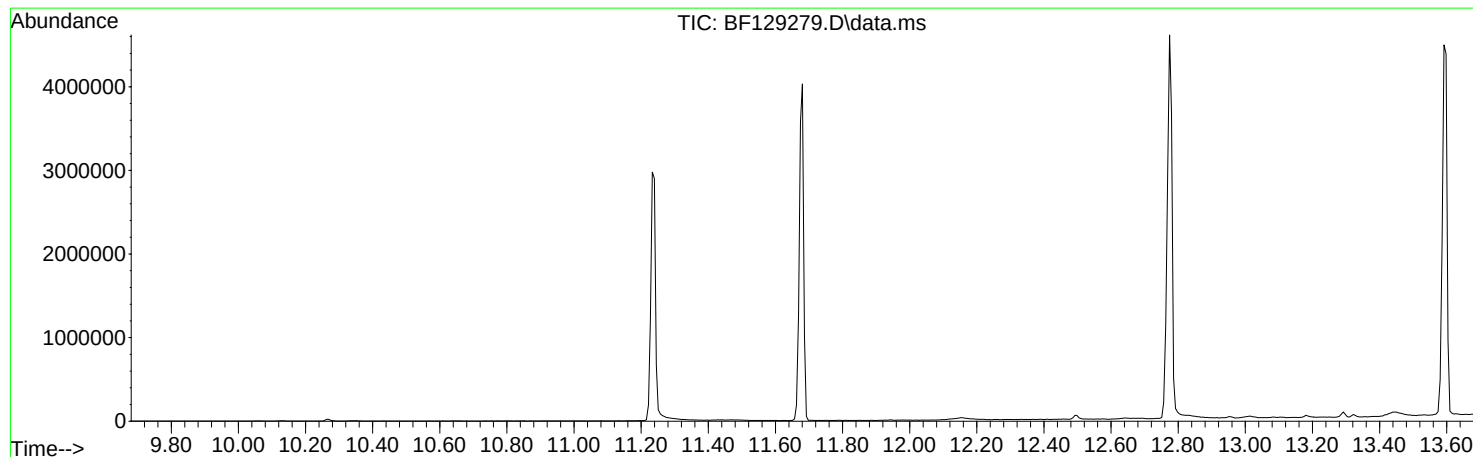

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	120605	PASS
68	69	0.00	2	1.8	2131	PASS
69	198	0.00	100	37.3	115658	PASS
70	69	0.00	2	0.6	663	PASS
127	198	10	80	51.2	159072	PASS
197	198	0.00	2	0.6	1871	PASS
198	198	100	100	100.0	310485	PASS
199	198	5	9	6.5	20325	PASS
275	198	10	60	28.9	89597	PASS
365	198	1	100	4.1	12598	PASS
441	198	0.01	100	16.7	51813	PASS
442	442	50	100	100.0	330283	PASS
443	442	15	24	19.4	63963	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/19/2022	BNA_F	<u>BF129279.D</u>
Compound Name	Response	Retention Time
DDT	808033	13.598
DDD	14916	13.292
DDE	2020	12.957
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16936	824969	2.05

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071922\
Data File : BF129279.D
Acq On : 19 Jul 2022 08:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 20 03:31:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 12:55:49 2022
Response via : Initial Calibration

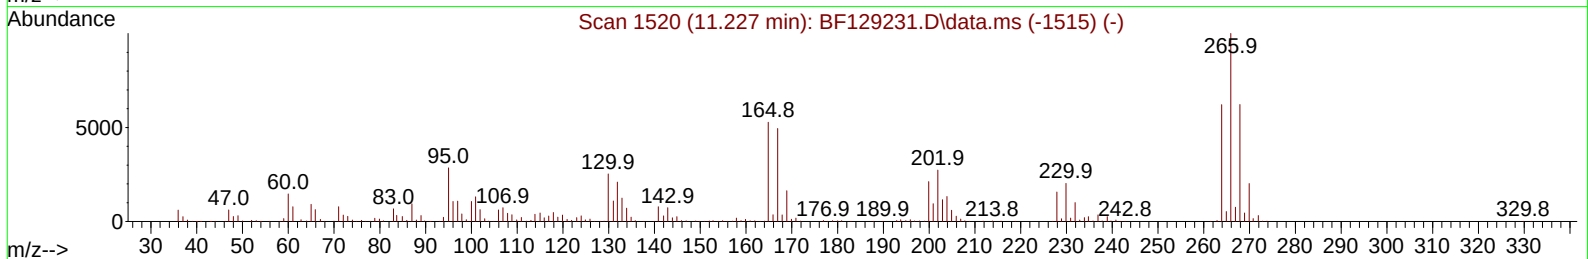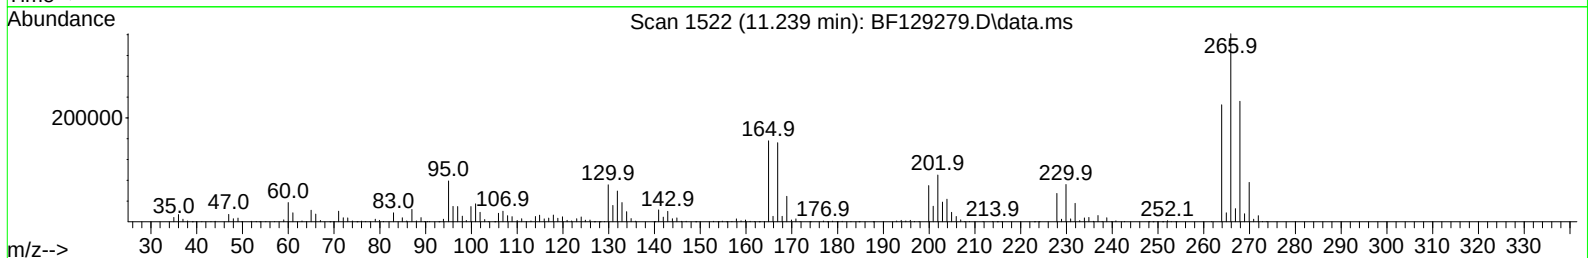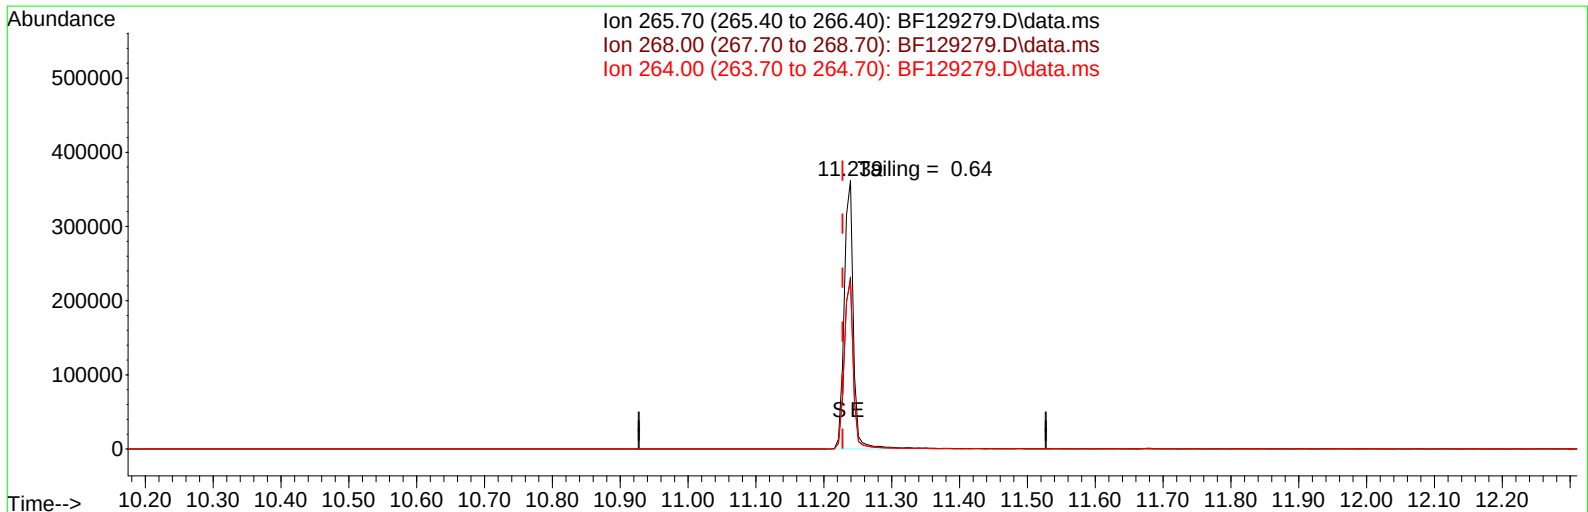

TIC: BF129279.D\data.ms

(70) Pentachlorophenol (C)

11.239min (+ 0.012) 361448.41 ng




response 337243

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.11
264.00	61.80	62.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071922\
 Data File : BF129279.D
 Acq On : 19 Jul 2022 08:56
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 20 03:31:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 15 12:55:49 2022
 Response via : Initial Calibration

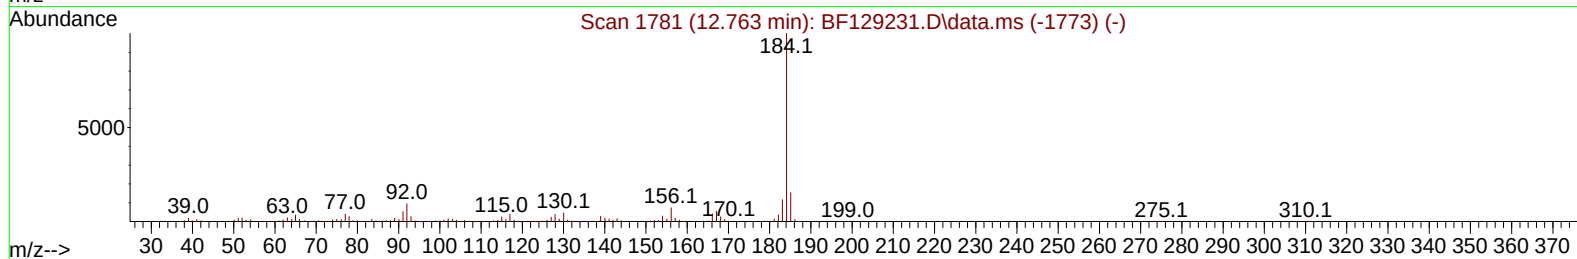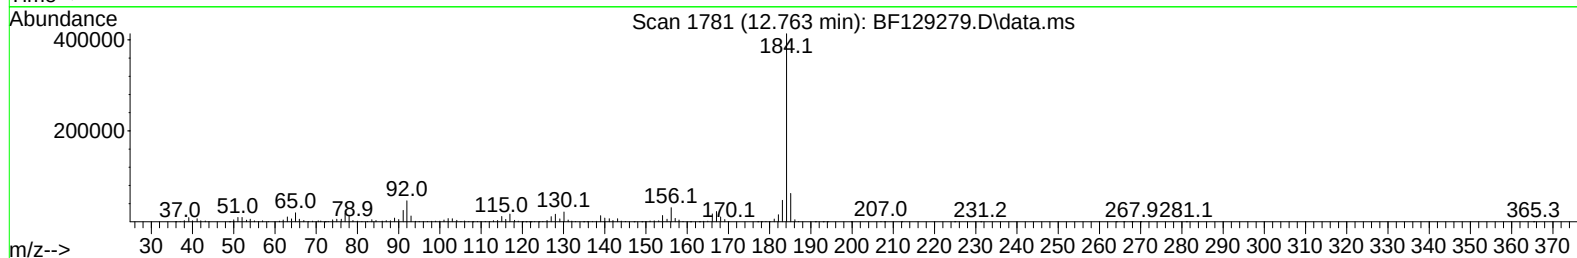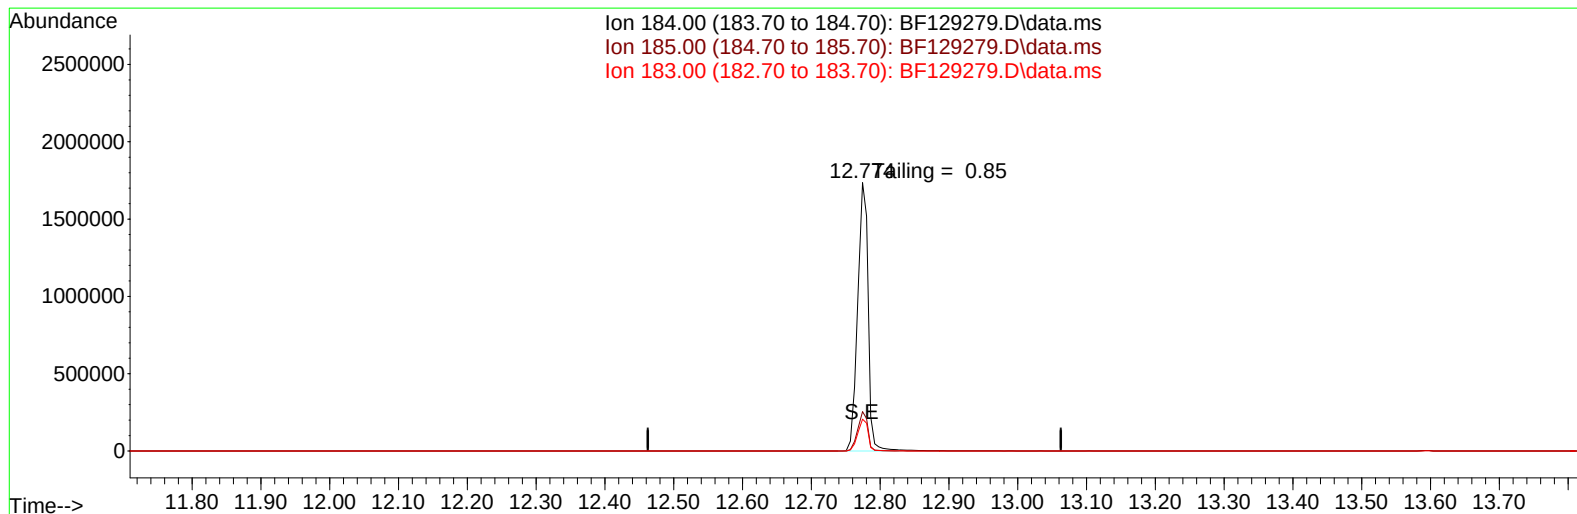

TIC: BF129279.D\data.ms

(77) Benzidine

12.763min (-12.763) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.90	0.00#
183.00	11.60	0.00#
0.00	0.00	0.00