


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071924\
Data File : BF138577.D
Acq On : 19 Jul 2024 08:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 09 16:58:40 2024

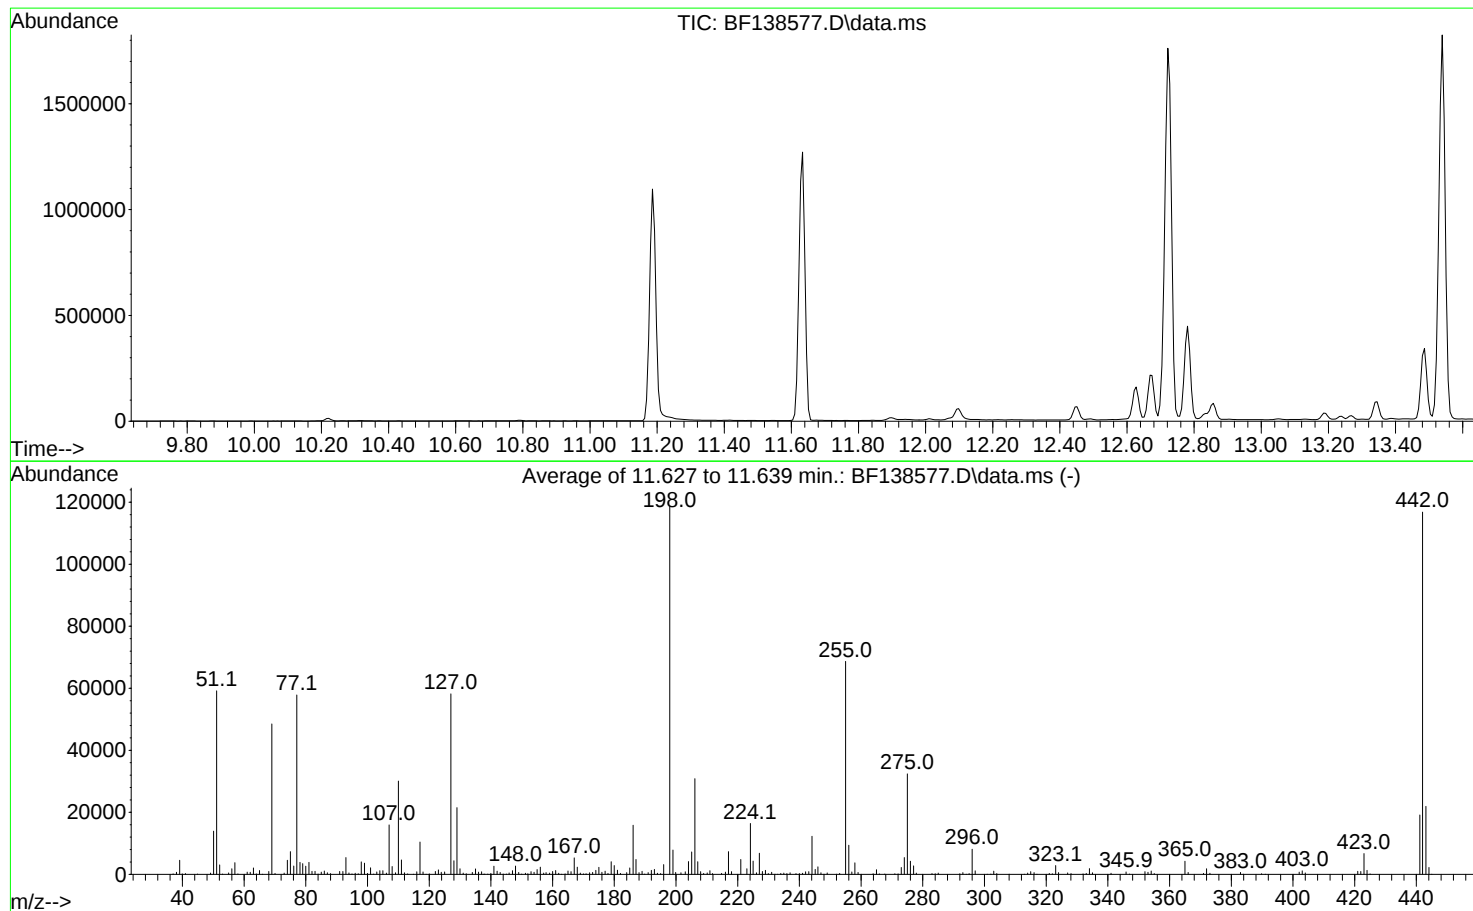

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.9	59165	PASS
68	69	0.00	2	1.9	939	PASS
69	198	0.00	100	40.9	48504	PASS
70	69	0.00	2	0.6	303	PASS
127	198	10	80	49.1	58195	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	118619	PASS
199	198	5	9	6.6	7822	PASS
275	198	10	60	27.3	32395	PASS
365	198	1	100	3.6	4219	PASS
441	198	0.01	100	16.1	19128	PASS
442	442	50	100	100.0	116821	PASS
443	442	15	24	18.8	21923	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/19/2024	BNA_F	<u>BF138577.D</u>
Compound Name	Response	Retention Time
DDT	430145	13.539
DDD	9049	13.269
DDE	949	12.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9998	440143	2.27

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071924\
Data File : BF138577.D
Acq On : 19 Jul 2024 08:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 19 11:56:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

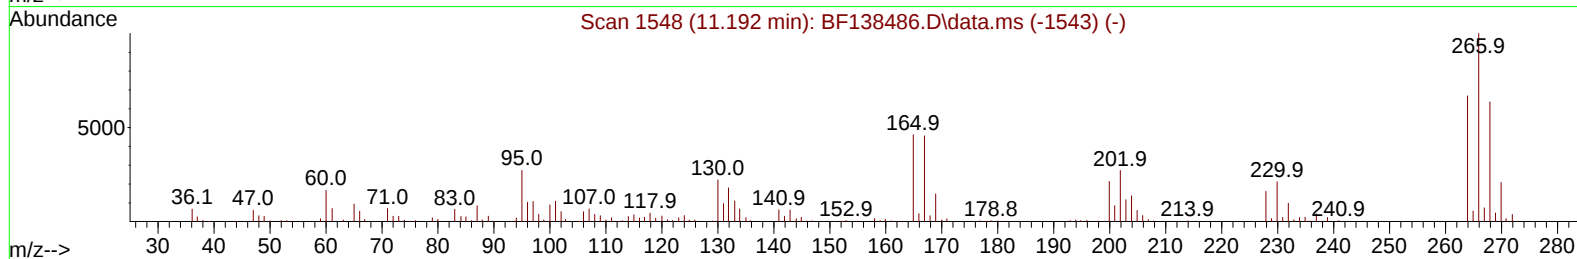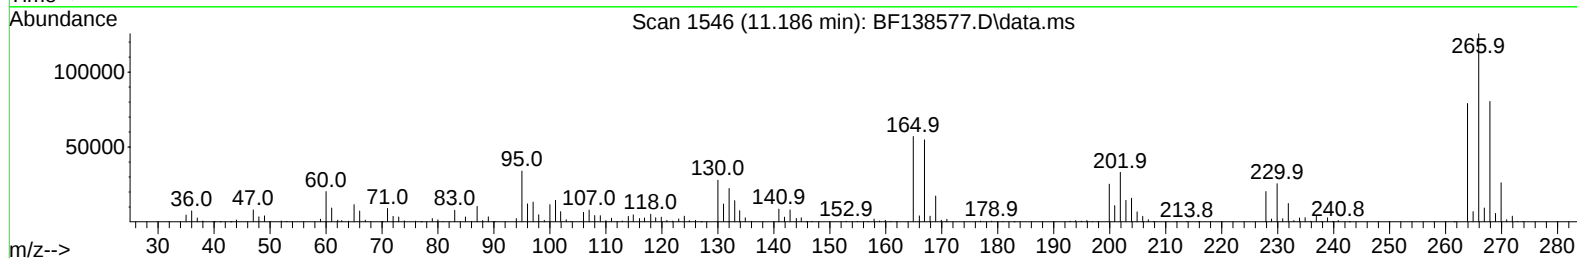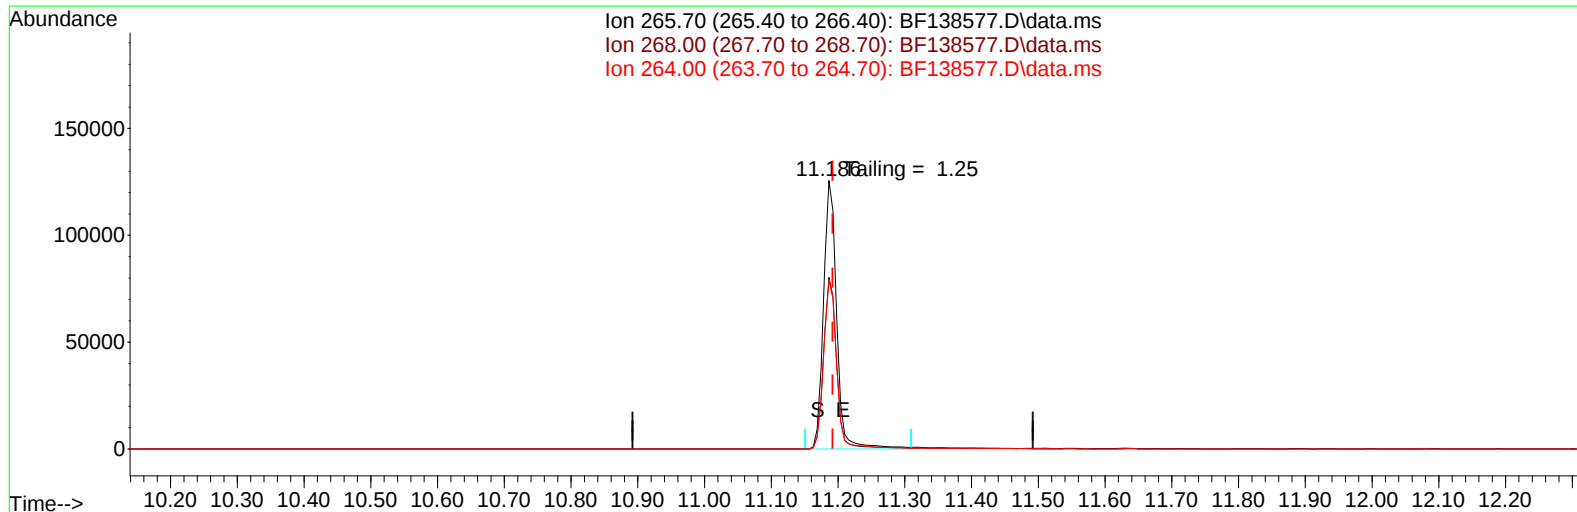

TIC: BF138577.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.006) 33825.46 ng




response 172777

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.01
264.00	66.90	62.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071924\
Data File : BF138577.D
Acq On : 19 Jul 2024 08:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 19 11:56:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

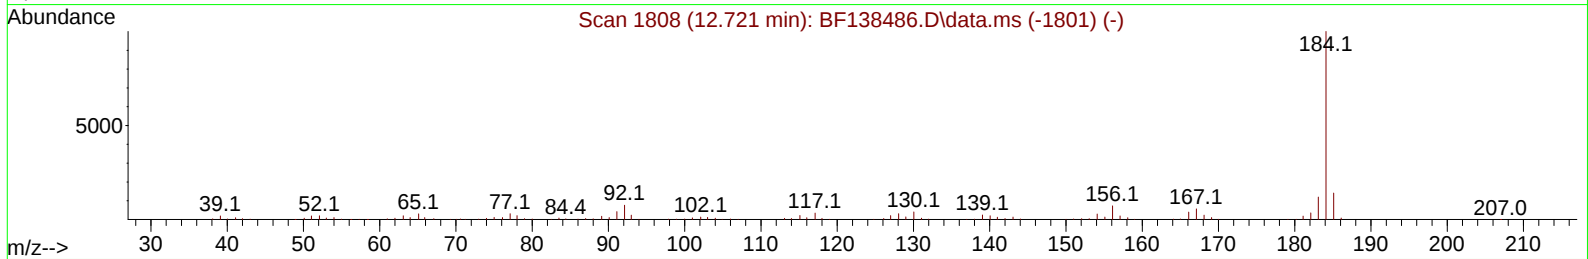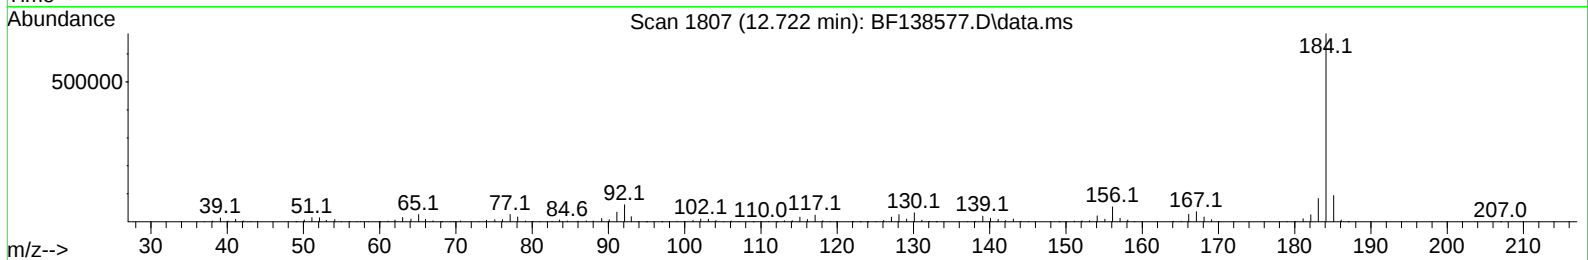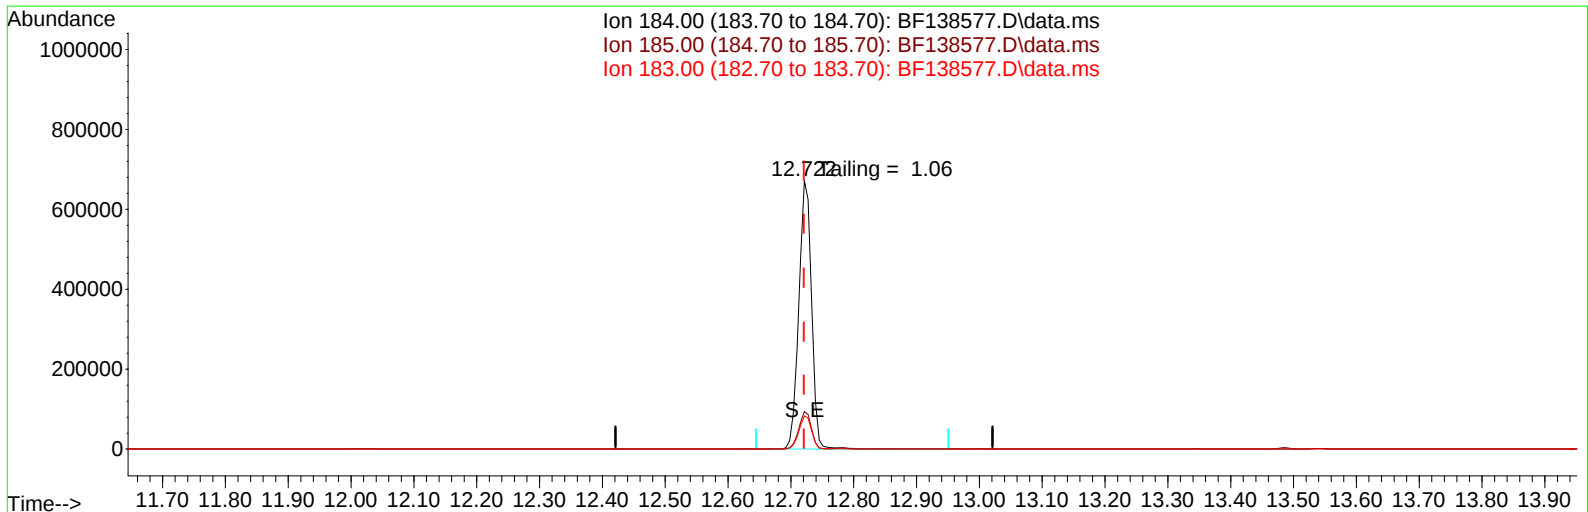

TIC: BF138577.D\data.ms

(77) Benzidine

12.722min (+ 0.001) 0.00 ng

response 952272

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.99
183.00	11.90	12.35
0.00	0.00	0.00