


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072016\
 Data File : BF089128.D
 Acq On : 20 Jul 2016 11:36
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 20 19:03:15 2016

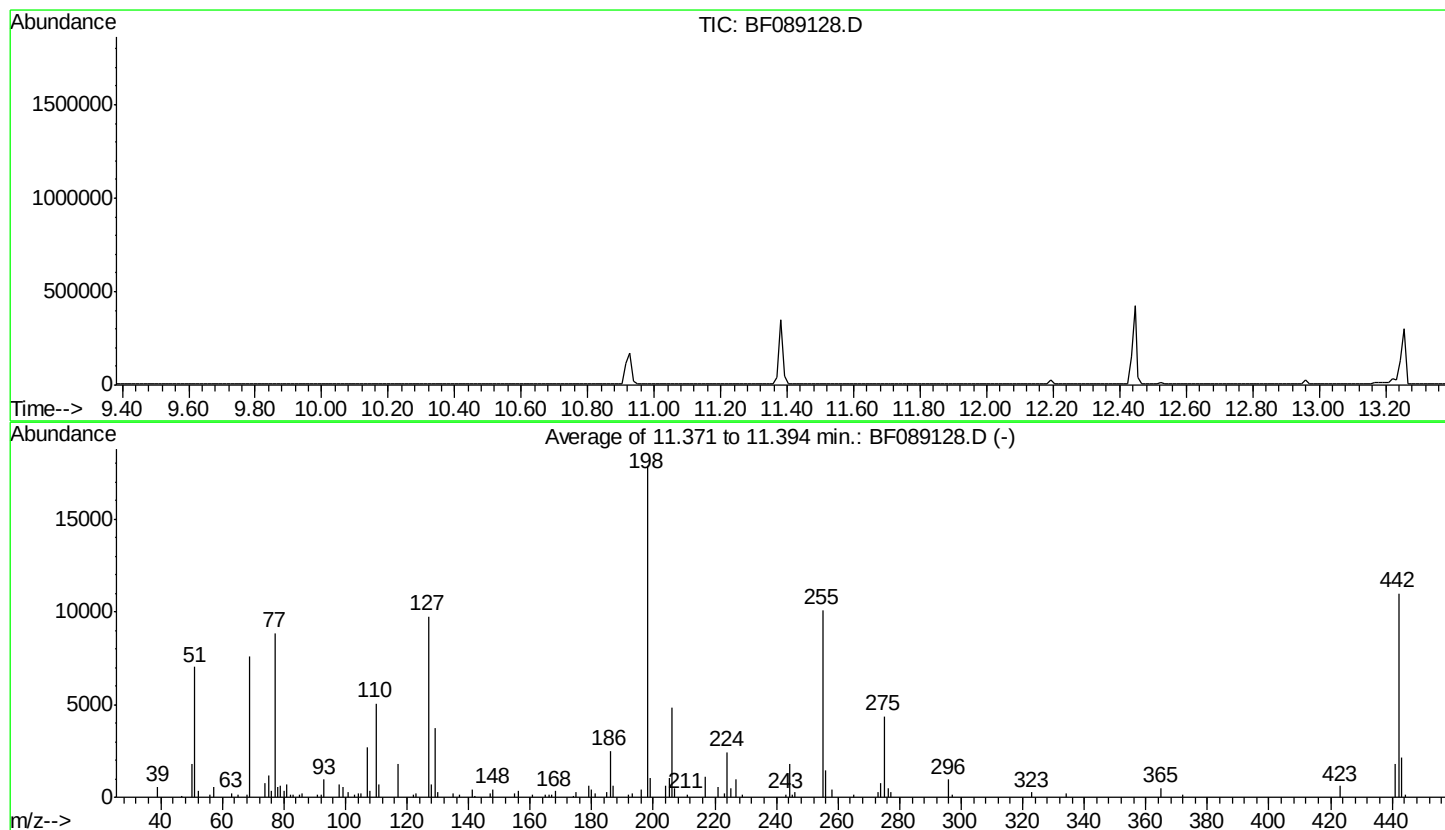

AutoFind: Scans 856, 857, 858; Background Corrected with Scan 853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	7015	PASS
68	69	0.00	2	1.9	144	PASS
69	198	0.00	100	42.6	7616	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.5	9751	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17887	PASS
199	198	5	9	5.7	1028	PASS
275	198	10	60	24.4	4361	PASS
365	198	1	100	2.8	499	PASS
441	442	0.01	24	16.4	1800	PASS
442	198	50	100	61.5	11008	PASS
443	442	15	24	19.6	2155	PASS