


Data Path : Z:\HPCHEM1\BNA F\Data\BF072017\  
 Data File : BF096902.D  
 Acq On : 20 Jul 2017 13:01  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF071317.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Jul 18 13:33:22 2017

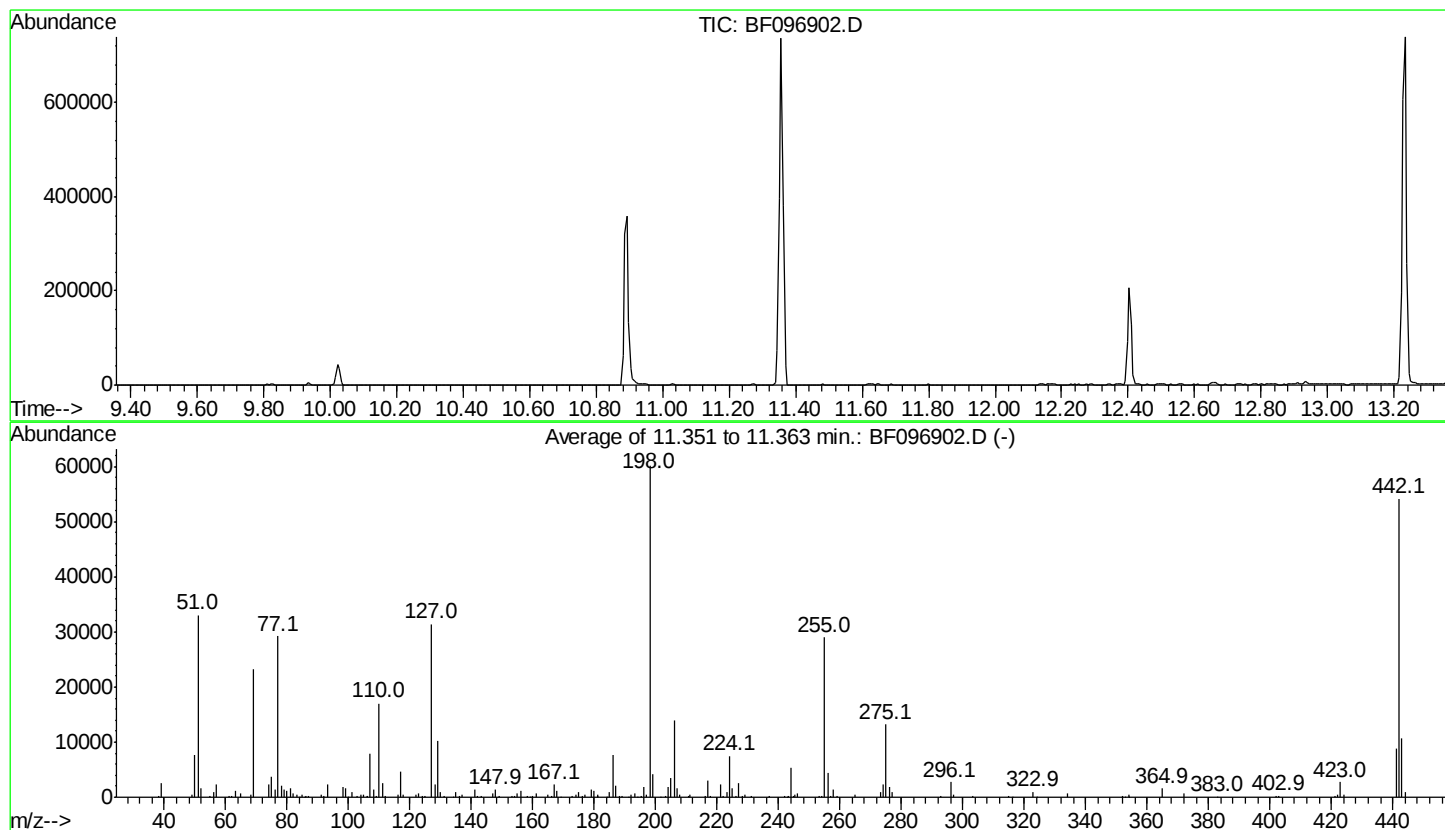

AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1587

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 54.9         | 33024      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 386        | PASS                |
| 69             | 198             | 0.00            | 100             | 38.6         | 23267      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 52.2         | 31437      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.6          | 366        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 60200      | PASS                |
| 199            | 198             | 5               | 9               | 7.0          | 4206       | PASS                |
| 275            | 198             | 10              | 60              | 21.9         | 13213      | PASS                |
| 365            | 198             | 1               | 100             | 2.6          | 1572       | PASS                |
| 441            | 442             | 0.01            | 24              | 16.4         | 8884       | PASS                |
| 442            | 198             | 50              | 100             | 90.0         | 54176      | PASS                |
| 443            | 442             | 15              | 24              | 19.7         | 10669      | PASS                |