


Data Path : Z:\HPCHEM1\BNA F\Data\BF072017\
 Data File : BF096927.D
 Acq On : 21 Jul 2017 2:13
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 18 13:33:22 2017

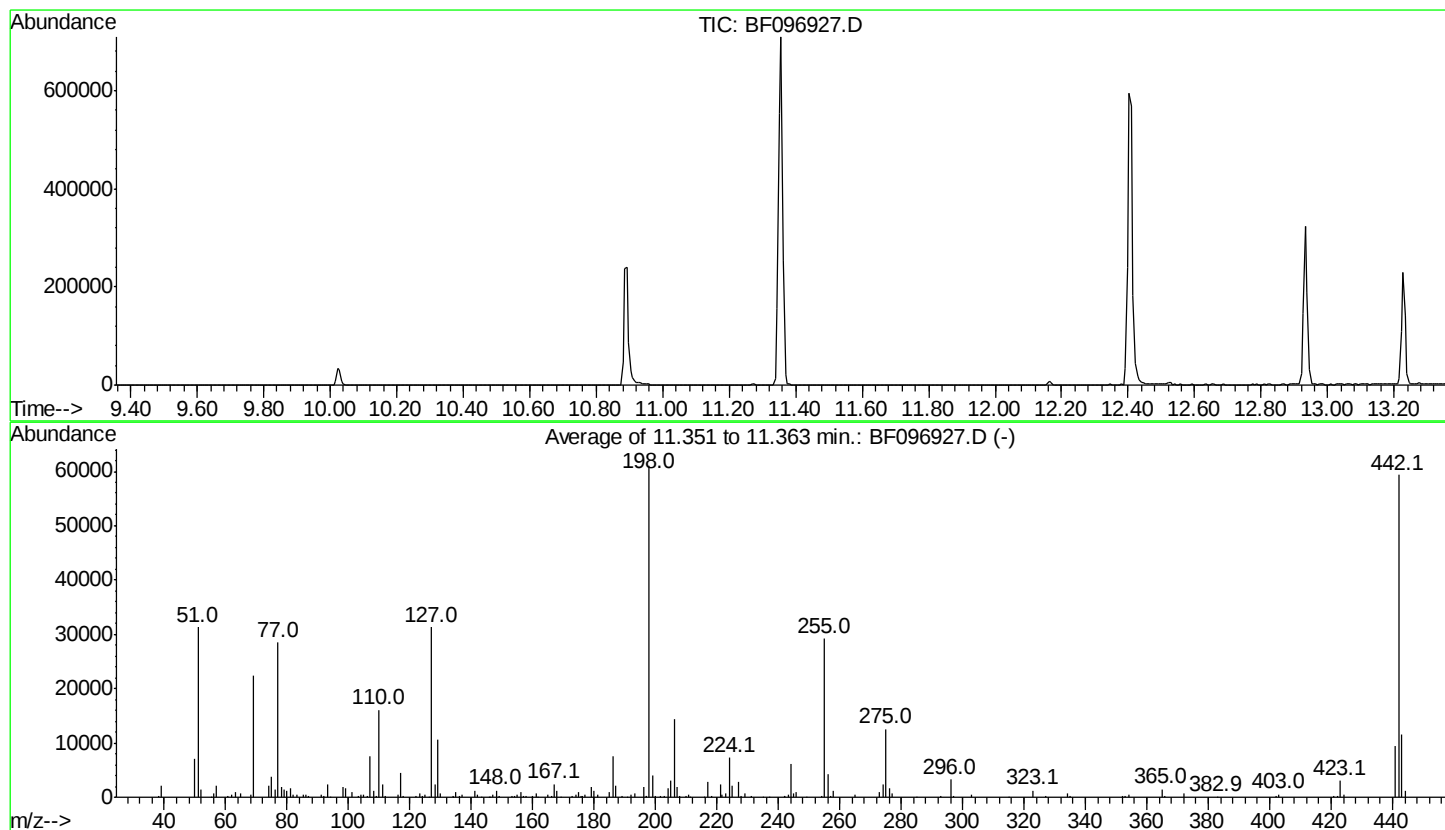

AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.3	31303	PASS
68	69	0.00	2	1.8	408	PASS
69	198	0.00	100	36.7	22406	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.2	31268	PASS
197	198	0.00	2	0.5	310	PASS
198	198	100	100	100.0	61072	PASS
199	198	5	9	6.7	4081	PASS
275	198	10	60	20.6	12604	PASS
365	198	1	100	2.3	1417	PASS
441	442	0.01	24	16.0	9504	PASS
442	198	50	100	97.2	59392	PASS
443	442	15	24	19.6	11634	PASS