

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072020\
 Data File : BF120927.D
 Acq On : 20 Jul 2020 9:57
 Operator : JU/CG
 Sample : PB130275BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB130275BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.157	8	12	26	rVB	153878	253404	4.38%	0.652%
2	5.440	565	570	573	rBV	3943721	4628917	79.92%	11.917%
3	6.445	735	741	744	rBV	3583179	4603390	79.48%	11.851%
4	6.816	800	804	807	rBV	1523486	1276212	22.04%	3.286%
5	7.381	894	900	903	rBV	2615954	3191154	55.10%	8.215%
6	8.098	1017	1022	1025	rBV	1750561	1688626	29.16%	4.347%
7	9.175	1199	1205	1208	rBV	4759948	5507300	95.09%	14.178%
8	9.851	1314	1320	1337	rVB	2020059	1966593	33.96%	5.063%
9	10.639	1448	1454	1475	rBV	3032503	3639261	62.84%	9.369%
10	11.333	1567	1572	1576	rBV	2123277	2078055	35.88%	5.350%
11	12.927	1836	1843	1846	rBV2	4685534	5791696	100.00%	14.910%
12	13.974	2016	2021	2024	rBV	2057587	2058352	35.54%	5.299%
13	15.421	2261	2267	2272	rBV	1571449	2095373	36.18%	5.394%
14	16.386	2425	2431	2440	rVB	32432	65009	1.12%	0.167%


Sum of corrected areas: 38843342

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072020\
Data File : BF120927.D
Acq On : 20 Jul 2020 9:57
Operator : JU/CG
Sample : PB130275BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130275BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

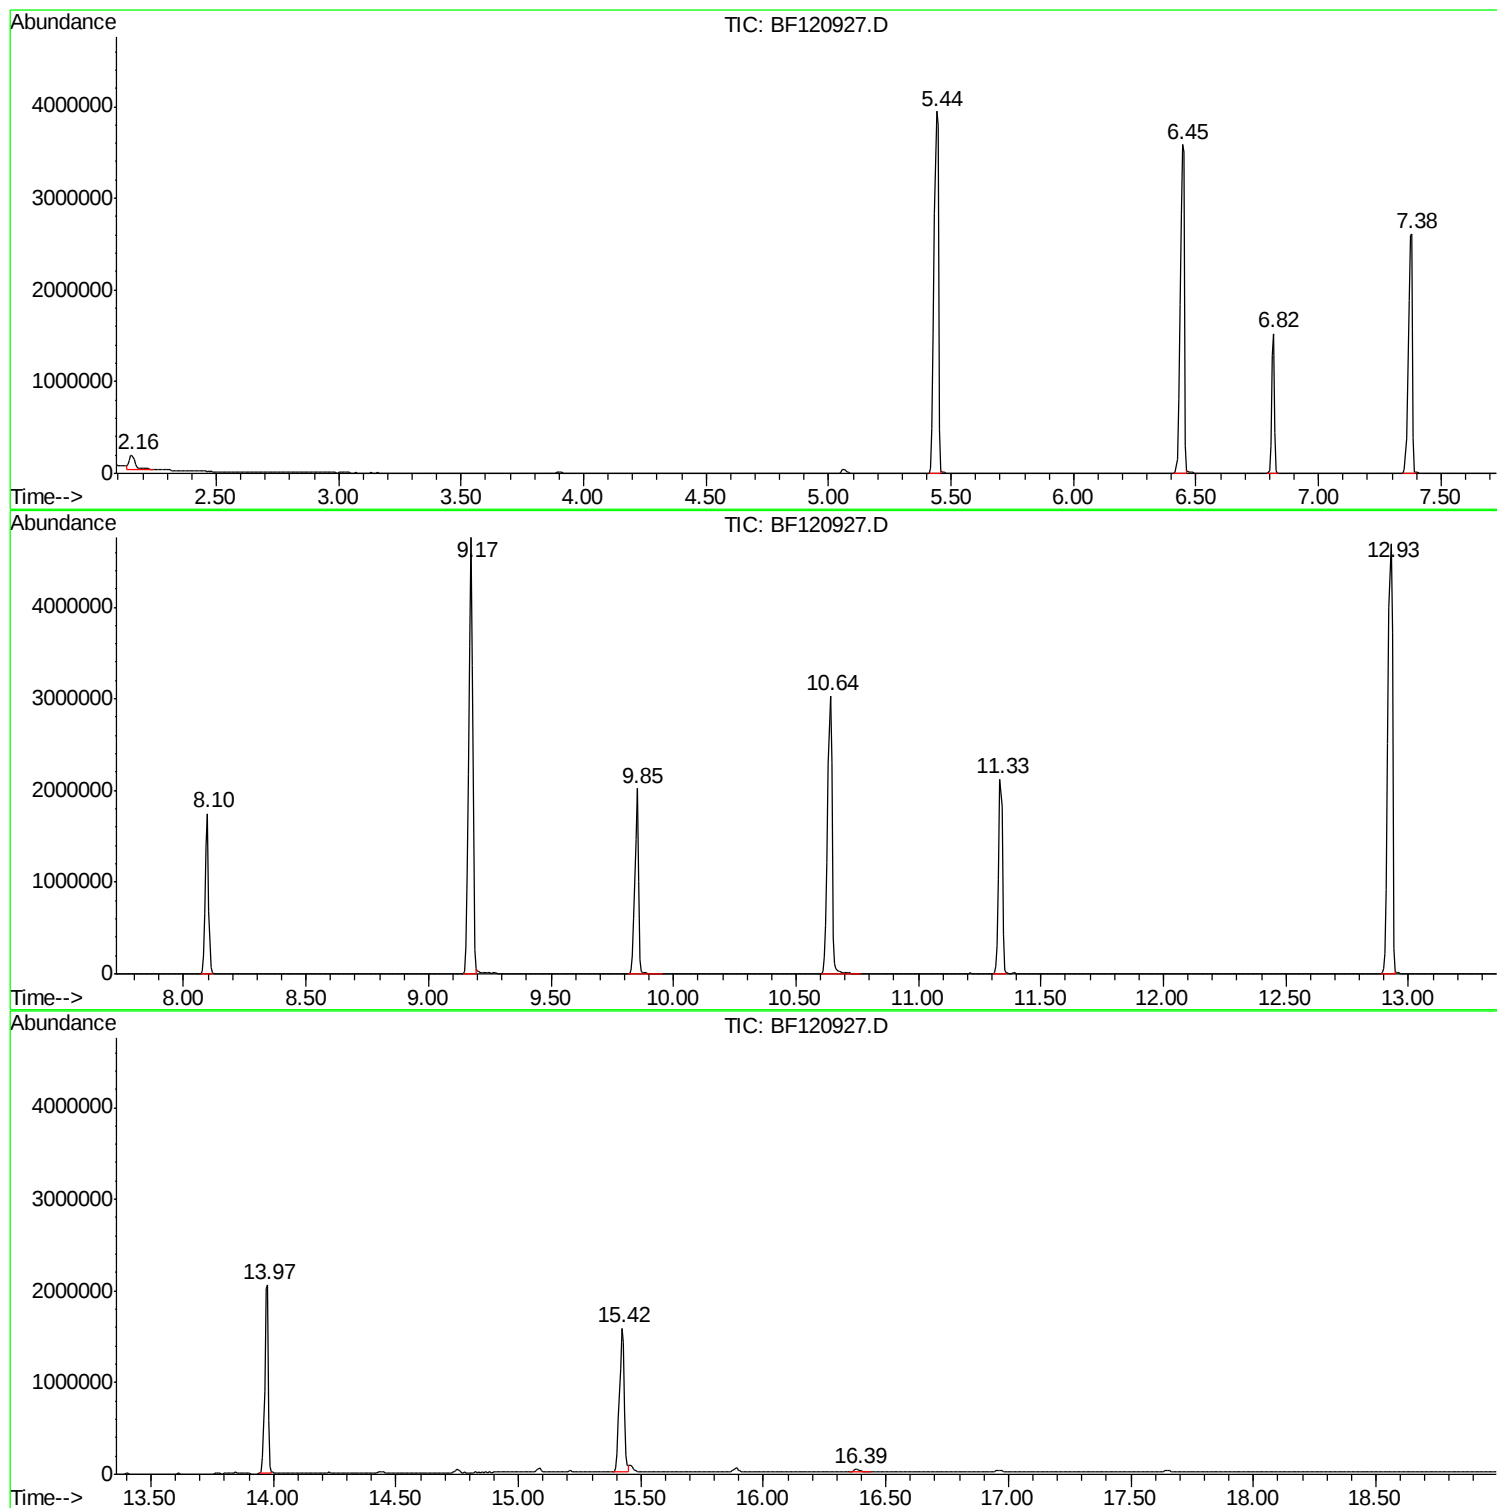

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072020\
Data File : BF120927.D
Acq On : 20 Jul 2020 9:57
Operator : JU/CG
Sample : PB130275BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130275BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.16	3.97 ng	253404	1,4-Dichlorobenzene-d4	6.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
3		3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	17
4		N-Ethylformamide	73	C3H7NO	000627-45-2	9
5		Borane, dimethoxy-	74	C2H7BO2	004542-61-4	9

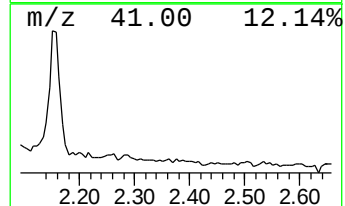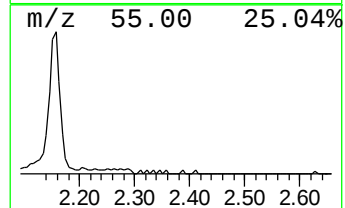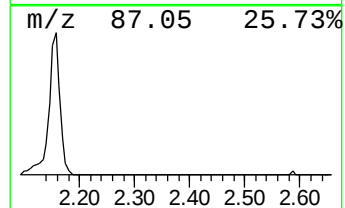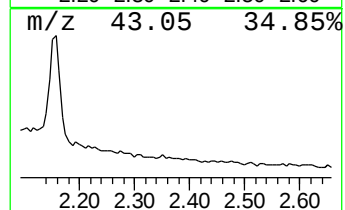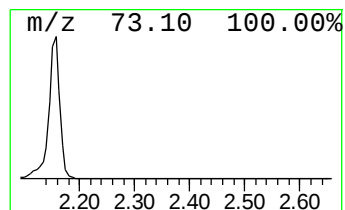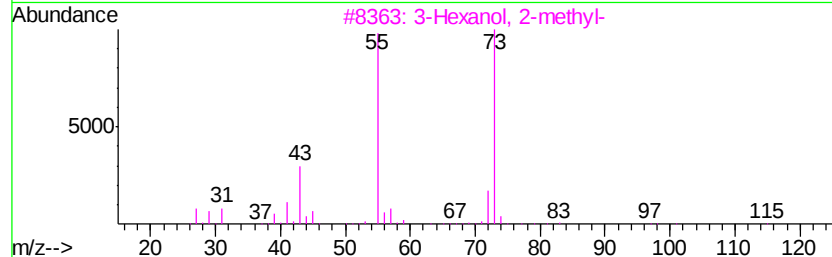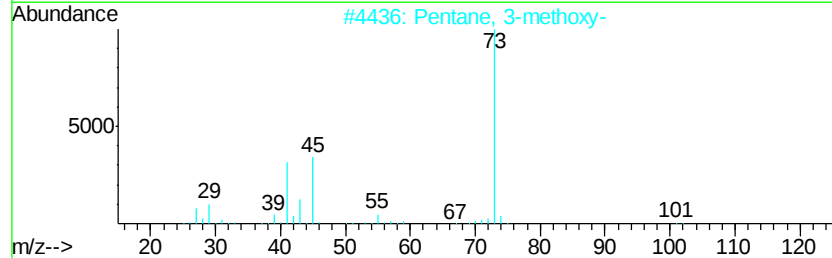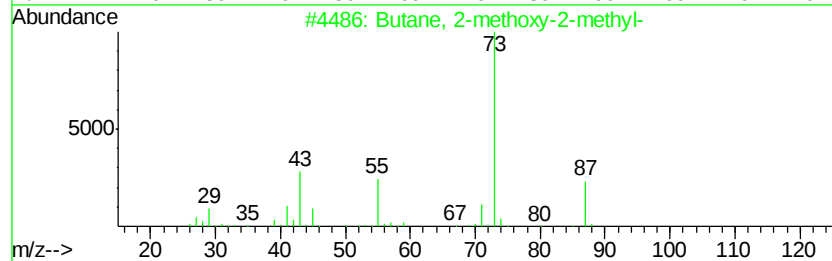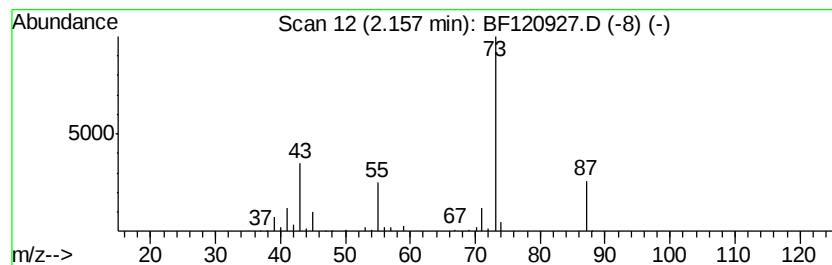

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072020\
Data File : BF120927.D
Acq On : 20 Jul 2020 9:57
Operator : JU/CG
Sample : PB130275BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130275BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	2.16	4.0	ng	253404	1	6.82	1276210	20.0