

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072022\
 Data File : BF129291.D
 Acq On : 20 Jul 2022 14:02
 Operator : CG\JU
 Sample : PB146238BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146238BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129291.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.016	285	294	301	rBV	99333	133244	1.64%	0.266%
2	5.528	545	551	554	rBV	5977487	6513101	80.24%	12.992%
3	6.522	714	720	723	rBV	5444603	6626007	81.63%	13.217%
4	6.892	779	783	787	rBV	1814910	1428189	17.59%	2.849%
5	7.457	873	879	882	rBV	4123224	4428784	54.56%	8.834%
6	8.175	996	1001	1005	rBV	2186083	1957594	24.12%	3.905%
7	9.257	1178	1185	1188	rBV	6963771	7639704	94.12%	15.239%
8	9.933	1295	1300	1304	rBV	2665252	2225448	27.42%	4.439%
9	10.728	1428	1435	1438	rBV	5208956	4993876	61.52%	9.961%
10	11.427	1549	1554	1557	rBV	2440290	2255017	27.78%	4.498%
11	13.016	1819	1824	1827	rBV	7793291	8117048	100.00%	16.191%
12	14.069	1999	2003	2007	rBV	2279390	2033932	25.06%	4.057%
13	15.563	2251	2257	2267	rBV	1407823	1781201	21.94%	3.553%




Sum of corrected areas: 50133145

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072022\
Data File : BF129291.D
Acq On : 20 Jul 2022 14:02
Operator : CG\JU
Sample : PB146238BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146238BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

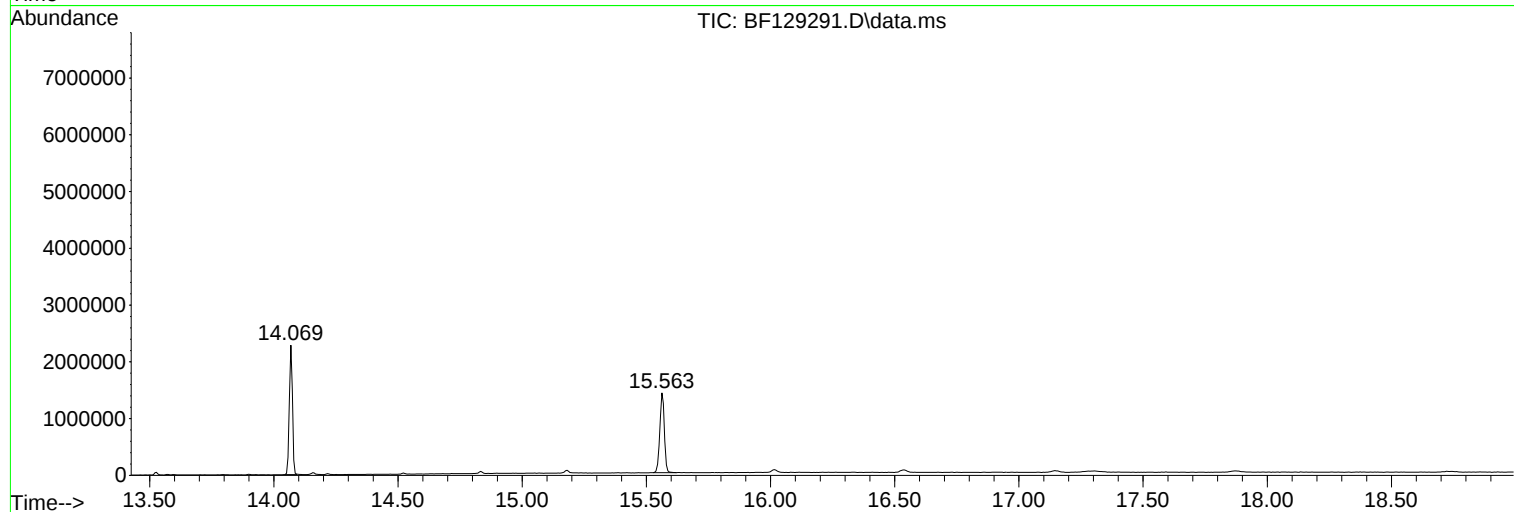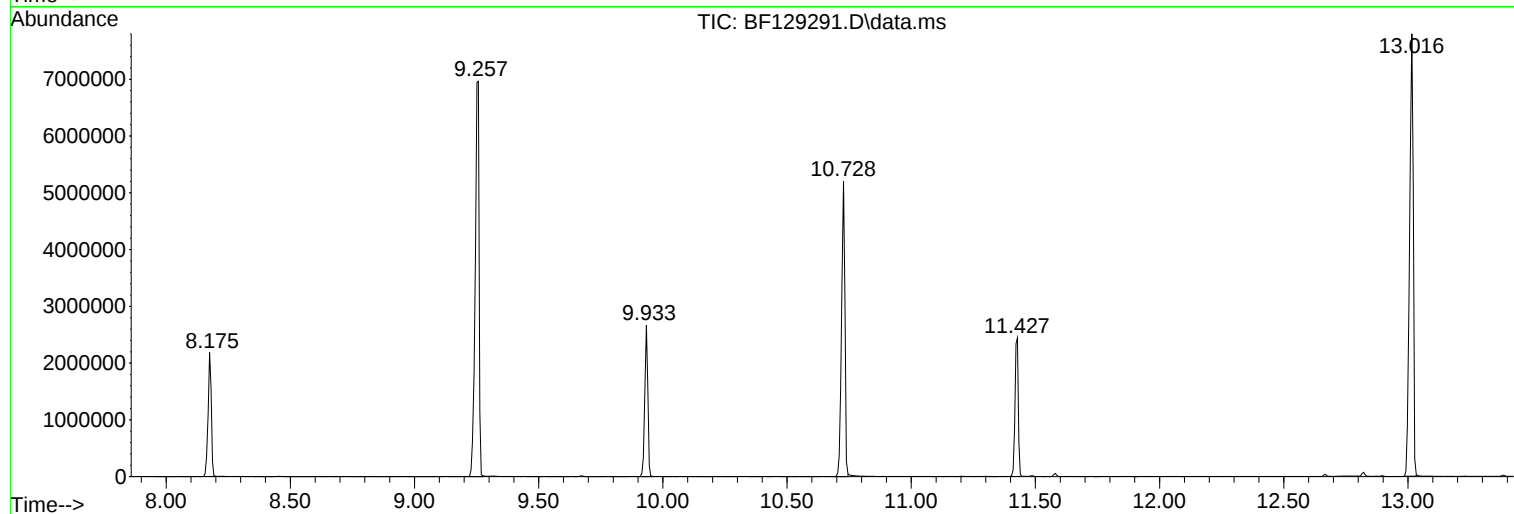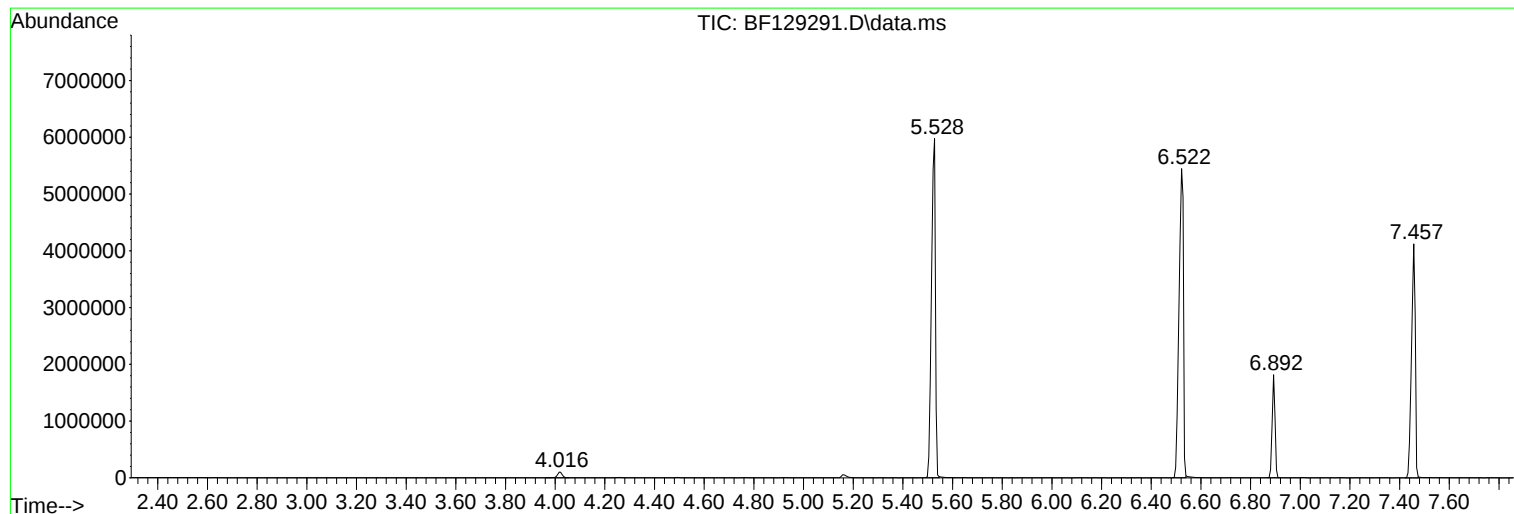

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072022\
Data File : BF129291.D
Acq On : 20 Jul 2022 14:02
Operator : CG\JU
Sample : PB146238BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146238BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072022\
Data File : BF129291.D
Acq On : 20 Jul 2022 14:02
Operator : CG\JU
Sample : PB146238BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146238BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------