


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072022\
 Data File : BF129282.D
 Acq On : 20 Jul 2022 09:05
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 20 13:42:18 2022

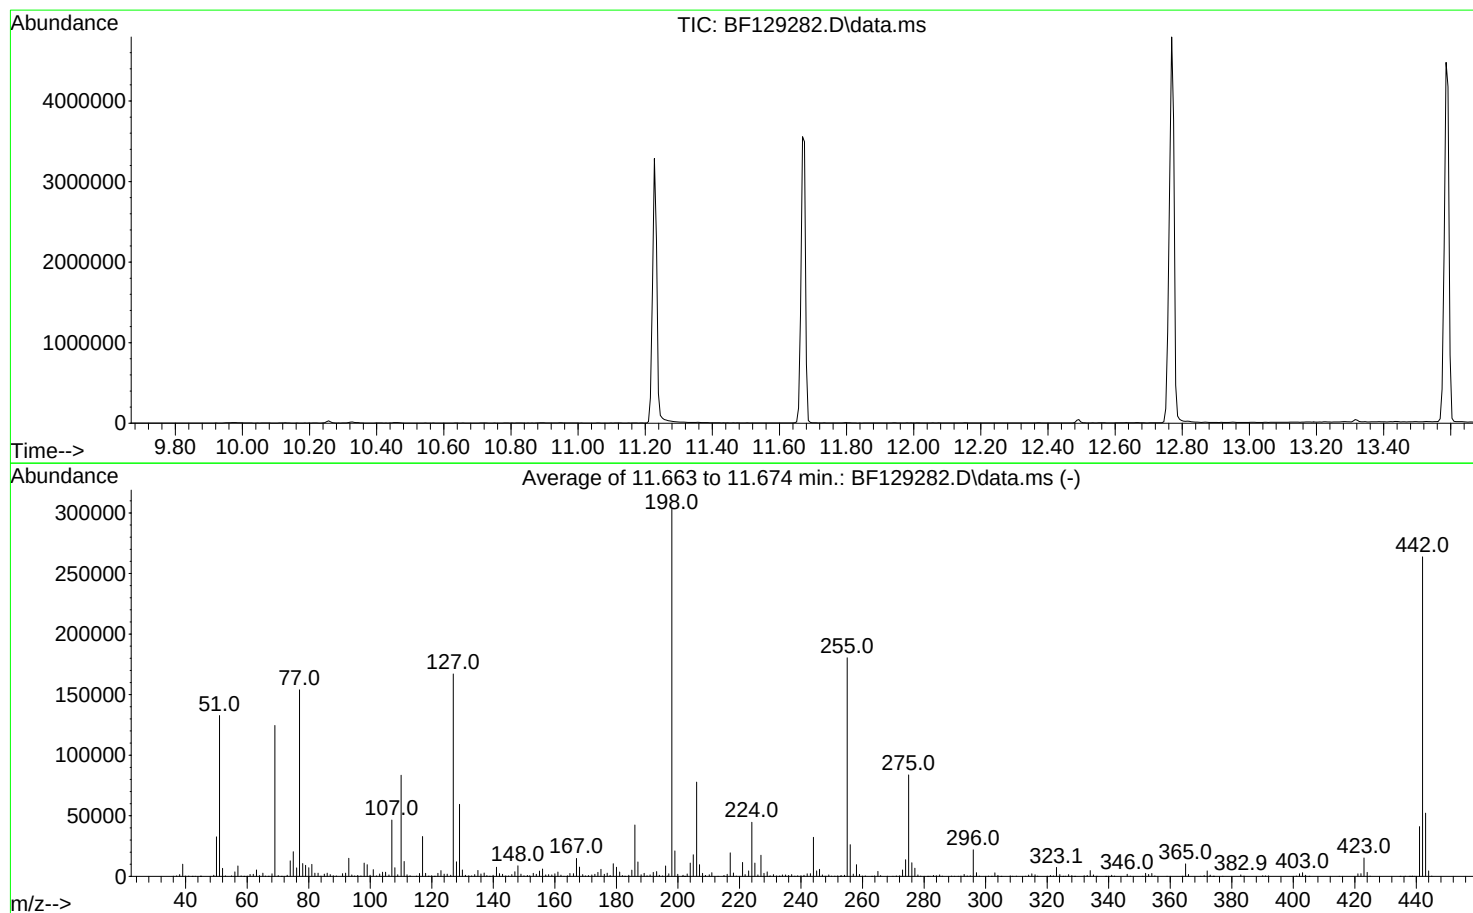

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	132685	PASS
68	69	0.00	2	1.7	2150	PASS
69	198	0.00	100	41.0	124563	PASS
70	69	0.00	2	0.6	719	PASS
127	198	10	80	55.0	167059	PASS
197	198	0.00	2	0.7	2157	PASS
198	198	100	100	100.0	303637	PASS
199	198	5	9	6.9	21019	PASS
275	198	10	60	27.6	83789	PASS
365	198	1	100	3.4	10364	PASS
441	198	0.01	100	13.6	41148	PASS
442	442	50	100	100.0	263747	PASS
443	442	15	24	19.8	52171	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/20/2022	BNA_F	<u>BF129282.D</u>
Compound Name	Response	Retention Time
DDT	797056	13.59
DDD	887	13.28
DDE	446	12.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1333	798389	0.17

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072022\
Data File : BF129282.D
Acq On : 20 Jul 2022 09:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 20 11:49:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 11:45:37 2022
Response via : Initial Calibration

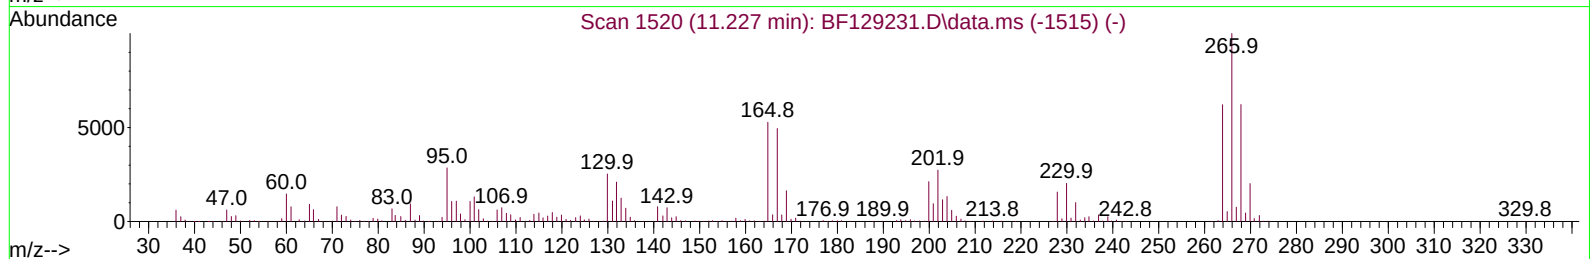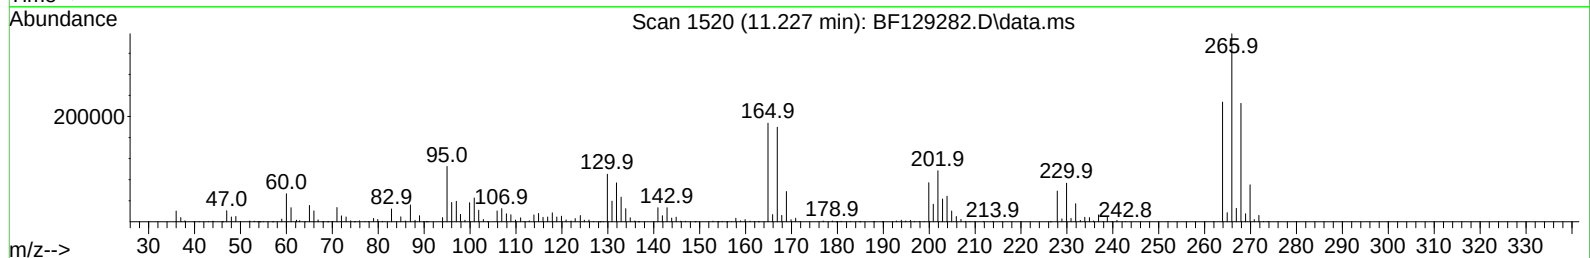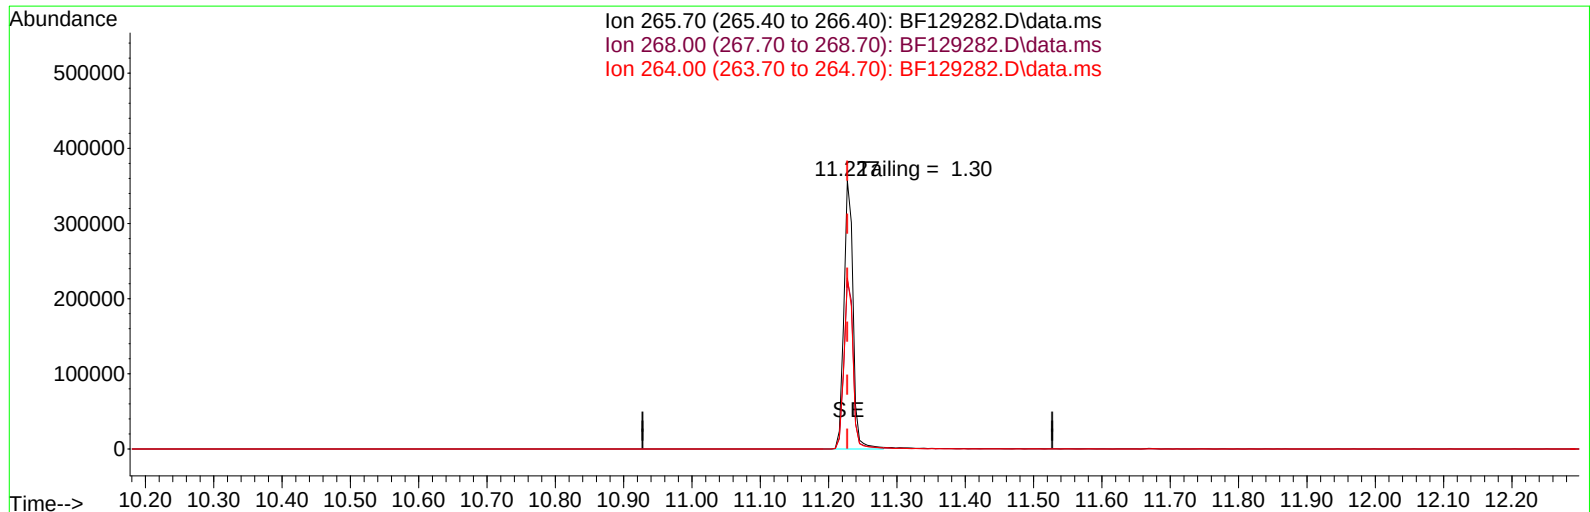

TIC: BF129282.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.000) 528072.82 ng




response 333099

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.96
264.00	61.80	63.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072022\
Data File : BF129282.D
Acq On : 20 Jul 2022 09:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 20 11:49:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 11:45:37 2022
Response via : Initial Calibration

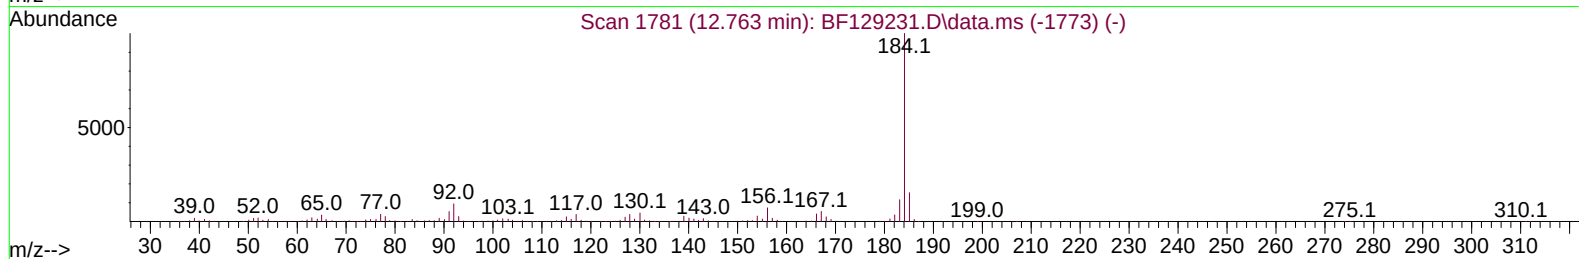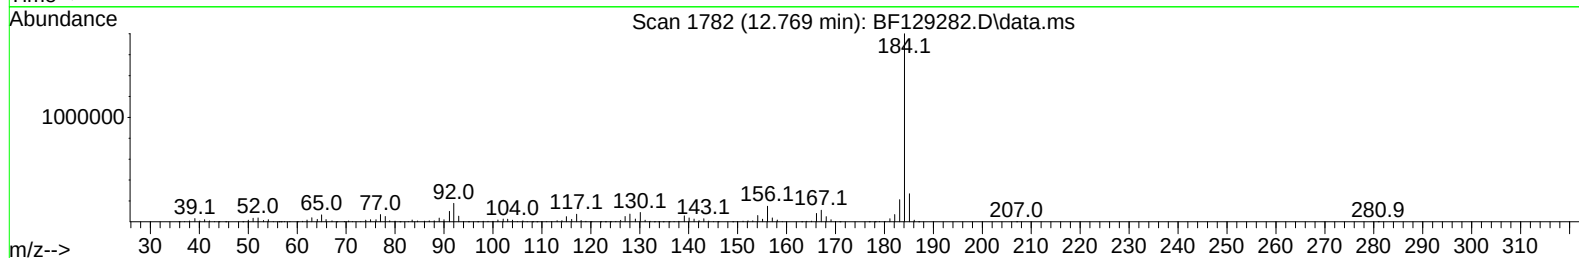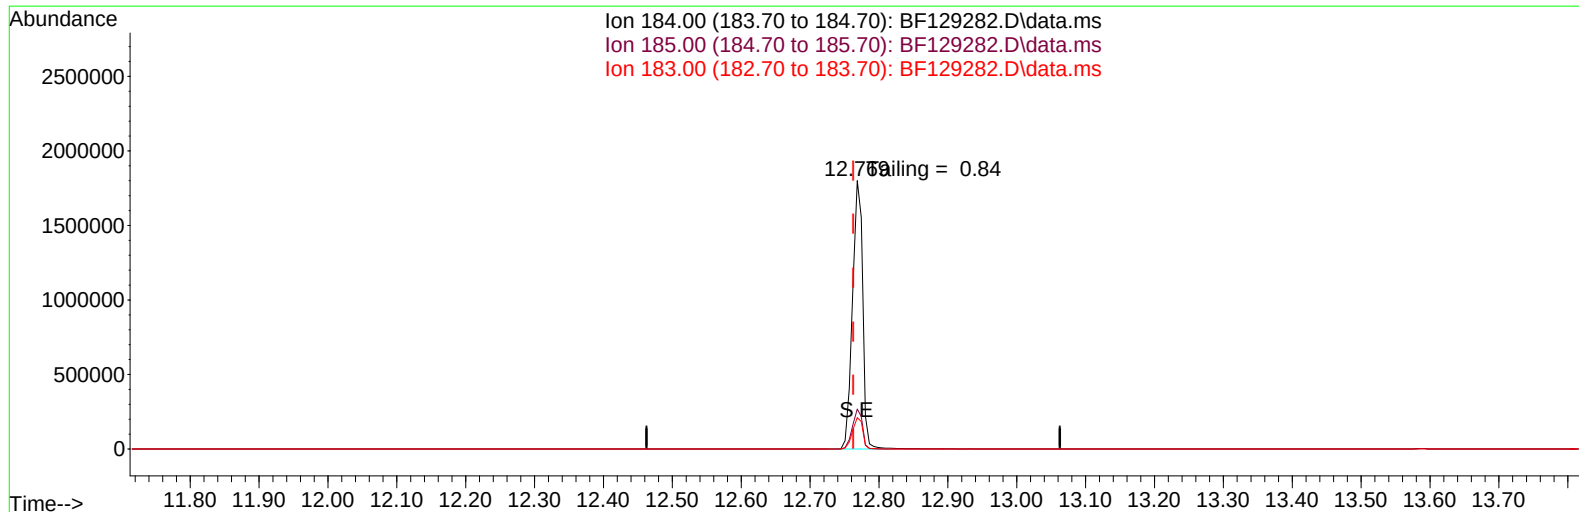

TIC: BF129282.D\data.ms

(77) Benzidine

12.769min (+ 0.006) 5779.63 ng m

response 1862276

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.94
183.00	11.60	11.73
0.00	0.00	0.00