

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072116\
 Data File : BF089170.D
 Acq On : 21 Jul 2016 10:15
 Operator : UM/SJ
 Sample : H4073-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TS-04

Quant Time: Jul 21 16:57:25 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 19:03:15 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.59	152	50545	20.00	ng	-0.01
21) Naphthalene-d8	7.88	136	221960	20.00	ng	0.00
38) Acenaphthene-d10	9.62	164	100953	20.00	ng	-0.01
63) Phenanthrene-d10	11.10	188	197731	20.00	ng	-0.01
75) Chrysene-d12	13.71	240	125094	20.00	ng	-0.01
86) Perylene-d12	15.06	264	90383	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.18	112	115773	34.84	ng	-0.01
7) Phenol-d6	6.25	99	148715	34.70	ng	-0.02
23) Nitrobenzene-d5	7.16	82	94717	22.67	ng	-0.01
41) 2,4,6-Tribromophenol	10.41	330	33400	36.75	ng	-0.01
44) 2-Fluorobiphenyl	8.96	172	204589	27.92	ng	-0.01
78) Terphenyl-d14	12.69	244	213579	37.03	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.36	163	101815	13.14	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072116\
Data File : BF089170.D
Acq On : 21 Jul 2016 10:15
Operator : UM/SJ
Sample : H4073-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TS-04

Quant Time: Jul 21 16:57:25 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 19:03:15 2016
Response via : Initial Calibration

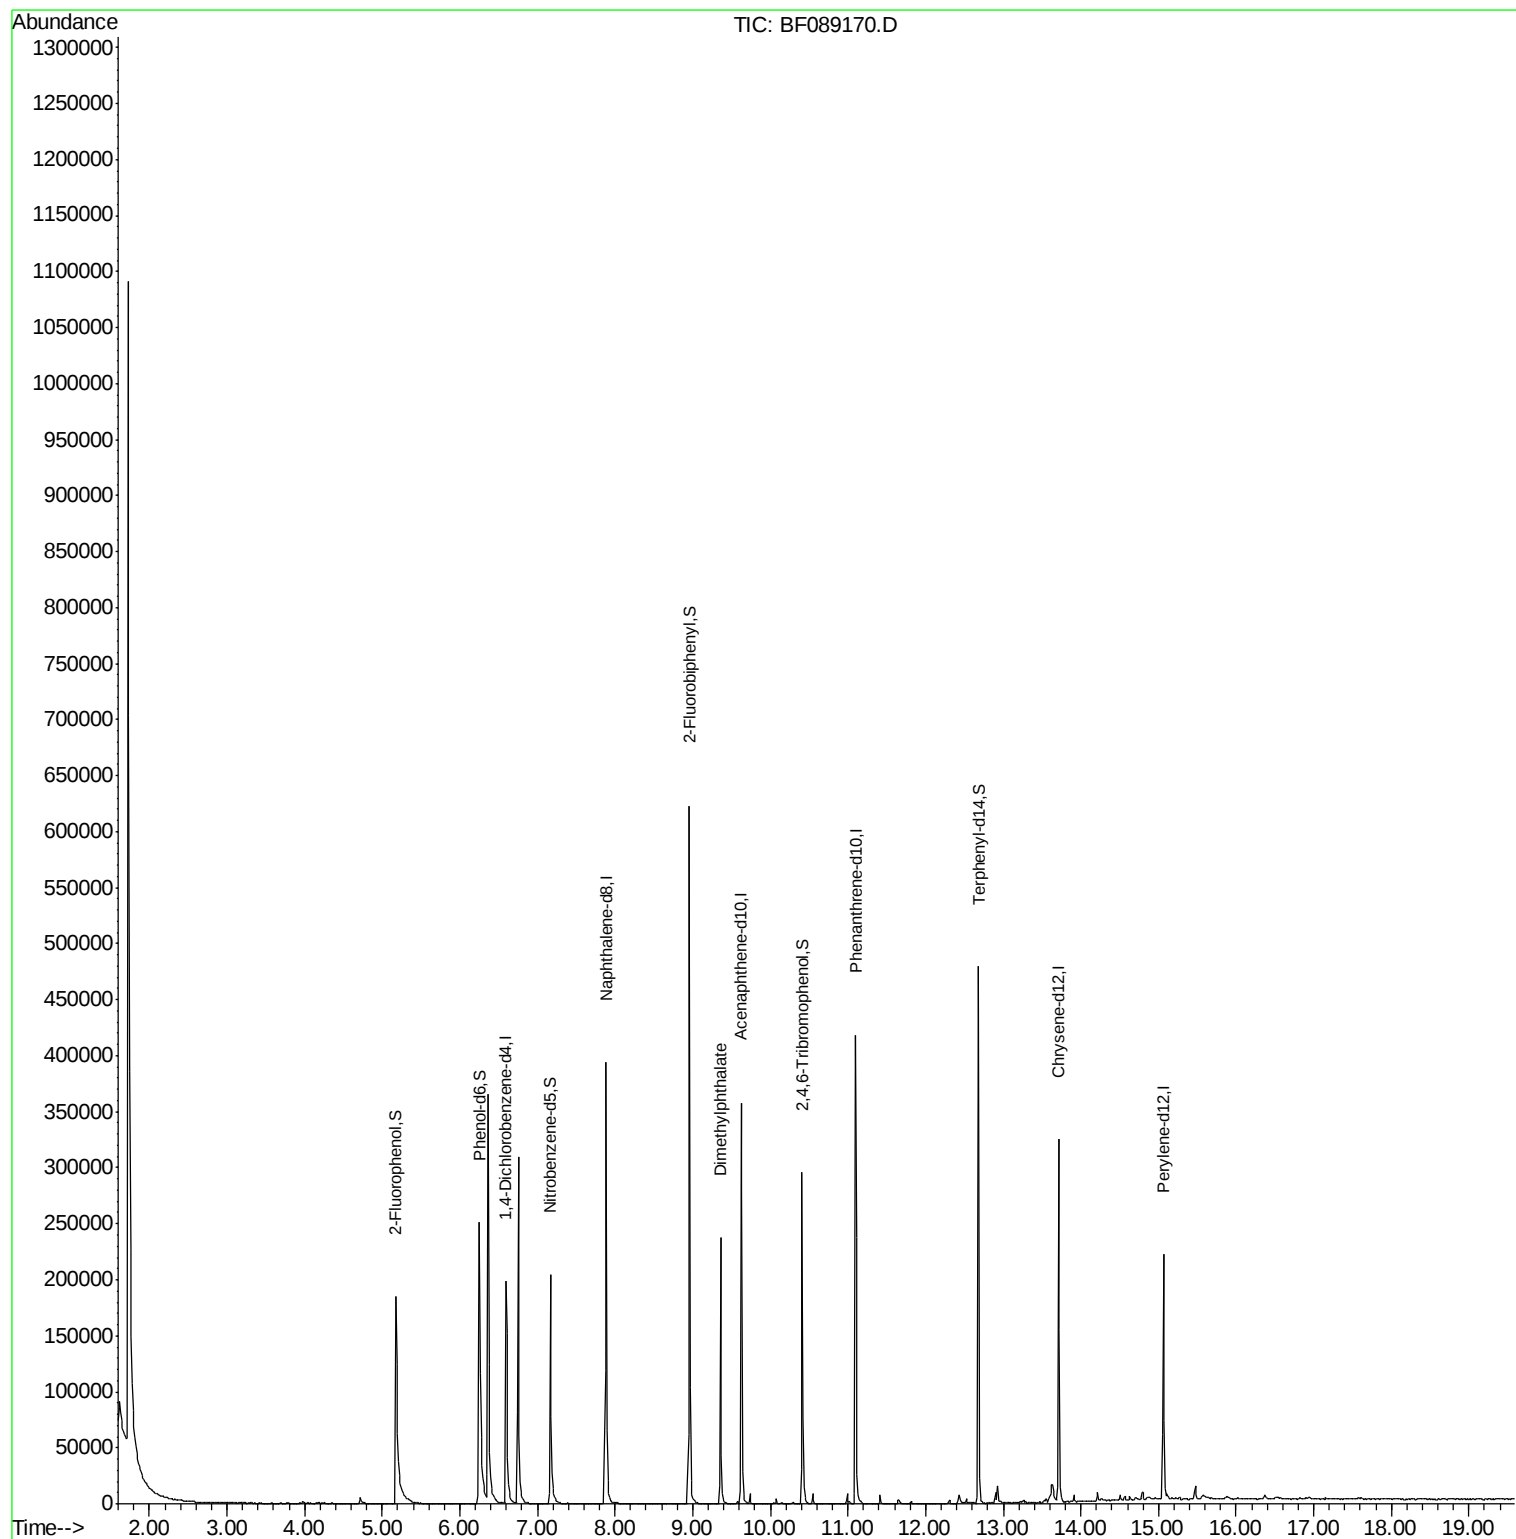

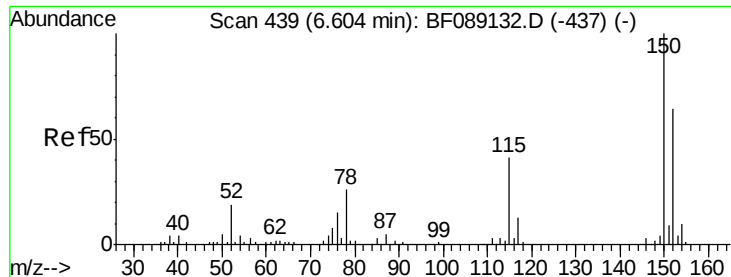

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.59 min Scan# 438

Delta R.T. -0.01 min

Lab File: BF089170.D

Acq: 21 Jul 2016 10:15

Instrument :

BNA_F

ClientSampleId :

TS-04


Tot Ion:152 Resp: 50545

Ion Ratio Lower Upper

152 100

150 157.8 125.1 187.7




115 76.0 51.1 76.7

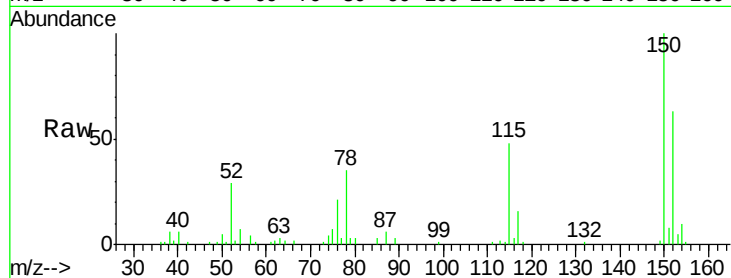

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

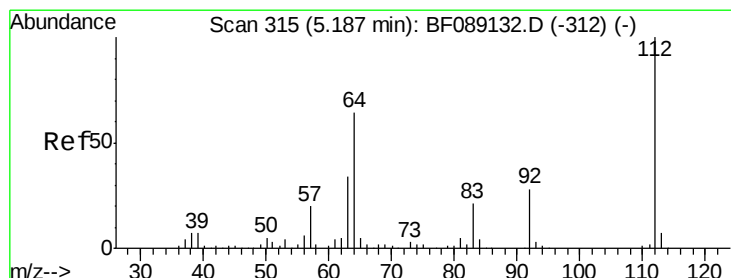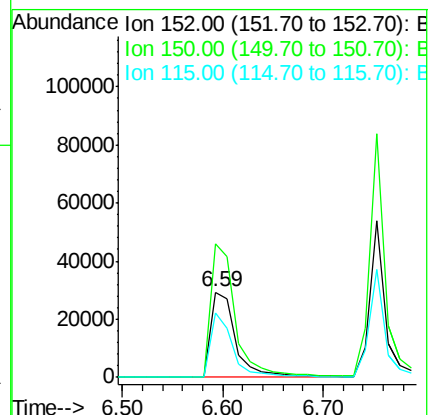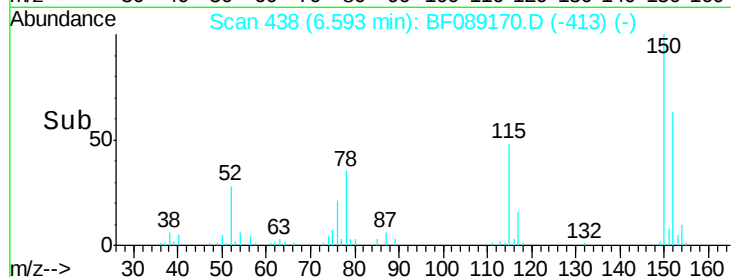

#5

2-Fluorophenol

Concen: 34.84 ng

RT: 5.18 min Scan# 314

Delta R.T. -0.01 min

Lab File: BF089170.D

Acq: 21 Jul 2016 10:15


Tgt Ion:112 Resp: 115773

Ion Ratio Lower Upper

112 100

64 64.2 51.0 76.4



63 34.2 27.3 40.9

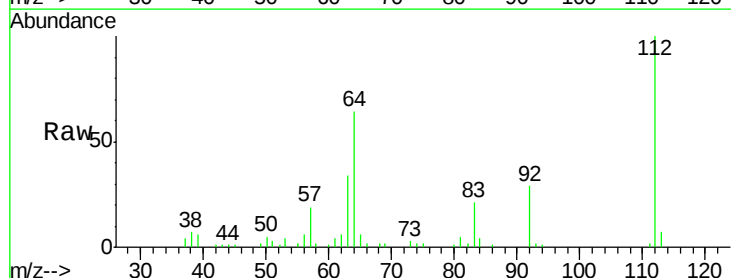


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

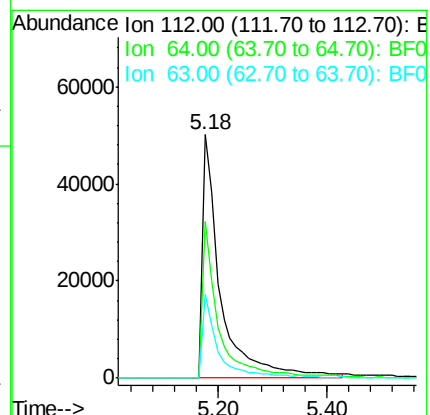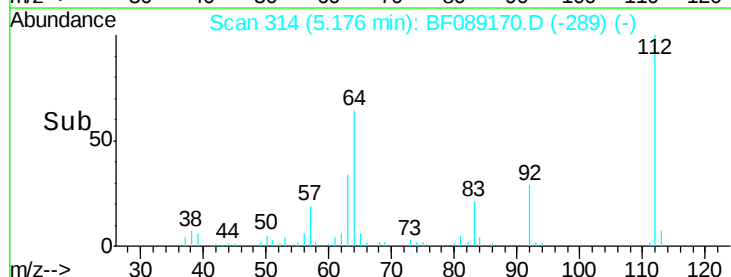

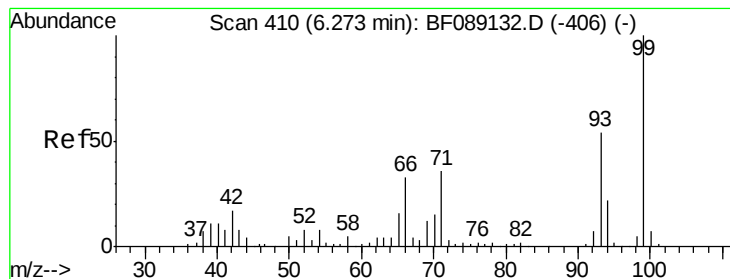

#7

Phenol-d6

Concen: 34.70 ng

RT: 6.25 min Scan# 408

Delta R.T. -0.02 min

Lab File: BF089170.D

Acq: 21 Jul 2016 10:15

Instrument :

BNA_F

ClientSampleId :

TS-04


Tot Ion: 99 Resp: 148715

Ion Ratio Lower Upper

99 100

42 16.4 13.5 20.3




71 35.9 28.9 43.3

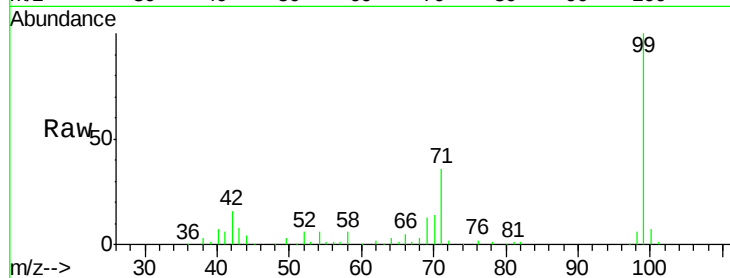

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

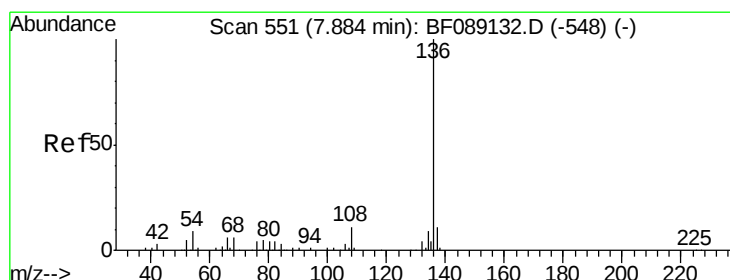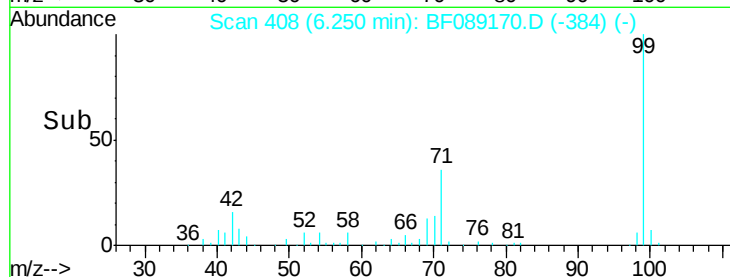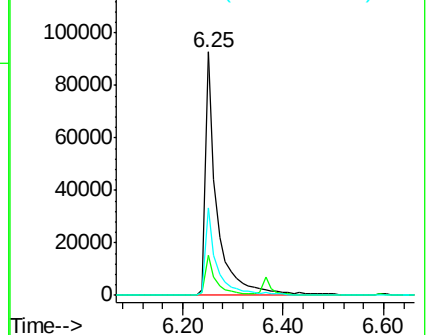

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.88 min Scan# 551

Delta R.T. 0.00 min

Lab File: BF089170.D

Acq: 21 Jul 2016 10:15

Tgt Ion: 136 Resp: 221960


Ion Ratio Lower Upper

136 100

137 10.8 8.8 13.2

54 6.3 7.0 10.4#

68 5.0 5.0 7.6#


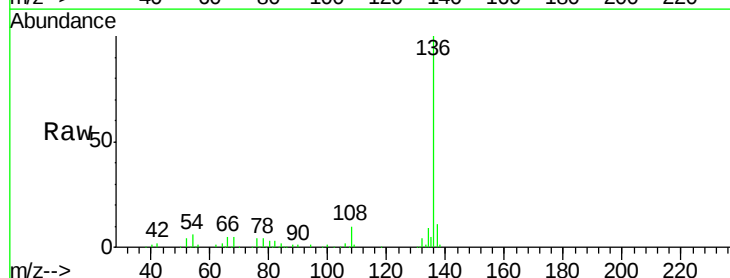



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

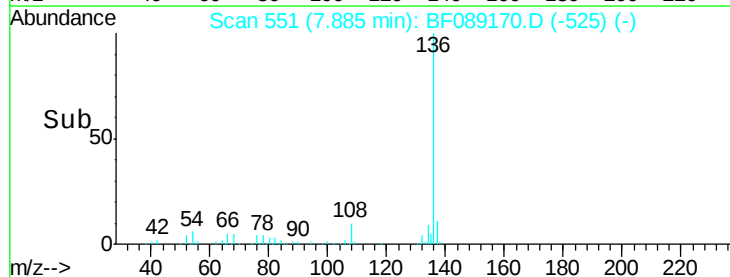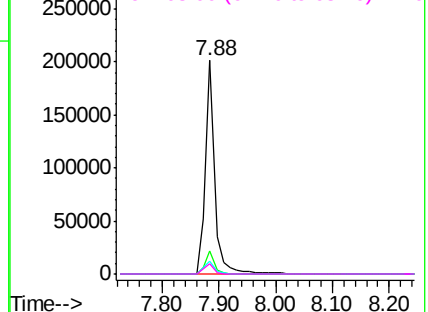


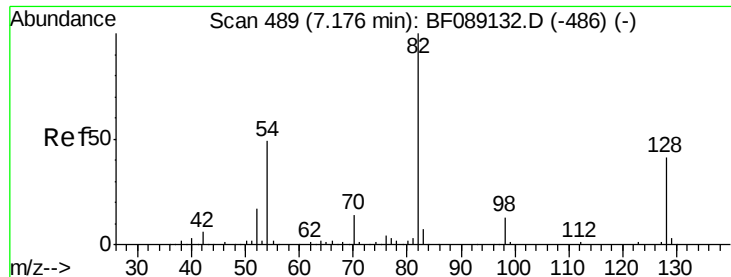




#23
 Nitrobenzene-d5
 Concen: 22.67 ng
 RT: 7.16 min Scan# 488
 Delta R.T. -0.01 min
 Lab File: BF089170.D
 Acq: 21 Jul 2016 10:15

Instrument :
 BNA_F
 ClientSampleId :
 TS-04

Tot Ion	82	Resp	94717
Ion Ratio	100	Lower	Upper
128	39.2	33.0	49.6
54	47.2	39.0	58.4

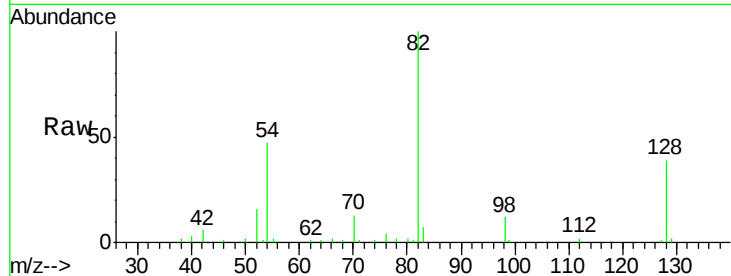


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

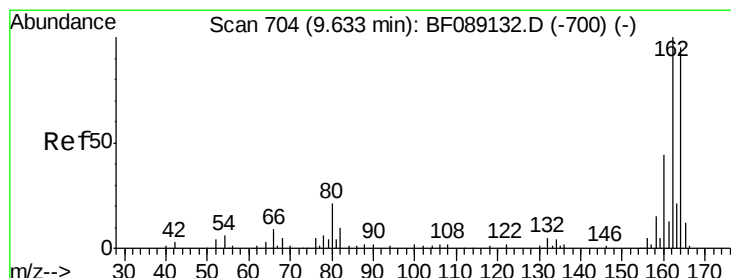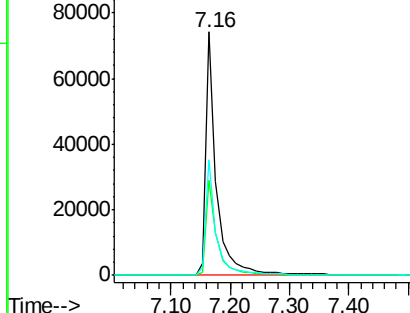
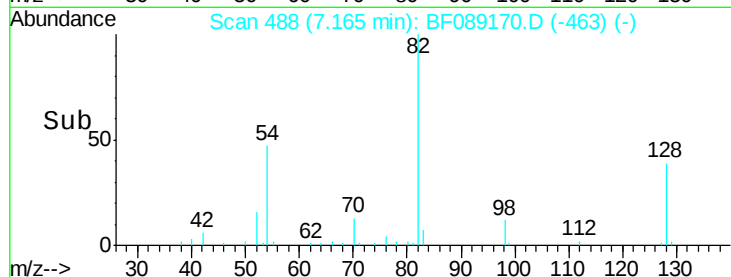



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.62 min Scan# 703
 Delta R.T. -0.01 min
 Lab File: BF089170.D
 Acq: 21 Jul 2016 10:15

Tgt Ion	164	Resp	100953
Ion Ratio	100	Lower	Upper
162	105.0	84.1	126.1
160	46.4	37.1	55.7

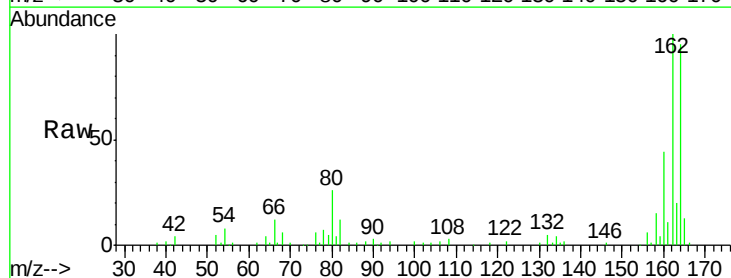

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

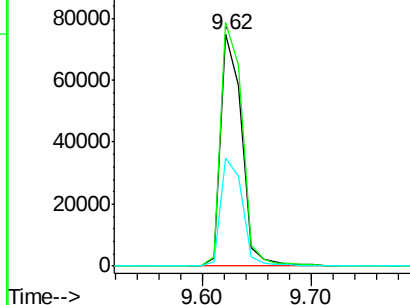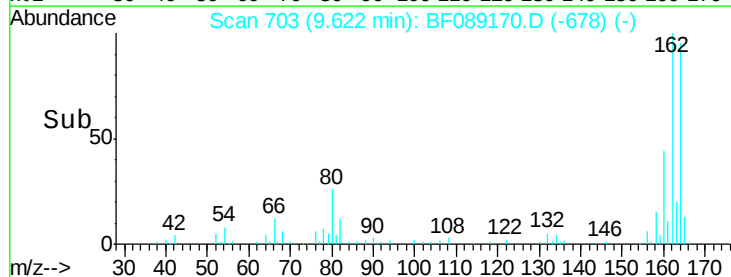


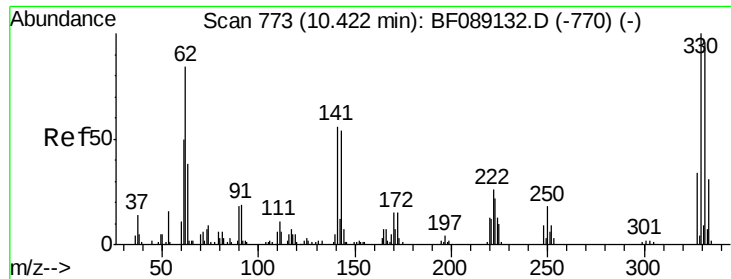




#41
 2,4,6-Tribromophenol
 Concen: 36.75 ng
 RT: 10.41 min Scan# 772
 Delta R.T. -0.01 min
 Lab File: BF089170.D
 Acq: 21 Jul 2016 10:15

Instrument :
 BNA_F
 ClientSampleId :
 TS-04

Tot Ion:330 Resp: 33400
 Ion Ratio Lower Upper
 330 100
 332 98.3 77.2 115.8
 141 48.5 42.2 63.2

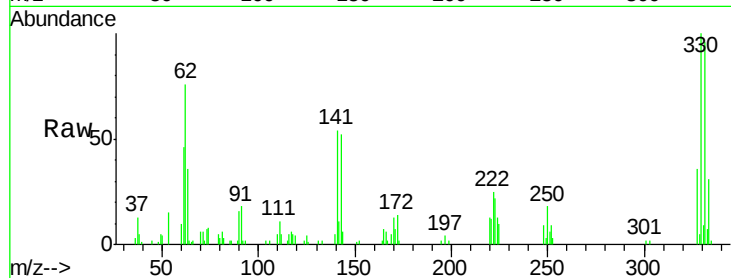


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

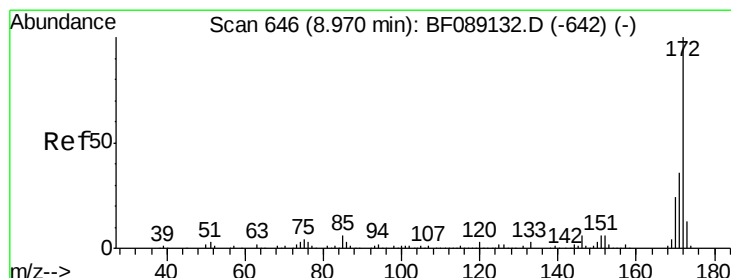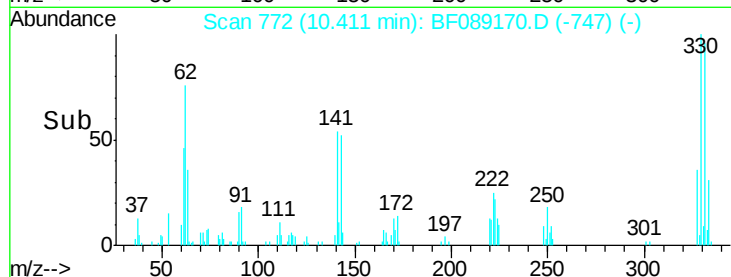
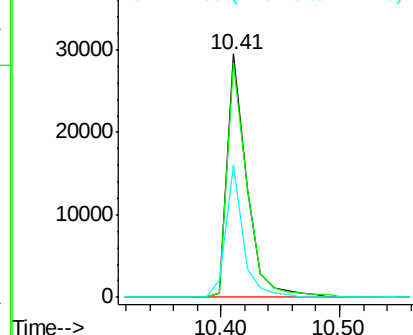



#44
 2-Fluorobiphenyl
 Concen: 27.92 ng
 RT: 8.96 min Scan# 645
 Delta R.T. -0.01 min
 Lab File: BF089170.D
 Acq: 21 Jul 2016 10:15

Tgt Ion:172 Resp: 204589
 Ion Ratio Lower Upper
 172 100
 171 35.2 29.2 43.8
 170 23.2 19.1 28.7

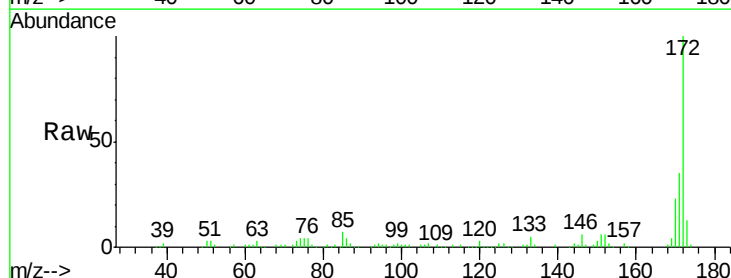

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

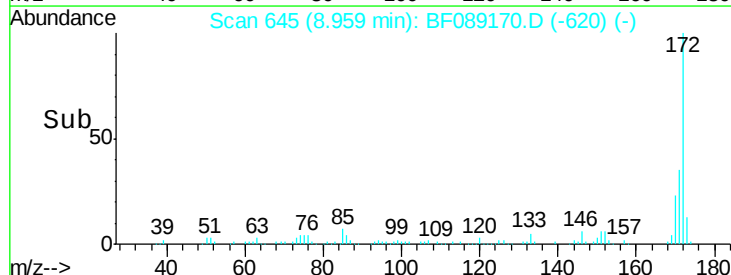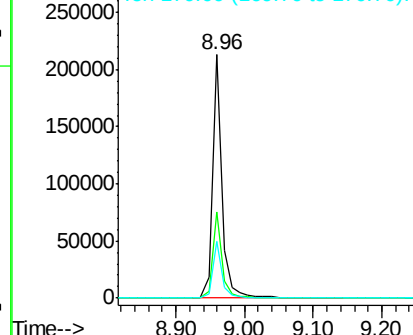

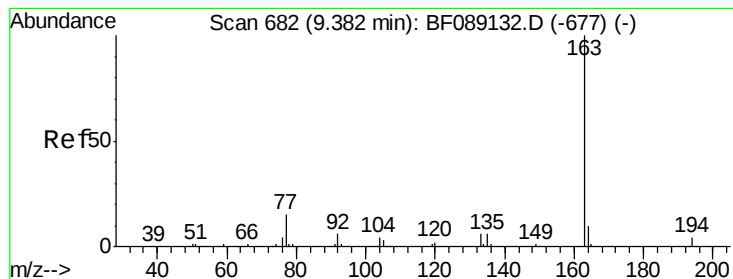

#49

Dimethylphthalate

Concen: 13.14 ng

RT: 9.36 min Scan# 680

Delta R.T. -0.02 min

Lab File: BF089170.D

Acq: 21 Jul 2016 10:15

Instrument :

BNA_F

ClientSampleId :

TS-04


Tot Ion:163 Resp: 101815

Ion Ratio Lower Upper

163 100

194 3.2 2.9 4.3




164 10.0 7.6 11.4

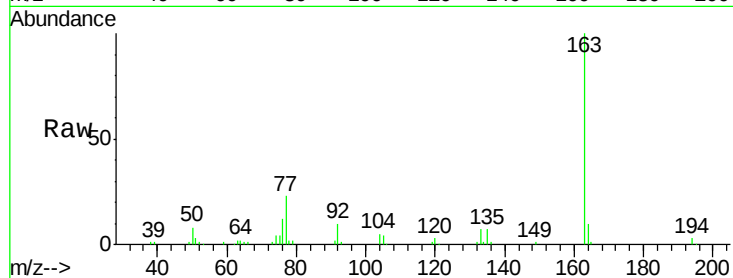

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

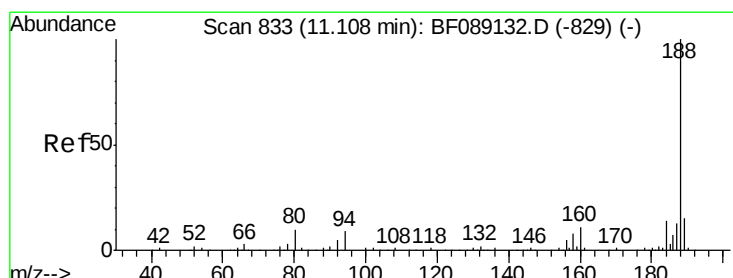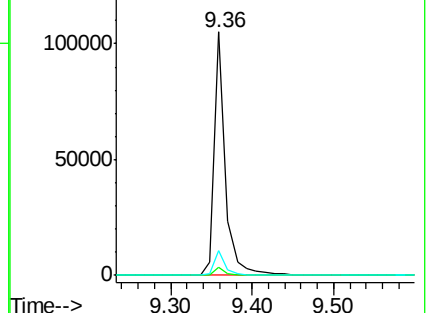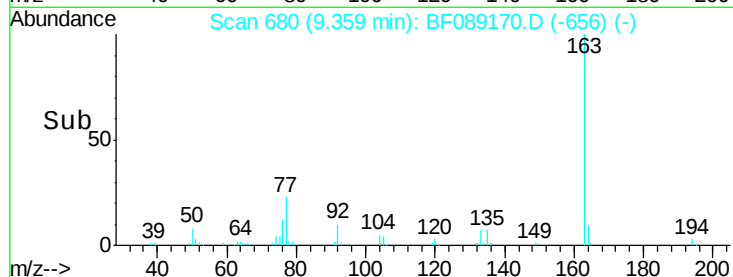

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.10 min Scan# 832

Delta R.T. -0.01 min

Lab File: BF089170.D

Acq: 21 Jul 2016 10:15


Tgt Ion:188 Resp: 197731

Ion Ratio Lower Upper

188 100

94 12.0 7.0 10.4#



80 14.1 7.7 11.5#

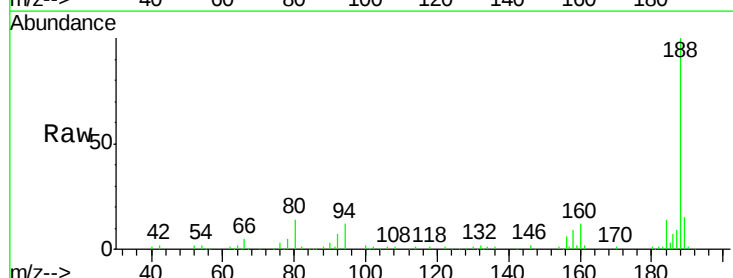


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

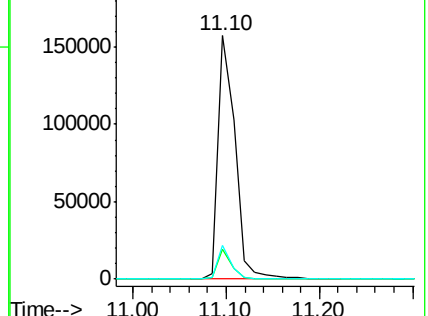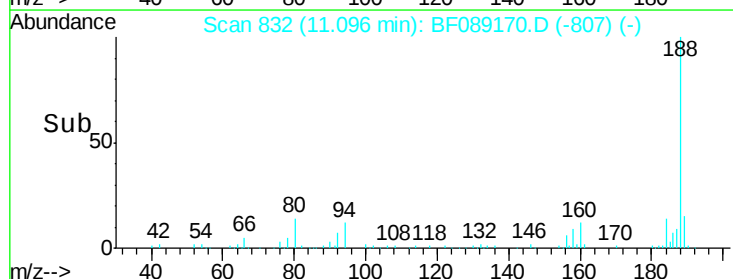

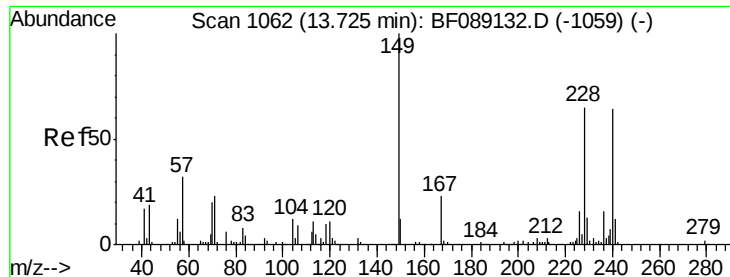

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.71 min Scan# 1061

Delta R.T. -0.01 min

Lab File: BF089170.D

Acq: 21 Jul 2016 10:15

Instrument :

BNA_F

ClientSampled :

TS-04


Tot Ion:240 Resp: 125094

Ion Ratio Lower Upper

240 100

120 14.9 13.6 20.4




236 24.9 20.5 30.7

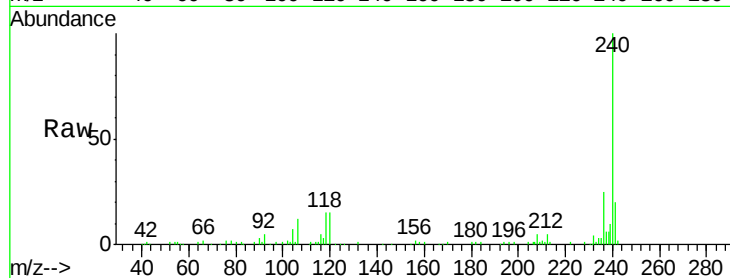

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

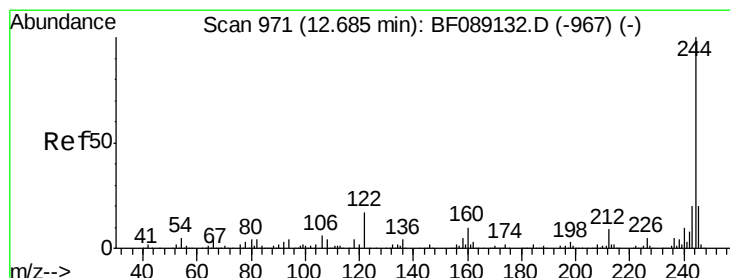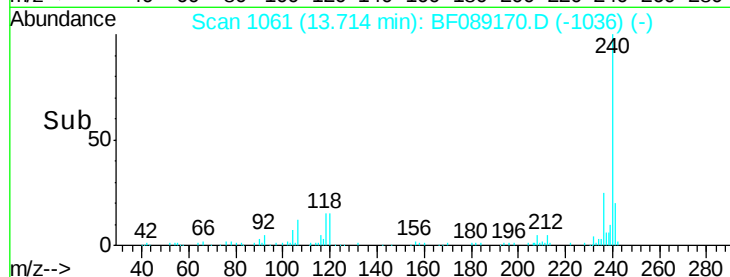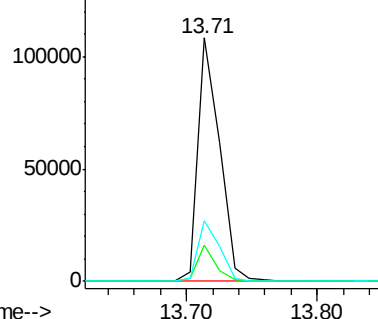

#78

Terphenyl-d14

Concen: 37.03 ng

RT: 12.69 min Scan# 971

Delta R.T. 0.00 min

Lab File: BF089170.D

Acq: 21 Jul 2016 10:15


Tgt Ion:244 Resp: 213579

Ion Ratio Lower Upper

244 100

212 7.2 7.0 10.4



122 8.0 13.8 20.8#



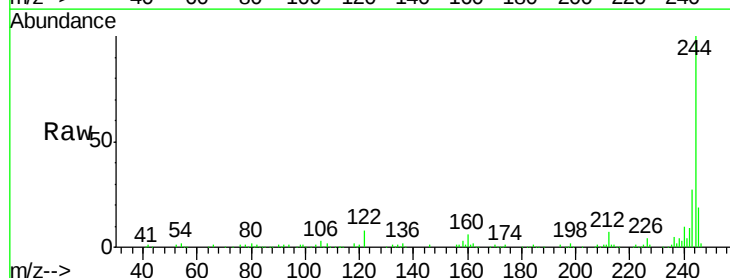


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

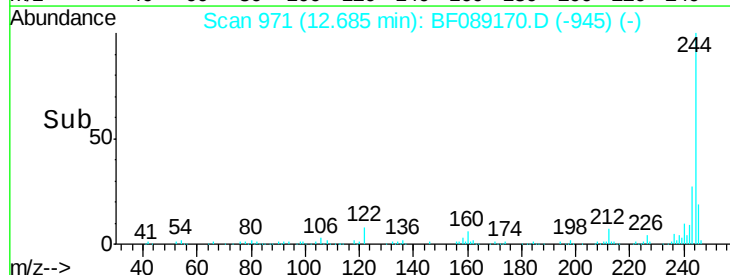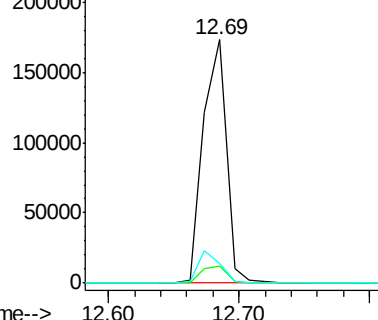

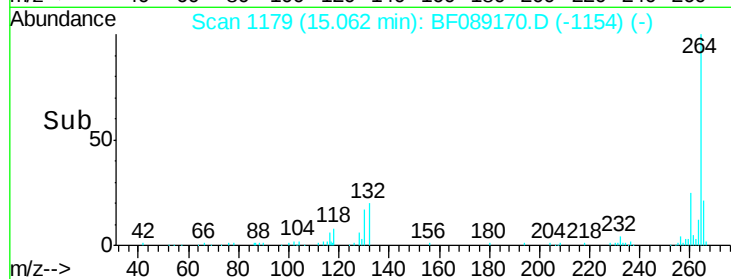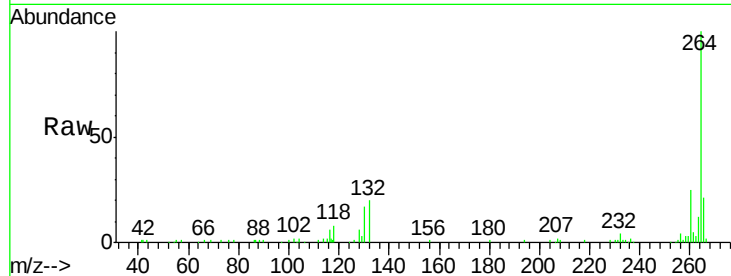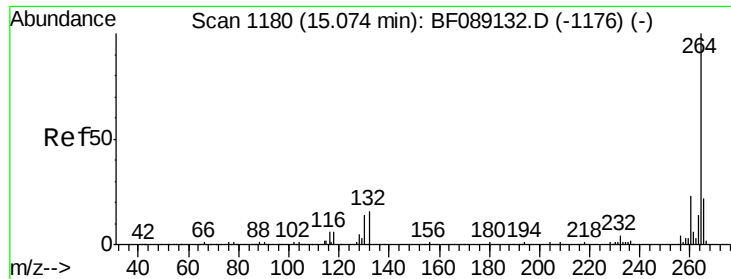

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 15.06 min Scan# 1179
 Delta R.T. -0.01 min
 Lab File: BF089170.D
 Acq: 21 Jul 2016 10:15

Instrument :
 BNA_F
 ClientSampleId :
 TS-04

Tot Ion: 264 Resp: 90383
 Ion Ratio Lower Upper
 264 100
 260 24.7 18.5 27.7
 265 21.2 17.3 25.9

