


Data Path : Z:\HPCHEM1\BNA F\DATA\BF072116\
 Data File : BF089161.D
 Acq On : 21 Jul 2016 5:49
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 20 19:03:15 2016

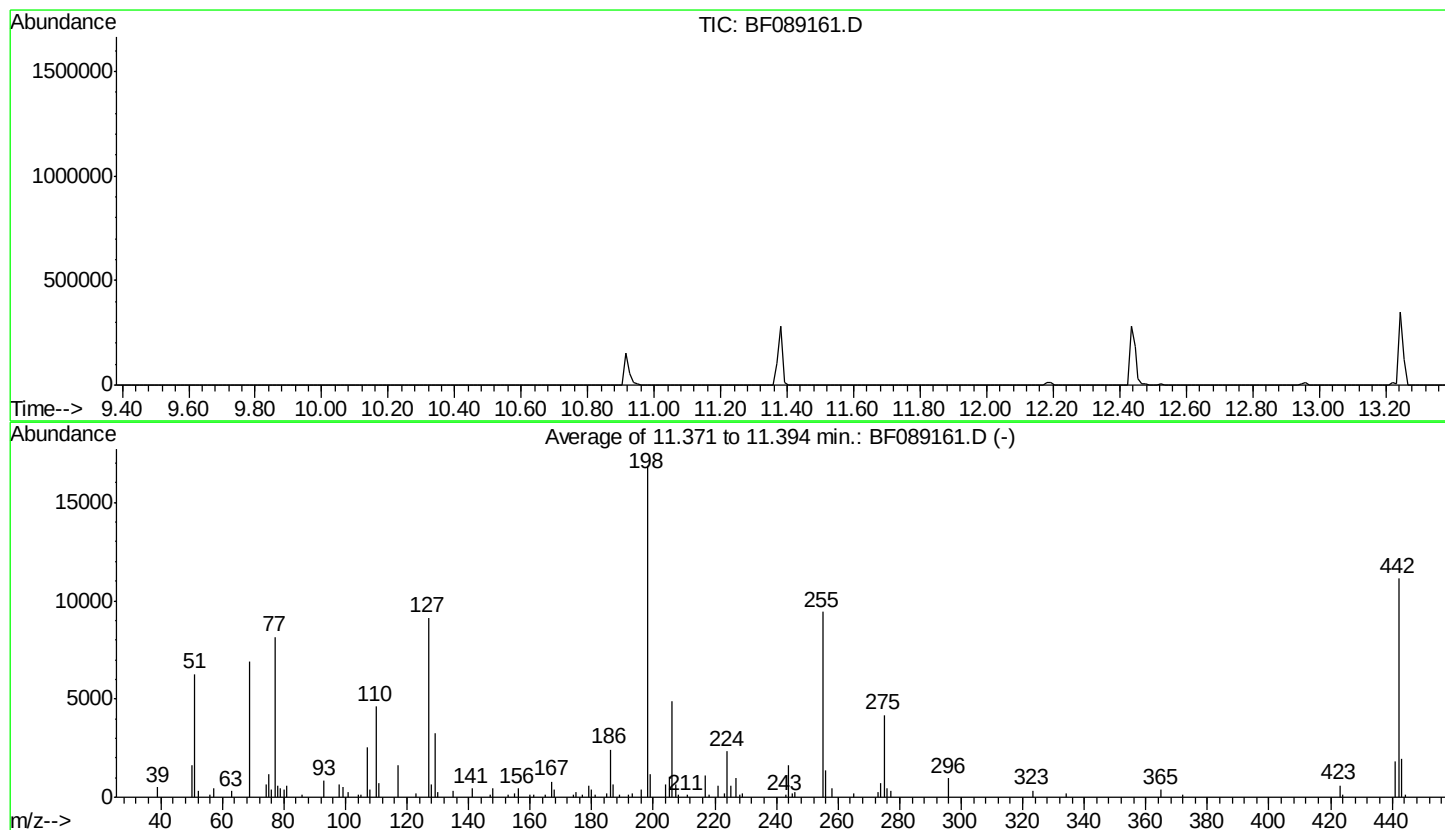

AutoFind: Scans 856, 857, 858; Background Corrected with Scan 853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	6258	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.1	6939	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.2	9140	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16877	PASS
199	198	5	9	6.9	1165	PASS
275	198	10	60	24.7	4172	PASS
365	198	1	100	2.3	387	PASS
441	442	0.01	24	16.2	1804	PASS
442	198	50	100	65.9	11126	PASS
443	442	15	24	17.5	1950	PASS