
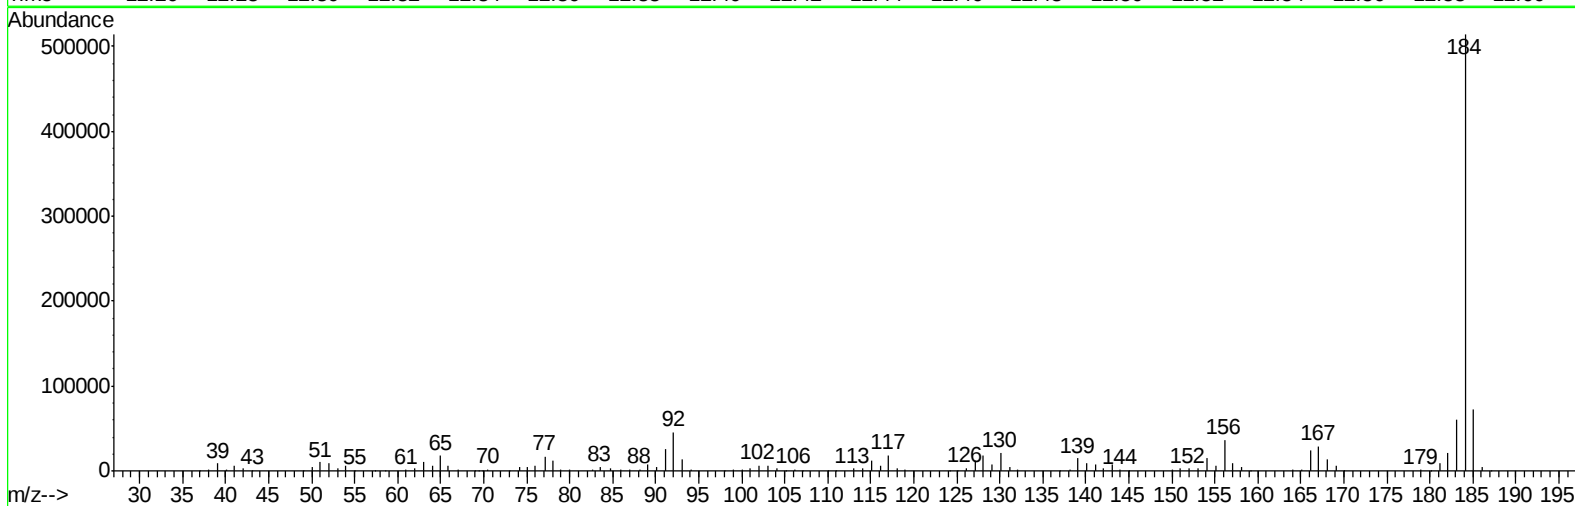


Data Path : Z:\HPCHEM1\BNA F\DATA\BF072117\
Data File : BF096936.D
Acq On : 21 Jul 2017 11:20
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 24 05:32:57 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 18 13:33:22 2017
Response via : Initial Calibration

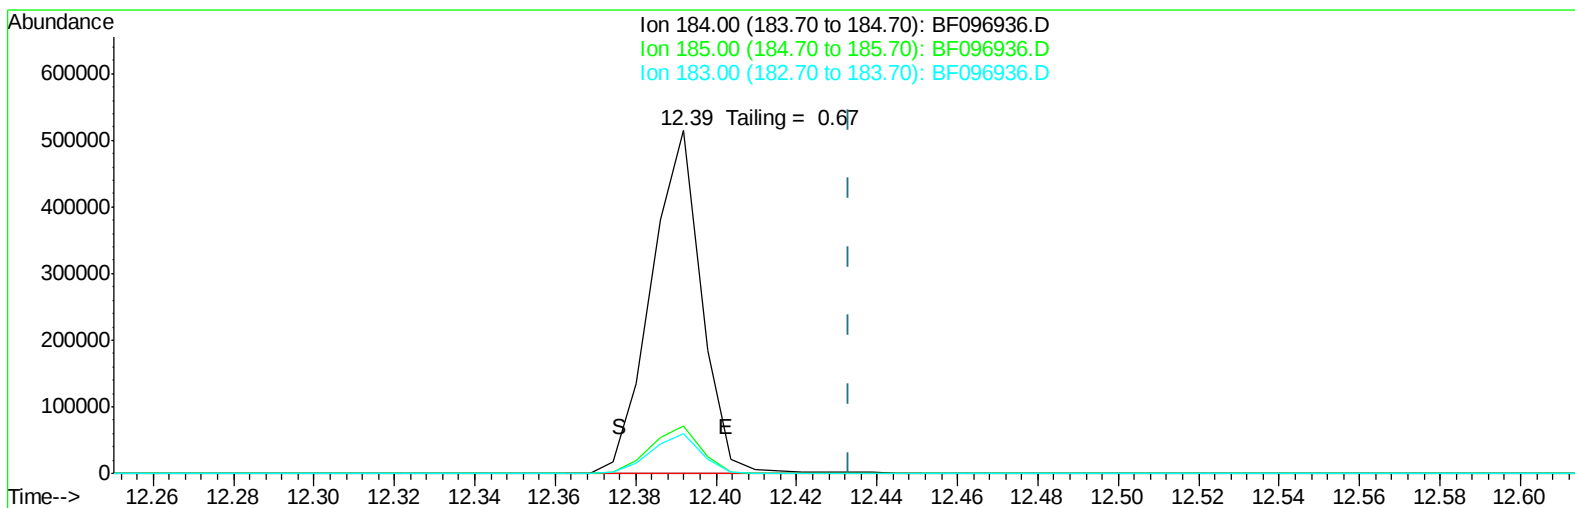

TIC: BF096936.D

(76) Benzidine



12.392min (-0.041) 26387.66ng

response 449525

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.97#
183.00	12.20	11.69
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072117\
Data File : BF096936.D
Acq On : 21 Jul 2017 11:20
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 24 05:32:57 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 18 13:33:22 2017
Response via : Initial Calibration

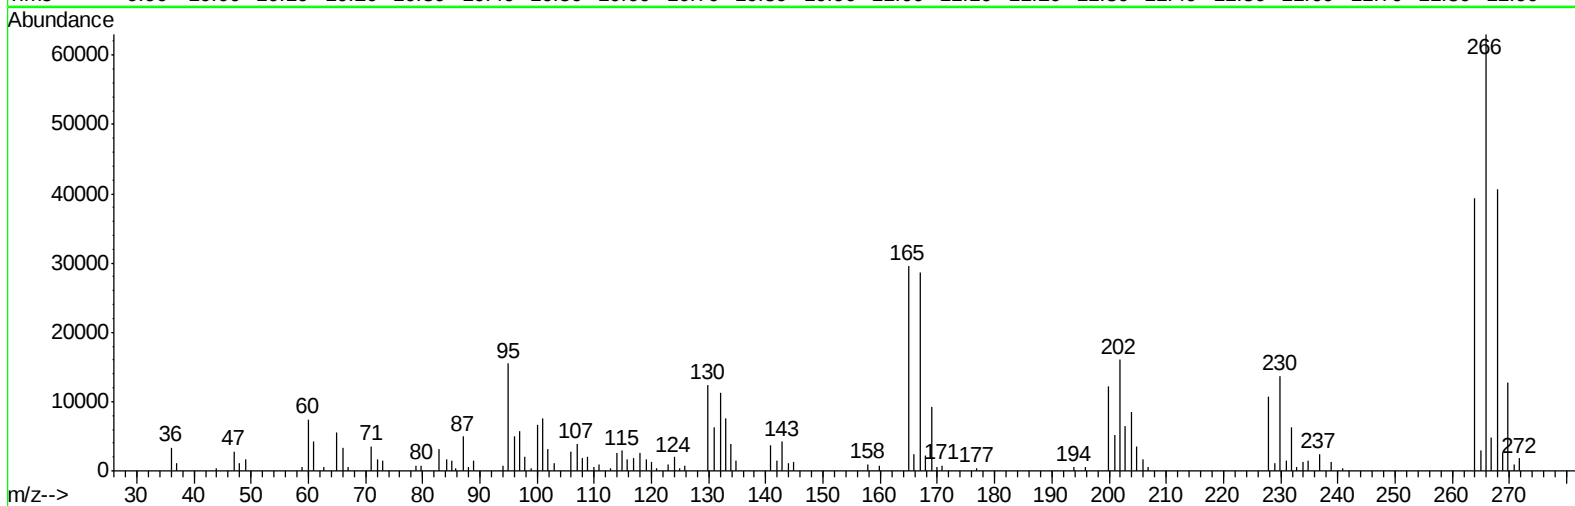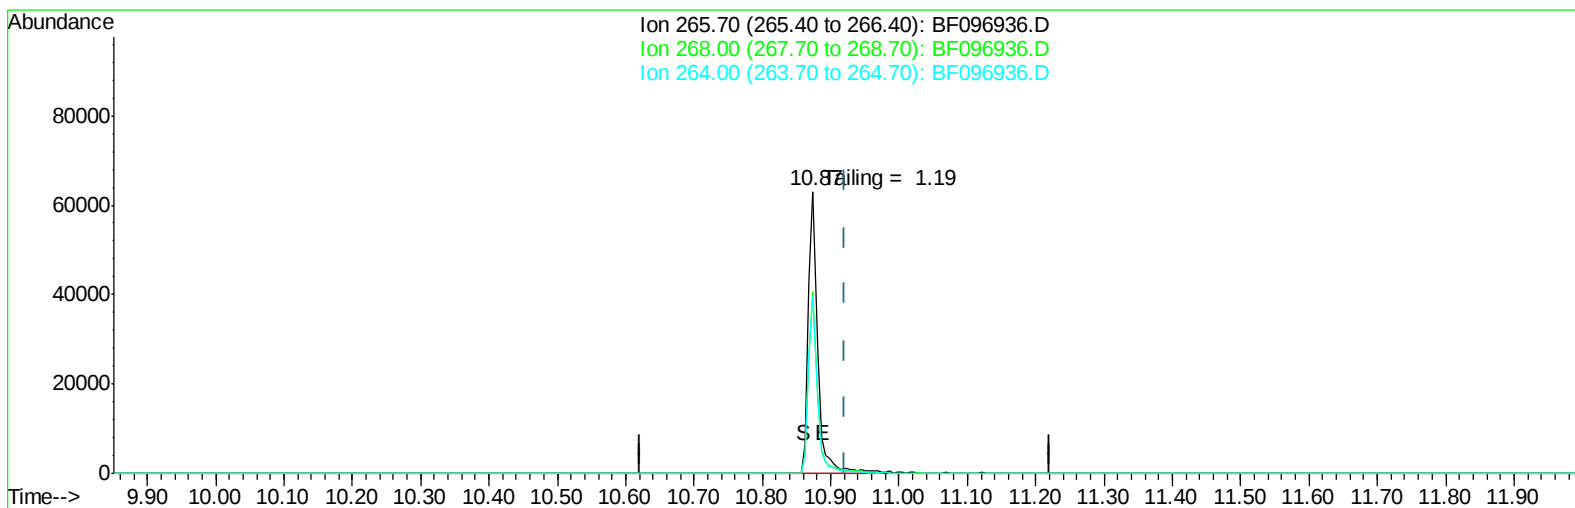

TIC: BF096936.D

(69) Pentachlorophenol (C)

10.874min (-0.047) 0.00ng

response 59355

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.46
264.00	64.60	62.57
0.00	0.00	0.00