

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072117\
 Data File : BF096967.D
 Acq On : 22 Jul 2017 3:43
 Operator : SJ/JU
 Sample : I4253-01DL 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-O-P-6-7-BASEDL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.781	471	475	486	rBV	401558	444138	22.86%	1.476%
2	5.151	535	538	547	rVV	319514	328625	16.92%	1.092%
3	6.081	691	696	698	rVV2	54327	62775	3.23%	0.209%
4	6.204	714	717	728	rVV	401254	396735	20.42%	1.318%
5	6.287	728	731	735	rVV	351036	346705	17.85%	1.152%
6	6.322	735	737	744	rVV	393492	363009	18.69%	1.206%
7	6.381	744	747	750	rVV	120980	102047	5.25%	0.339%
8	6.492	763	766	772	rBV	94084	99088	5.10%	0.329%
9	6.551	773	776	778	rBV	712608	693622	35.71%	2.304%
10	6.569	778	779	783	rVV2	368578	376894	19.40%	1.252%
11	6.604	783	785	789	rVB2	386099	317602	16.35%	1.055%
12	6.722	800	805	812	rVB2	1048758	1266709	65.21%	4.208%
13	6.840	822	825	828	rVV2	132808	162856	8.38%	0.541%
14	6.887	831	833	835	rVB2	85356	67247	3.46%	0.223%
15	7.116	866	872	875	rBV4	251604	356870	18.37%	1.186%
16	7.216	884	889	892	rVB3	47011	64213	3.31%	0.213%
17	7.251	892	895	897	rBV2	50495	60976	3.14%	0.203%
18	7.281	897	900	903	rVB4	59744	74503	3.84%	0.248%
19	7.334	906	909	911	rVB	84004	67344	3.47%	0.224%
20	7.363	911	914	920	rVB	164982	164114	8.45%	0.545%
21	7.469	927	932	936	rBV4	79273	124801	6.42%	0.415%
22	7.510	936	939	947	rBV6	171070	335739	17.28%	1.115%
23	7.581	947	951	954	rBV4	241347	279374	14.38%	0.928%
24	7.622	954	958	959	rBV4	62887	77325	3.98%	0.257%
25	7.645	959	962	965	rVB2	266436	222728	11.47%	0.740%
26	7.675	965	967	970	rVB2	61290	65105	3.35%	0.216%
27	7.710	970	973	977	rBV2	108035	131708	6.78%	0.438%
28	7.787	983	986	988	rBV3	175594	198414	10.21%	0.659%
29	7.839	991	995	997	rBV	1074310	1089104	56.07%	3.618%
30	7.857	997	998	1006	rVB	1037265	889610	45.80%	2.955%
31	7.922	1006	1009	1015	rVB2	218168	212875	10.96%	0.707%
32	7.975	1015	1018	1020	rVB3	65892	76641	3.95%	0.255%
33	8.016	1020	1025	1027	rBV4	120798	168711	8.69%	0.560%
34	8.086	1034	1037	1039	rBV	168273	139173	7.16%	0.462%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072117\
 Data File : BF096967.D
 Acq On : 22 Jul 2017 3:43
 Operator : SJ/JU
 Sample : I4253-01DL 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-O-P-6-7-BASEDL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	8.122	1040	1043	1045	rBV3	51631	56727	2.92%	0.188%
36	8.204	1054	1057	1059	rBV2	202748	205470	10.58%	0.683%
37	8.228	1059	1061	1067	rVB2	165698	204479	10.53%	0.679%
38	8.281	1067	1070	1073	rBV2	362415	392950	20.23%	1.305%
39	8.310	1073	1075	1077	rVB	219097	152634	7.86%	0.507%
40	8.345	1079	1081	1085	rVB2	98925	123394	6.35%	0.410%
41	8.404	1089	1091	1093	rBV	223330	165026	8.50%	0.548%
42	8.451	1096	1099	1101	rBV2	316523	248551	12.80%	0.826%
43	8.551	1111	1116	1119	rVB	2102299	1942455	100.00%	6.453%
44	8.586	1119	1122	1124	rBV3	49665	61469	3.16%	0.204%
45	8.651	1129	1133	1137	rVB	1492698	1370659	70.56%	4.554%
46	8.728	1144	1146	1148	rBV2	82065	80434	4.14%	0.267%
47	8.751	1148	1150	1153	rVV3	145792	171734	8.84%	0.571%
48	8.781	1153	1155	1158	rVB3	89073	106104	5.46%	0.353%
49	8.816	1158	1161	1165	rVB4	73987	111060	5.72%	0.369%
50	8.857	1165	1168	1169	rBV3	69885	73126	3.76%	0.243%
51	8.881	1169	1172	1174	rVB	226813	185252	9.54%	0.615%
52	8.910	1174	1177	1180	rVB	296207	244056	12.56%	0.811%
53	8.969	1185	1187	1190	rBV2	117286	83633	4.31%	0.278%
54	9.010	1191	1194	1200	rVV	540376	505639	26.03%	1.680%
55	9.057	1200	1202	1205	rVV2	90837	94293	4.85%	0.313%
56	9.104	1206	1210	1217	rVB	407340	643968	33.15%	2.139%
57	9.175	1217	1222	1226	rBV	673584	991944	51.07%	3.295%
58	9.251	1229	1235	1237	rBV	901075	1026467	52.84%	3.410%
59	9.275	1237	1239	1242	rVV	648757	561562	28.91%	1.866%
60	9.298	1242	1243	1246	rVV2	204819	206246	10.62%	0.685%
61	9.328	1246	1248	1251	rVV	373155	344391	17.73%	1.144%
62	9.363	1251	1254	1261	rVB2	370130	485291	24.98%	1.612%
63	9.445	1265	1268	1273	rVB	216701	209390	10.78%	0.696%
64	9.498	1275	1277	1281	rVB3	154320	159964	8.24%	0.531%
65	9.539	1281	1284	1286	rBV	365770	297937	15.34%	0.990%
66	9.586	1286	1292	1294	rBV3	803752	954585	49.14%	3.171%
67	9.616	1294	1297	1299	rVV2	183002	202169	10.41%	0.672%
68	9.692	1307	1310	1315	rVB	266491	335412	17.27%	1.114%
69	9.733	1315	1317	1320	rBV2	80522	86156	4.44%	0.286%
70	9.792	1323	1327	1330	rVB2	282645	331147	17.05%	1.100%
71	9.828	1330	1333	1336	rBV	264896	228429	11.76%	0.759%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072117\
 Data File : BF096967.D
 Acq On : 22 Jul 2017 3:43
 Operator : SJ/JU
 Sample : I4253-01DL 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-O-P-6-7-BASEDL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	9.863	1336	1339	1343	rVB2	157995	156608	8.06%	0.520%
73	9.904	1343	1346	1348	rBV2	167338	153471	7.90%	0.510%
74	9.933	1348	1351	1353	rVB	164823	134378	6.92%	0.446%
75	9.992	1357	1361	1363	rBV2	141235	225956	11.63%	0.751%
76	10.010	1363	1364	1366	rVV2	146763	76836	3.96%	0.255%
77	10.033	1366	1368	1371	rVB	250387	202886	10.44%	0.674%
78	10.098	1372	1379	1381	rBV5	132649	202463	10.42%	0.673%
79	10.128	1381	1384	1386	rVB2	140107	111079	5.72%	0.369%
80	10.151	1386	1388	1391	rBV2	63019	67981	3.50%	0.226%
81	10.257	1402	1406	1408	rBV2	289223	306952	15.80%	1.020%
82	10.369	1421	1425	1429	rVB4	178392	217077	11.18%	0.721%
83	10.416	1429	1433	1434	rBV3	62709	84265	4.34%	0.280%
84	10.486	1442	1445	1446	rBV	309058	252175	12.98%	0.838%
85	10.504	1446	1448	1449	rVV2	358718	310489	15.98%	1.032%
86	10.522	1449	1451	1457	rVB	494472	462067	23.79%	1.535%
87	10.704	1479	1482	1484	rBV3	91246	92735	4.77%	0.308%
88	10.951	1521	1524	1527	rVV2	228222	220440	11.35%	0.732%
89	10.980	1527	1529	1535	rVB	245395	245644	12.65%	0.816%
90	11.057	1539	1542	1544	rVV	719818	604972	31.14%	2.010%
91	11.080	1544	1546	1550	rVV	303167	253266	13.04%	0.841%
92	11.133	1552	1555	1559	rVB	84915	90187	4.64%	0.300%
93	11.375	1594	1596	1601	rVB2	108533	105854	5.45%	0.352%
94	11.780	1663	1665	1668	rBV	76037	58726	3.02%	0.195%
95	12.004	1700	1703	1706	rVB	283916	237579	12.23%	0.789%
96	12.263	1744	1747	1753	rBV	146803	129622	6.67%	0.431%
97	12.486	1781	1785	1788	rVB	127028	121868	6.27%	0.405%
98	12.639	1808	1811	1819	rVB	212542	212791	10.95%	0.707%
99	13.680	1984	1988	1991	rBV	681065	699701	36.02%	2.325%
100	15.045	2216	2220	2225	rBV	487699	590765	30.41%	1.963%


Sum of corrected areas: 30100416

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072117\
Data File : BF096967.D
Acq On : 22 Jul 2017 3:43
Operator : SJ/JU
Sample : I4253-01DL 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-O-P-6-7-BASEDL

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

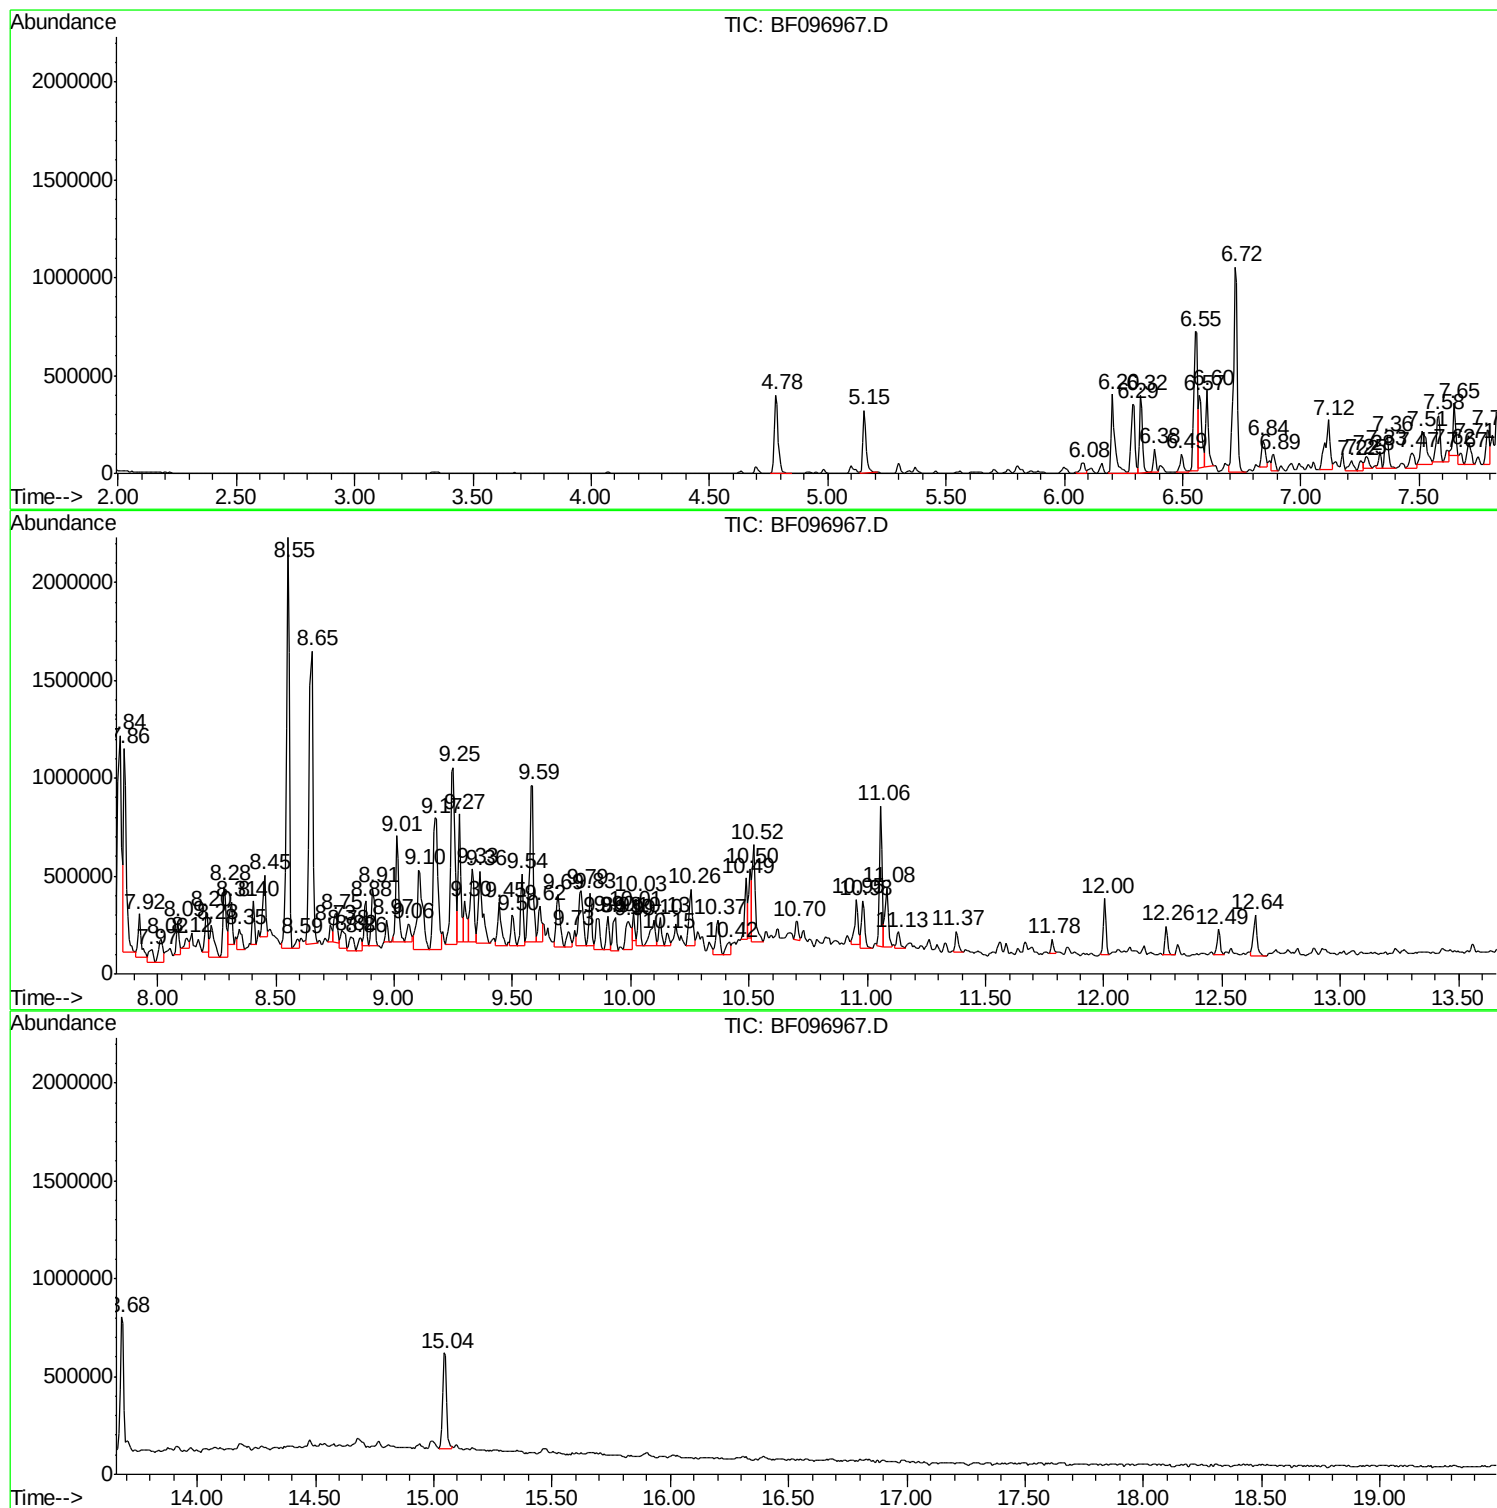

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF072117\
Data_File : BF096967.D
Acq_On : 22-Jul-2017 3:433
Operator : SJ/JUU
Sample : I4253-01DL_10XX
Misc :
ALS_Vial : 30 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
E2-O-P-6-7-BASEDL

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
